

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042023\
Data File : FF012514.D
Signal(s) : FID2B.ch
Acq On : 20 Apr 2023 09:34
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 21 00:54:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.005	2144409	17.840 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.896	63755	0.505 ug/ml
15) N-TETRATRIACONTANE	19.676	45043	0.397 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042023\
Data File : FF012514.D
Signal(s) : FID2B.ch
Acq On : 20 Apr 2023 09:34
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 21 00:54:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

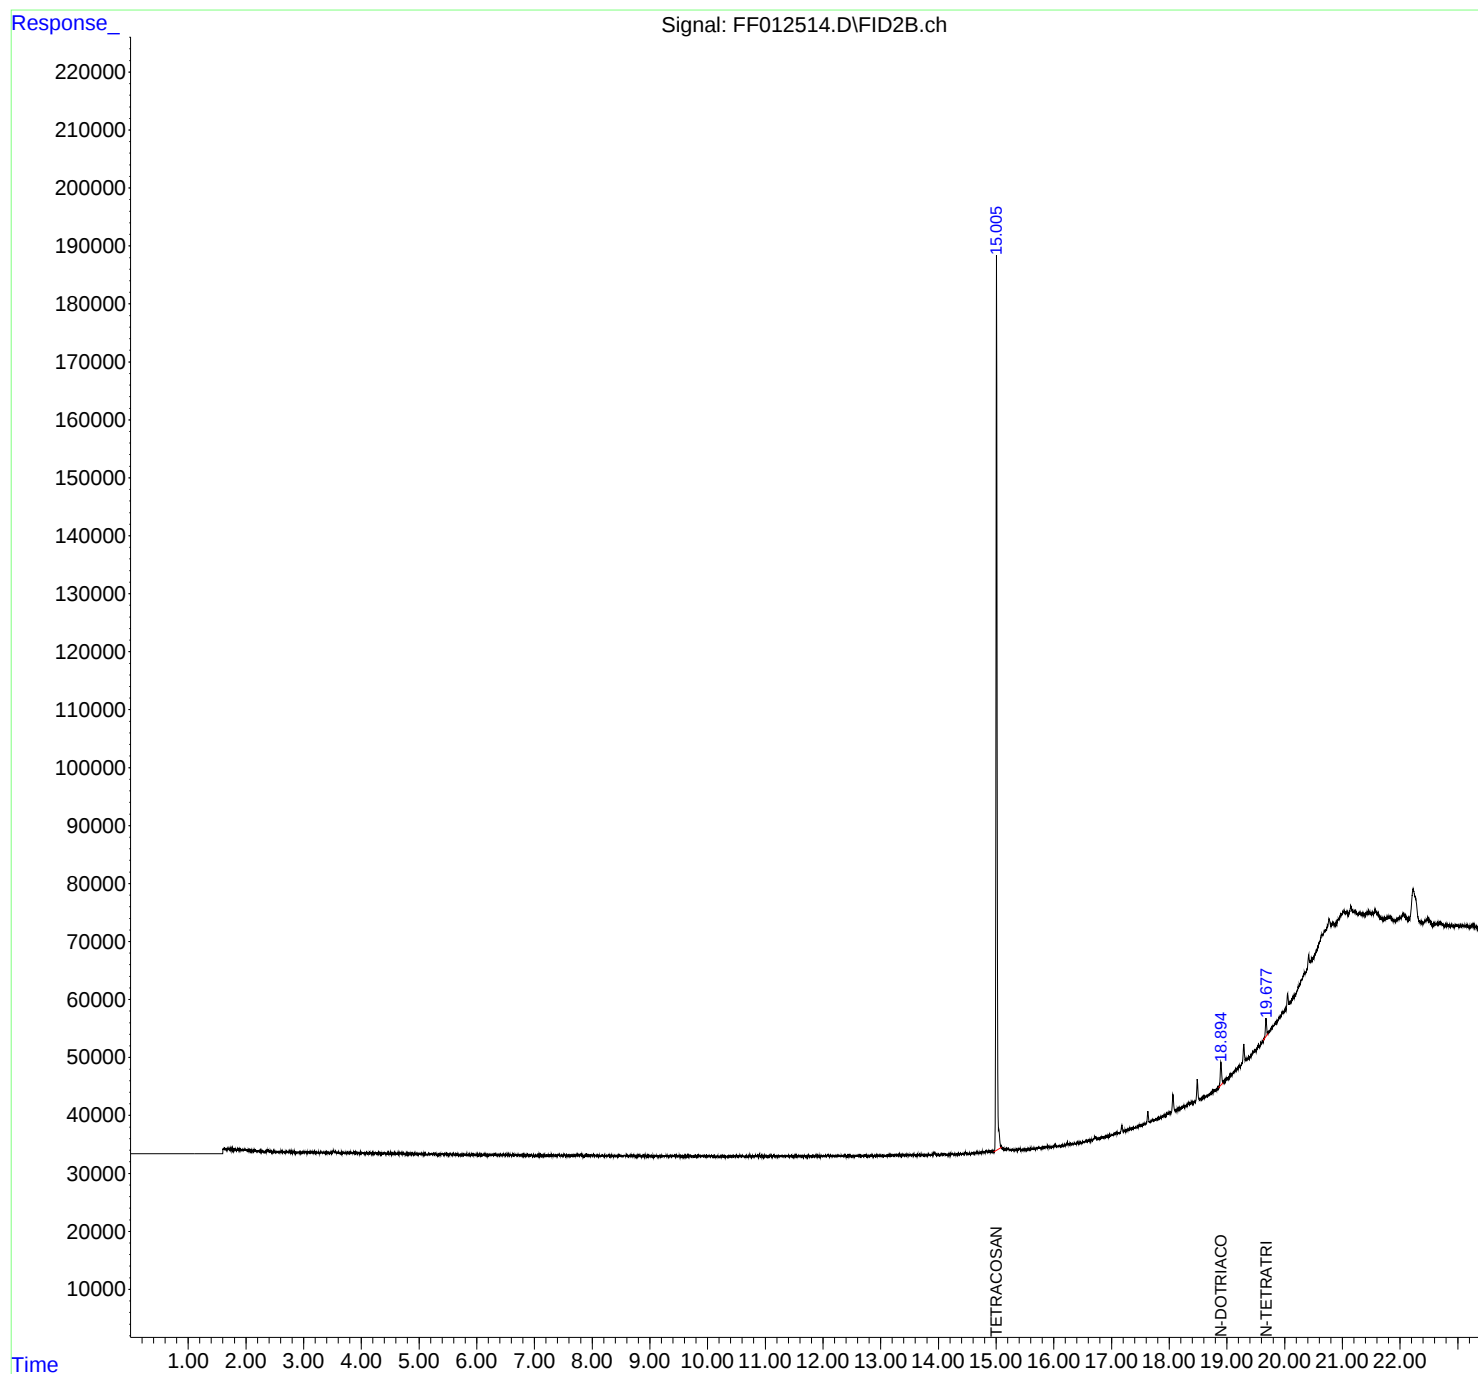


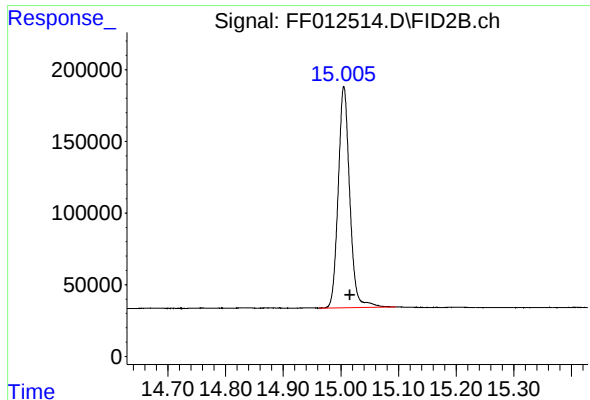

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.005 min
Delta R.T.: -0.011 min
Response: 2144409
Conc: 17.84 ug/ml

Instrument :
FID_F
ClientSampleId :

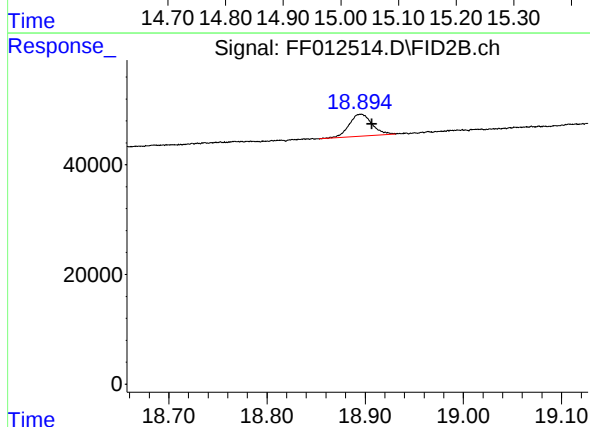

#14 N-DOTRIACONTANE

R.T.: 18.896 min
Delta R.T.: -0.011 min
Response: 63755
Conc: 0.51 ug/ml

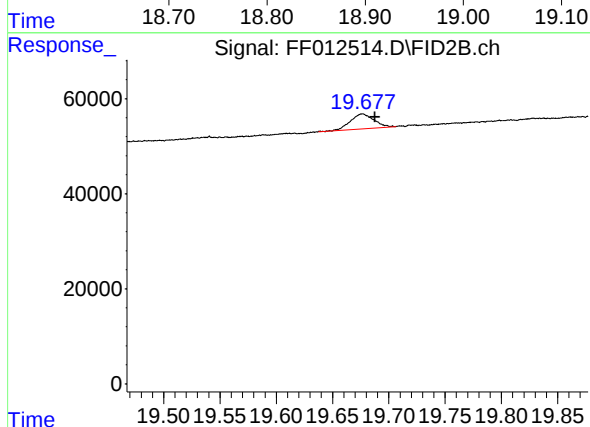

#15 N-TETRATRIACONTANE

R.T.: 19.676 min
Delta R.T.: -0.011 min
Response: 45043
Conc: 0.40 ug/ml