

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042023\
 Data File : FF012516.D
 Signal(s) : FID2B.ch
 Acq On : 20 Apr 2023 10:32
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 21 00:54:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
 Quant Title :
 QLast Update : Thu Apr 13 15:26:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.737	2030766	16.442 ug/ml
12) N-OCTACOSANE	17.178	2105598	15.965 ug/ml
13) N-TRIACONTANE	18.062	138920	1.065 ug/ml
14) N-DOTRIACONTANE	18.894	187573	1.487 ug/ml
15) N-TETRATRIACONTANE	19.676	142325	1.255 ug/ml
16) N-HEXATRIACONTANE	20.417	109978	1.077 ug/ml
17) N-OCTATRIACONTANE	21.150	288409	2.960 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042023\
Data File : FF012516.D
Signal(s) : FID2B.ch
Acq On : 20 Apr 2023 10:32
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 21 00:54:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

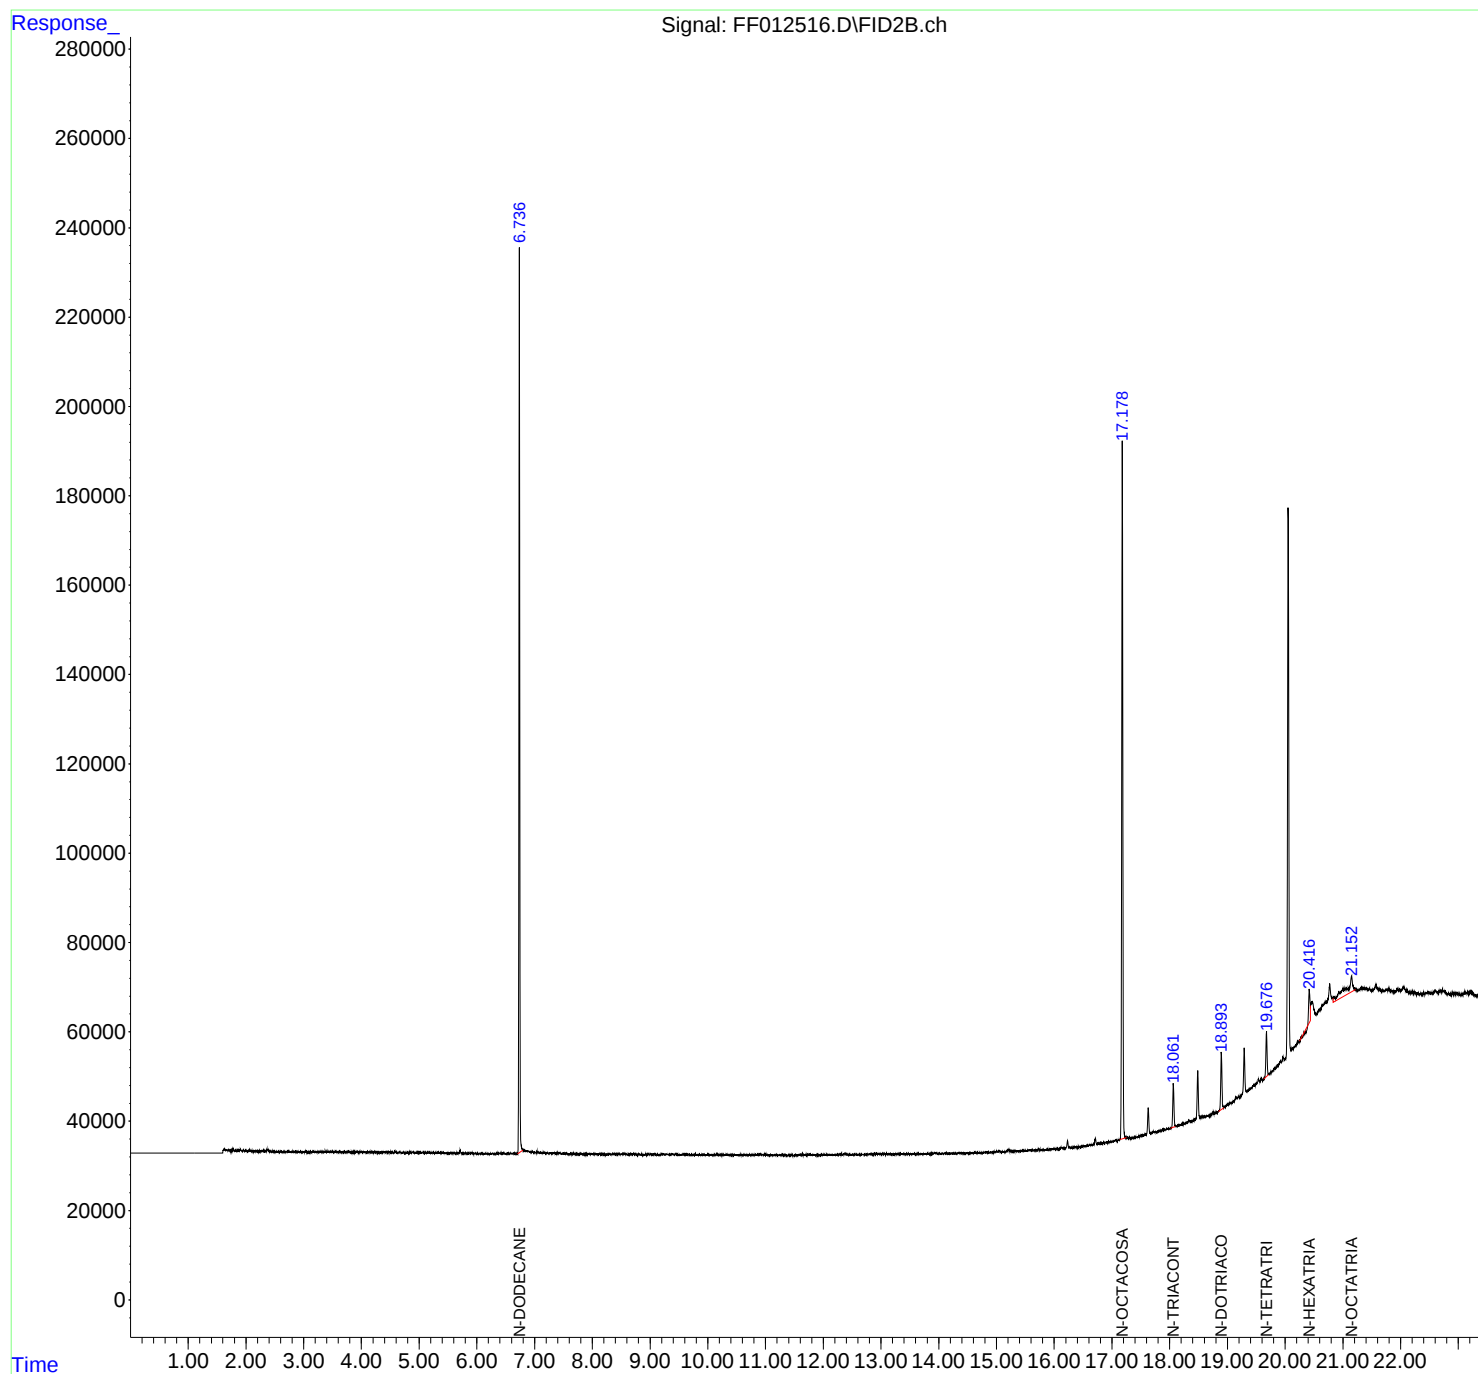

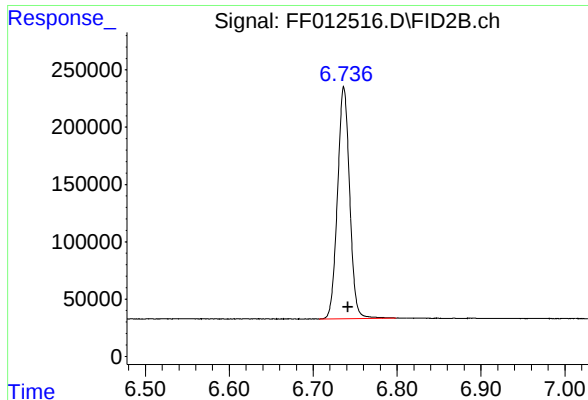


#3 N-DODECANE

R.T.: 6.737 min
Delta R.T.: -0.005 min
Response: 2030766
Conc: 16.44 ug/ml

Instrument :


FID_F

ClientSampleId :

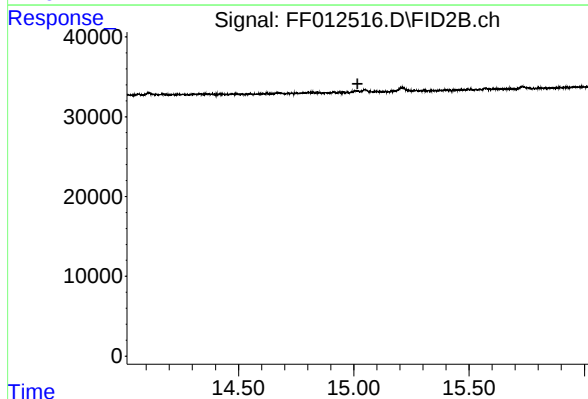


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.016 min
Response: 0
Conc: N.D.

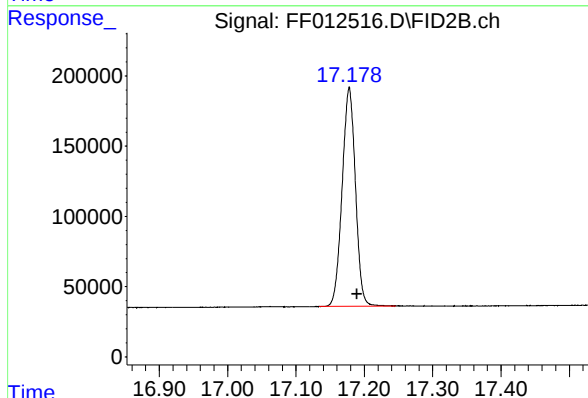


#12 N-OCTACOSANE

R.T.: 17.178 min
Delta R.T.: -0.011 min
Response: 2105598
Conc: 15.97 ug/ml

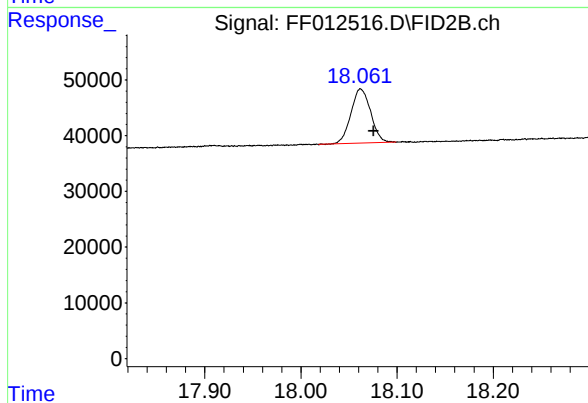

#13 N-TRIACONTANE


R.T.: 18.062 min
Delta R.T.: -0.013 min
Response: 138920
Conc: 1.06 ug/ml

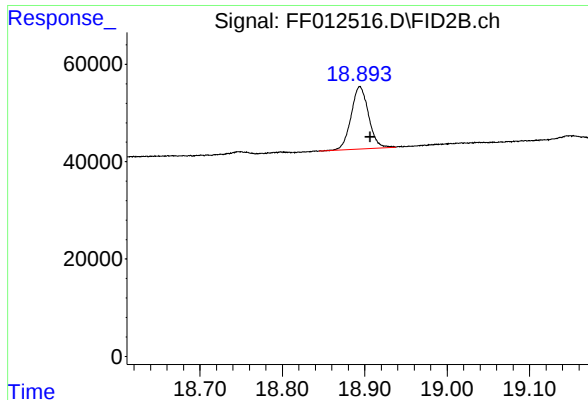

#14 N-DOTRIACONTANE


R.T.: 18.894 min
Delta R.T.: -0.013 min
Response: 187573
Conc: 1.49 ug/ml

Instrument :
FID_F
ClientSampleId :

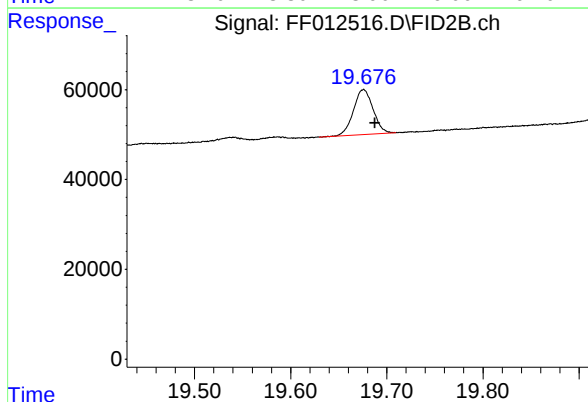


#15 N-TETRATRIACONTANE

R.T.: 19.676 min
Delta R.T.: -0.012 min
Response: 142325
Conc: 1.26 ug/ml

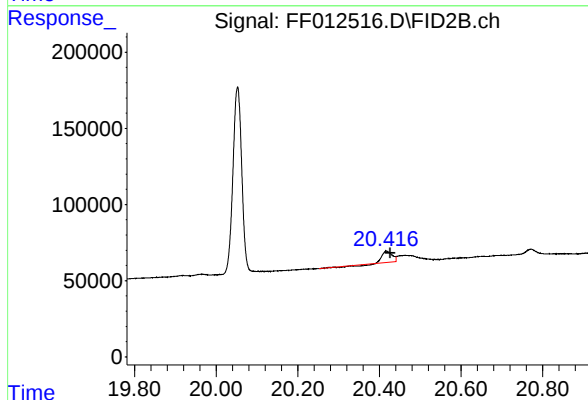

#16 N-HEXATRIACONTANE

R.T.: 20.417 min
Delta R.T.: -0.010 min
Response: 109978
Conc: 1.08 ug/ml

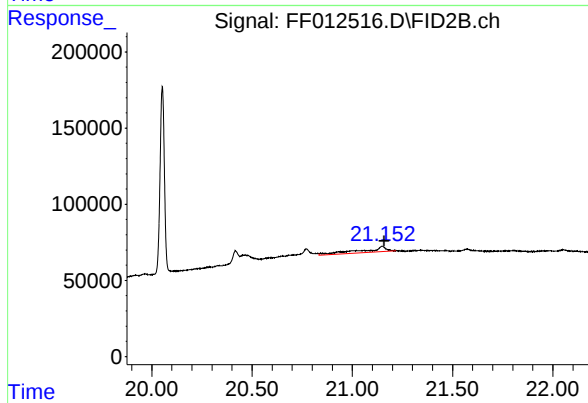

#17 N-OCTATRIACONTANE

R.T.: 21.150 min
Delta R.T.: -0.010 min
Response: 288409
Conc: 2.96 ug/ml