

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042023\
 Data File : FF012519.D
 Signal(s) : FID2B.ch
 Acq On : 20 Apr 2023 14:27
 Operator : YP\AJ
 Sample : 02406-02
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 21 00:54:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
 Quant Title :
 QLast Update : Thu Apr 13 15:26:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.006	1553218	12.922 ug/ml
Target Compounds			
7) N-EICOSANE	12.983f	270352	1.963 ug/ml
10) N-TETRACOSANE	15.204	158505	1.172 ug/ml
11) N-HEXACOSANE	16.229	43922	0.330 ug/ml
12) N-OCTACOSANE	17.177	35153	0.267 ug/ml
13) N-TRIACONTANE	18.063	67919	0.521 ug/ml
14) N-DOTRIACONTANE	18.884	238589	1.891 ug/ml
15) N-TETRATRIACONTANE	19.677	74234	0.655 ug/ml
16) N-HEXATRIACONTANE	20.418	181944	1.782 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042023\
Data File : FF012519.D
Signal(s) : FID2B.ch
Acq On : 20 Apr 2023 14:27
Operator : YP\AJ
Sample : 02406-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 21 00:54:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

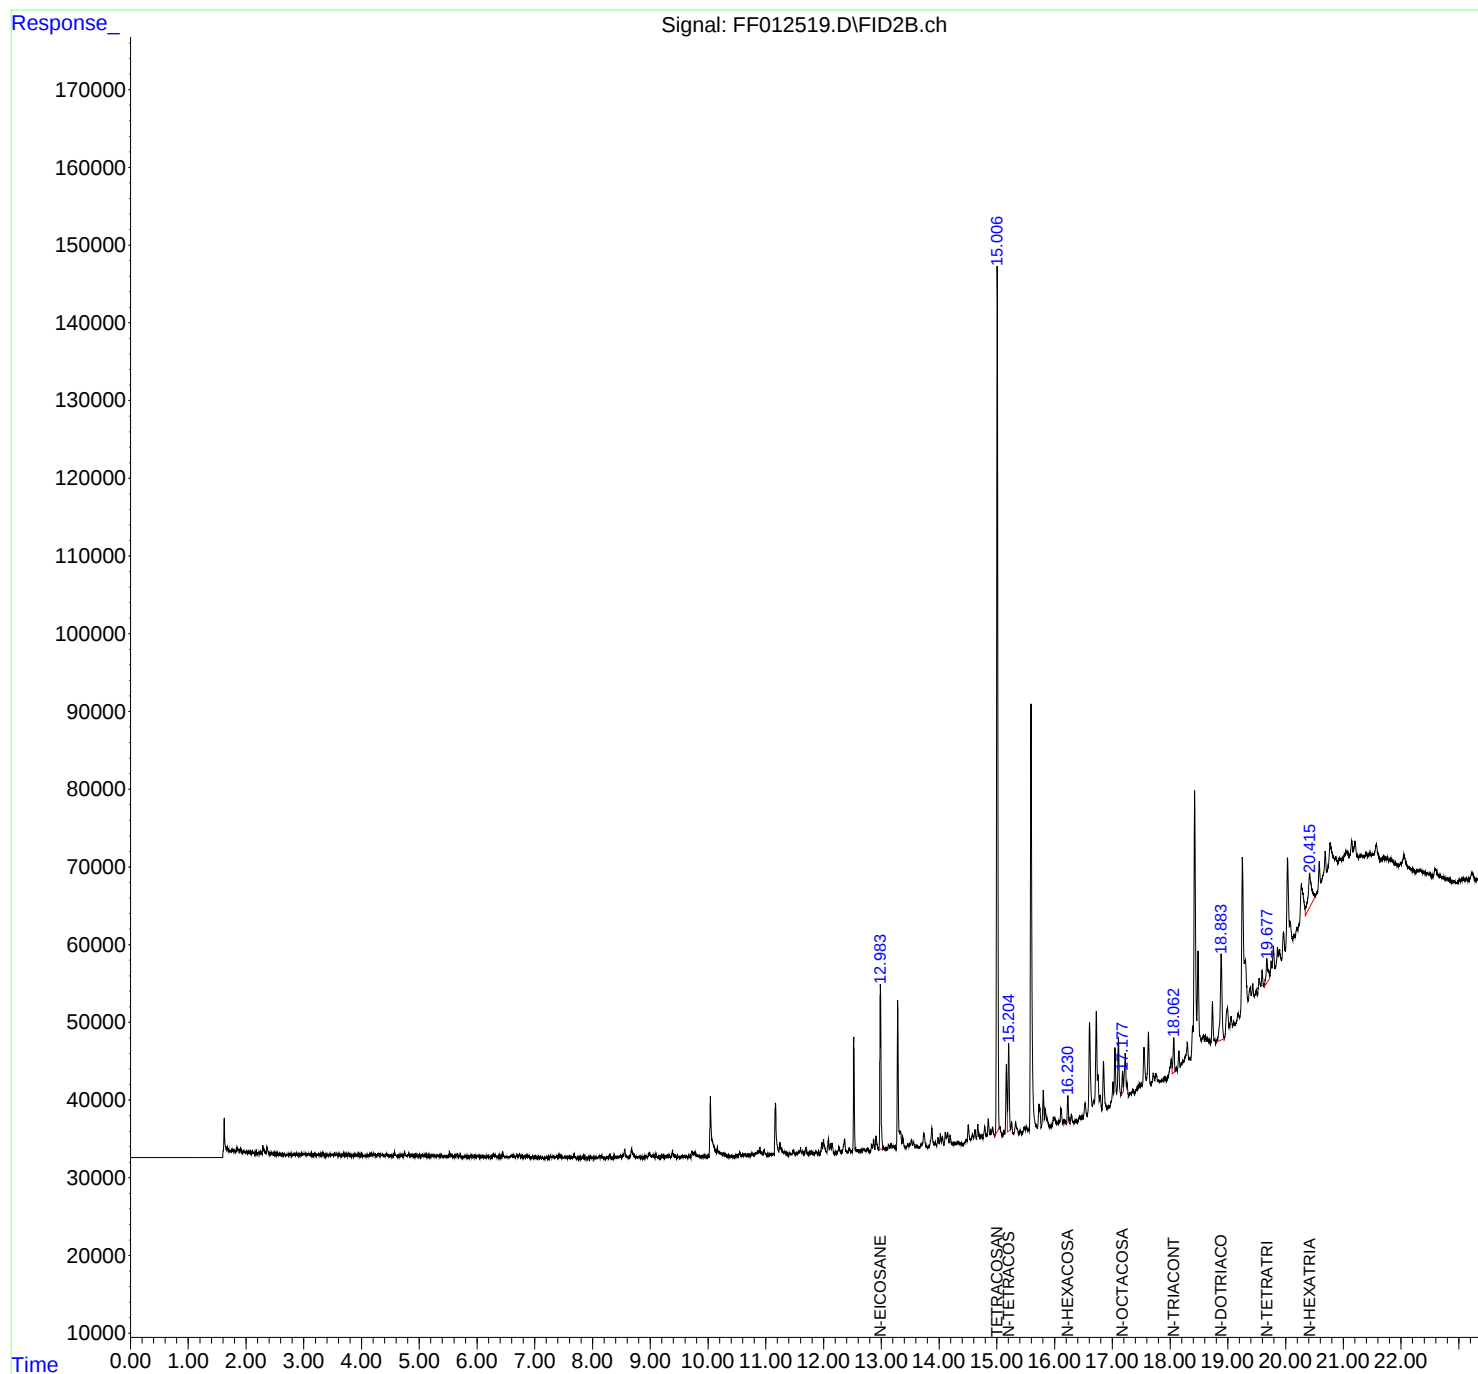


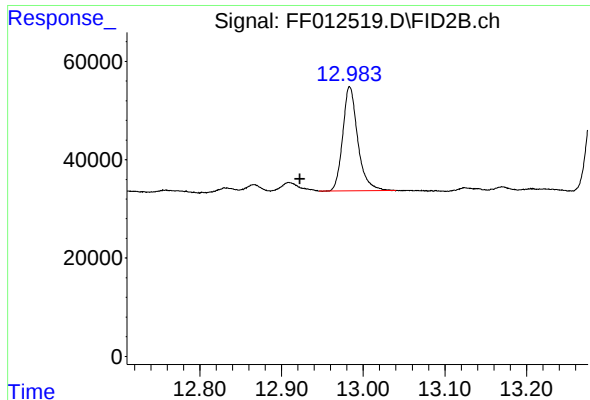

#7 N-EICOSANE


R.T.: 12.983 min
Delta R.T.: 0.061 min
Response: 270352
Conc: 1.96 ug/ml

Instrument :
FID_F
ClientSampleId :

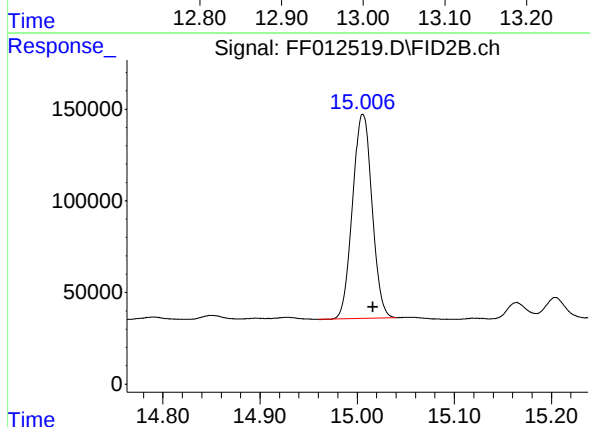


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.006 min
Delta R.T.: -0.010 min
Response: 1553218
Conc: 12.92 ug/ml

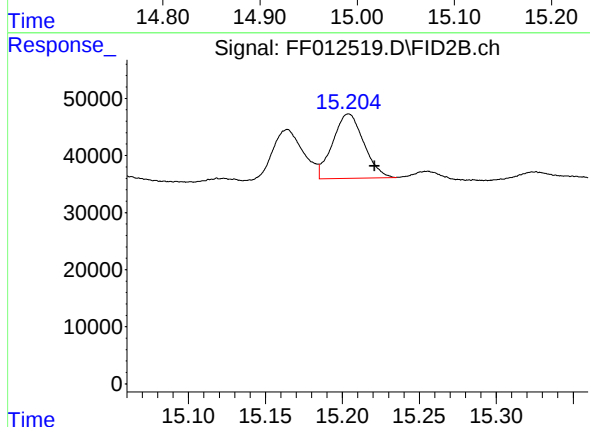


#10 N-TETRACOSANE

R.T.: 15.204 min
Delta R.T.: -0.017 min
Response: 158505
Conc: 1.17 ug/ml

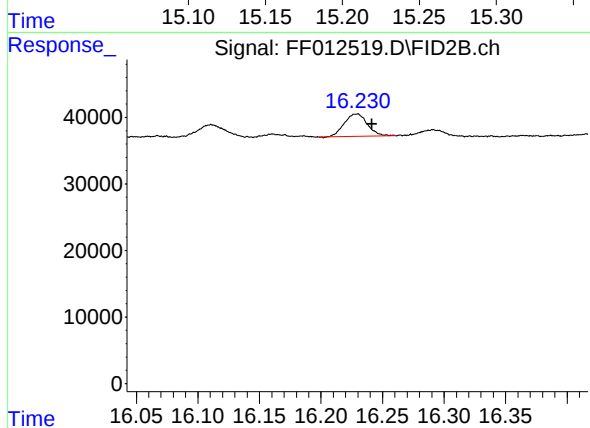

#11 N-HEXACOSANE


R.T.: 16.229 min
Delta R.T.: -0.012 min
Response: 43922
Conc: 0.33 ug/ml

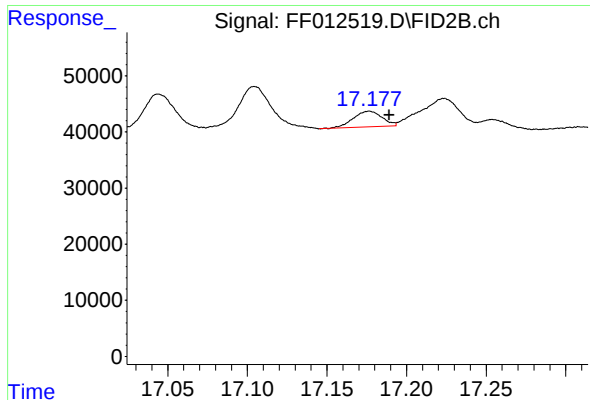

#12 N-OCTACOSANE


R.T.: 17.177 min
Delta R.T.: -0.013 min
Response: 35153
Conc: 0.27 ug/ml

Instrument :
FID_F
ClientSampleId :

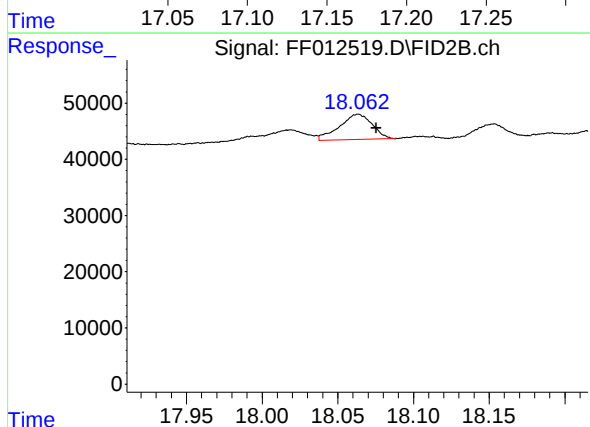


#13 N-TRIACONTANE

R.T.: 18.063 min
Delta R.T.: -0.012 min
Response: 67919
Conc: 0.52 ug/ml

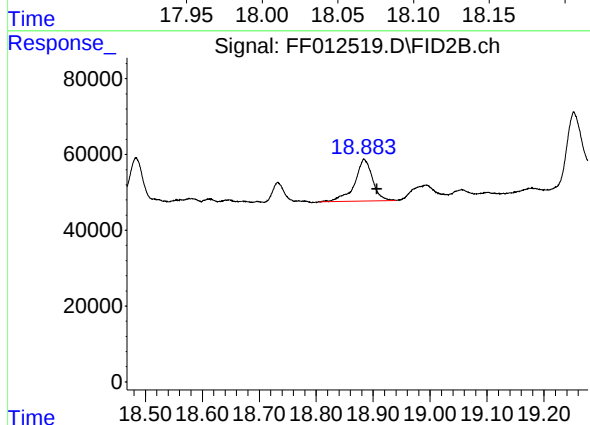


#14 N-DOTRIACONTANE

R.T.: 18.884 min
Delta R.T.: -0.023 min
Response: 238589
Conc: 1.89 ug/ml

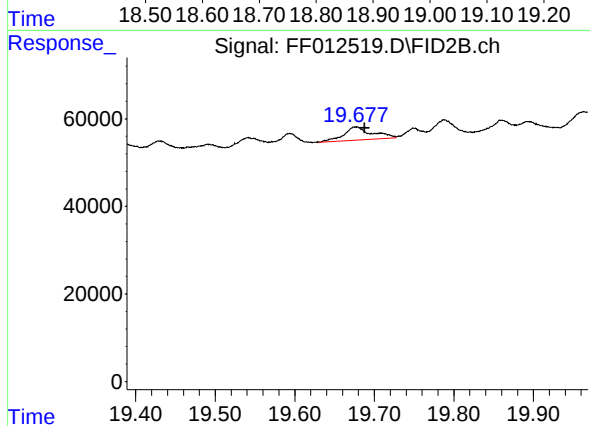

#15 N-TETRATRIACONTANE

R.T.: 19.677 min
Delta R.T.: -0.011 min
Response: 74234
Conc: 0.65 ug/ml

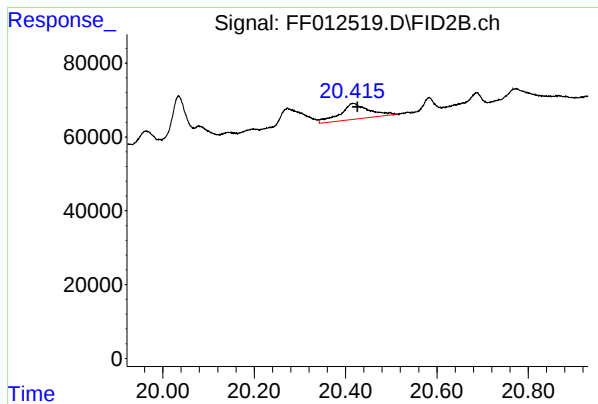

#16 N-HEXATRIACONTANE

R.T.: 20.418 min
Delta R.T.: -0.009 min
Response: 181944
Conc: 1.78 ug/ml

Instrument :
FID_F
ClientSampleId :