

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042023\
Data File : FF012517.D
Signal(s) : FID2B.ch
Acq On : 20 Apr 2023 13:29
Operator : YP\AJ
Sample : PB152237BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB152237BL

Integration File: autoint1.e
Quant Time: Apr 21 00:54:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.004	1580076	13.145 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042023\
Data File : FF012517.D
Signal(s) : FID2B.ch
Acq On : 20 Apr 2023 13:29
Operator : YP\AJ
Sample : PB152237BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB152237BL

Integration File: autoint1.e
Quant Time: Apr 21 00:54:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

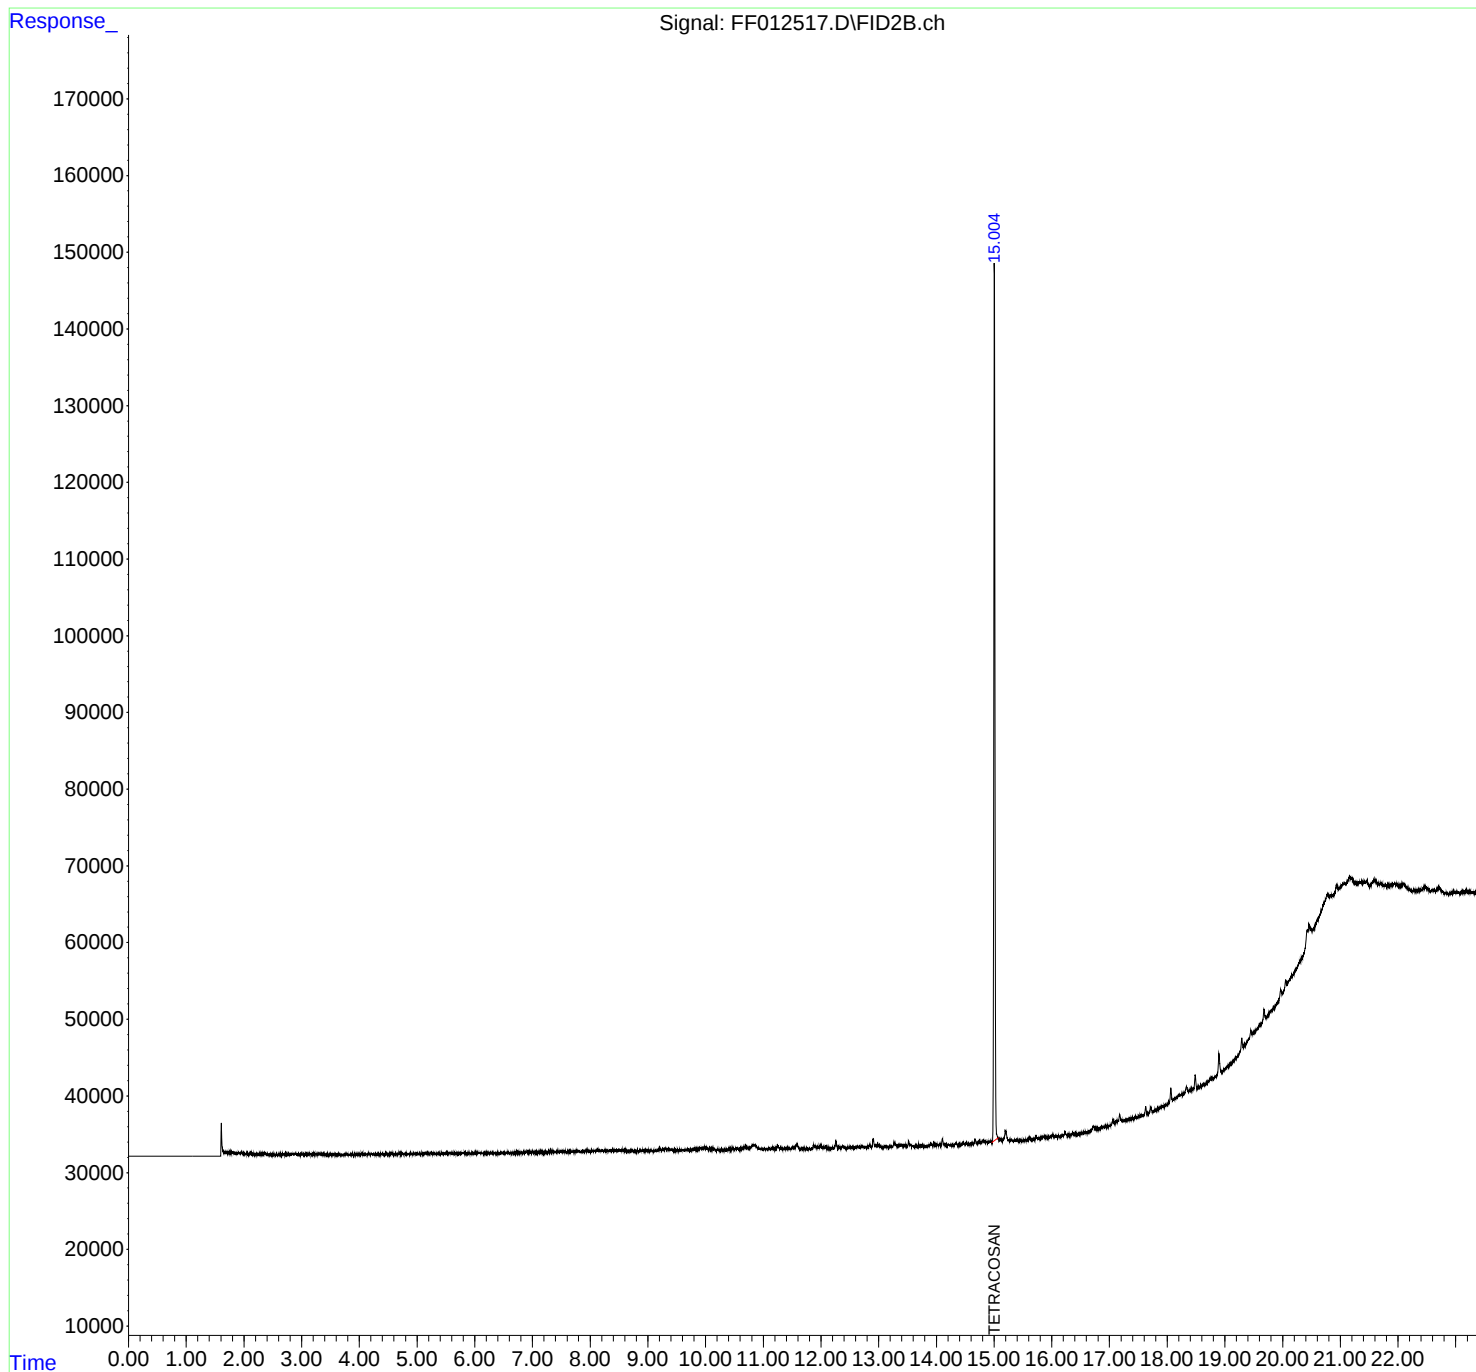

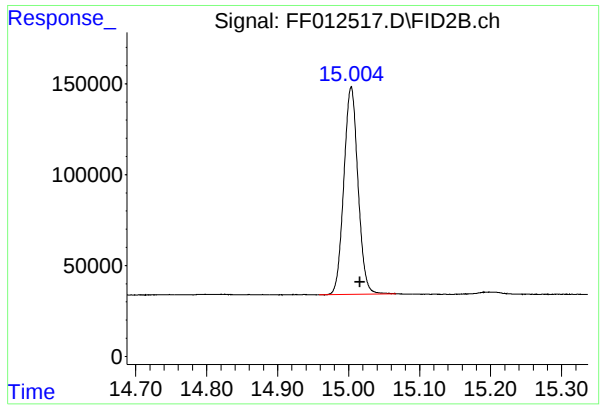

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.004 min
Delta R.T.: -0.012 min
Response: 1580076
Conc: 13.14 ug/ml

Instrument :
FID_F
ClientSampleId :
PB152237BL