

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
 Data File : FF008291.D
 Signal(s) : FID2B.ch
 Acq On : 21 Apr 2021 15:58
 Operator : DD\AJ
 Sample : M2097-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 22 03:40:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
 Quant Title :
 QLast Update : Tue Apr 06 02:37:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.774	2120131	19.320 ug/ml
Target Compounds			
4) N-TETRADECANE	8.331	72661	0.560 ug/ml
7) N-EICOSANE	12.748f	197174	1.549 ug/ml
10) N-TETRACOSANE	14.968	226455	1.817 ug/ml
11) N-HEXACOSANE	15.996	128370	1.049 ug/ml
12) N-OCTACOSANE	16.944	202686	1.660 ug/ml
13) N-TRIACONTANE	17.829	222516	1.821 ug/ml
14) N-DOTRIACONTANE	18.654	473417	3.904 ug/ml
15) N-TETRATRIACONTANE	19.520f	454374	4.017 ug/ml
16) N-HEXATRIACONTANE	20.131f	127176	1.236 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
Data File : FF008291.D
Signal(s) : FID2B.ch
Acq On : 21 Apr 2021 15:58
Operator : DD\AJ
Sample : M2097-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 22 03:40:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
Quant Title :
QLast Update : Tue Apr 06 02:37:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

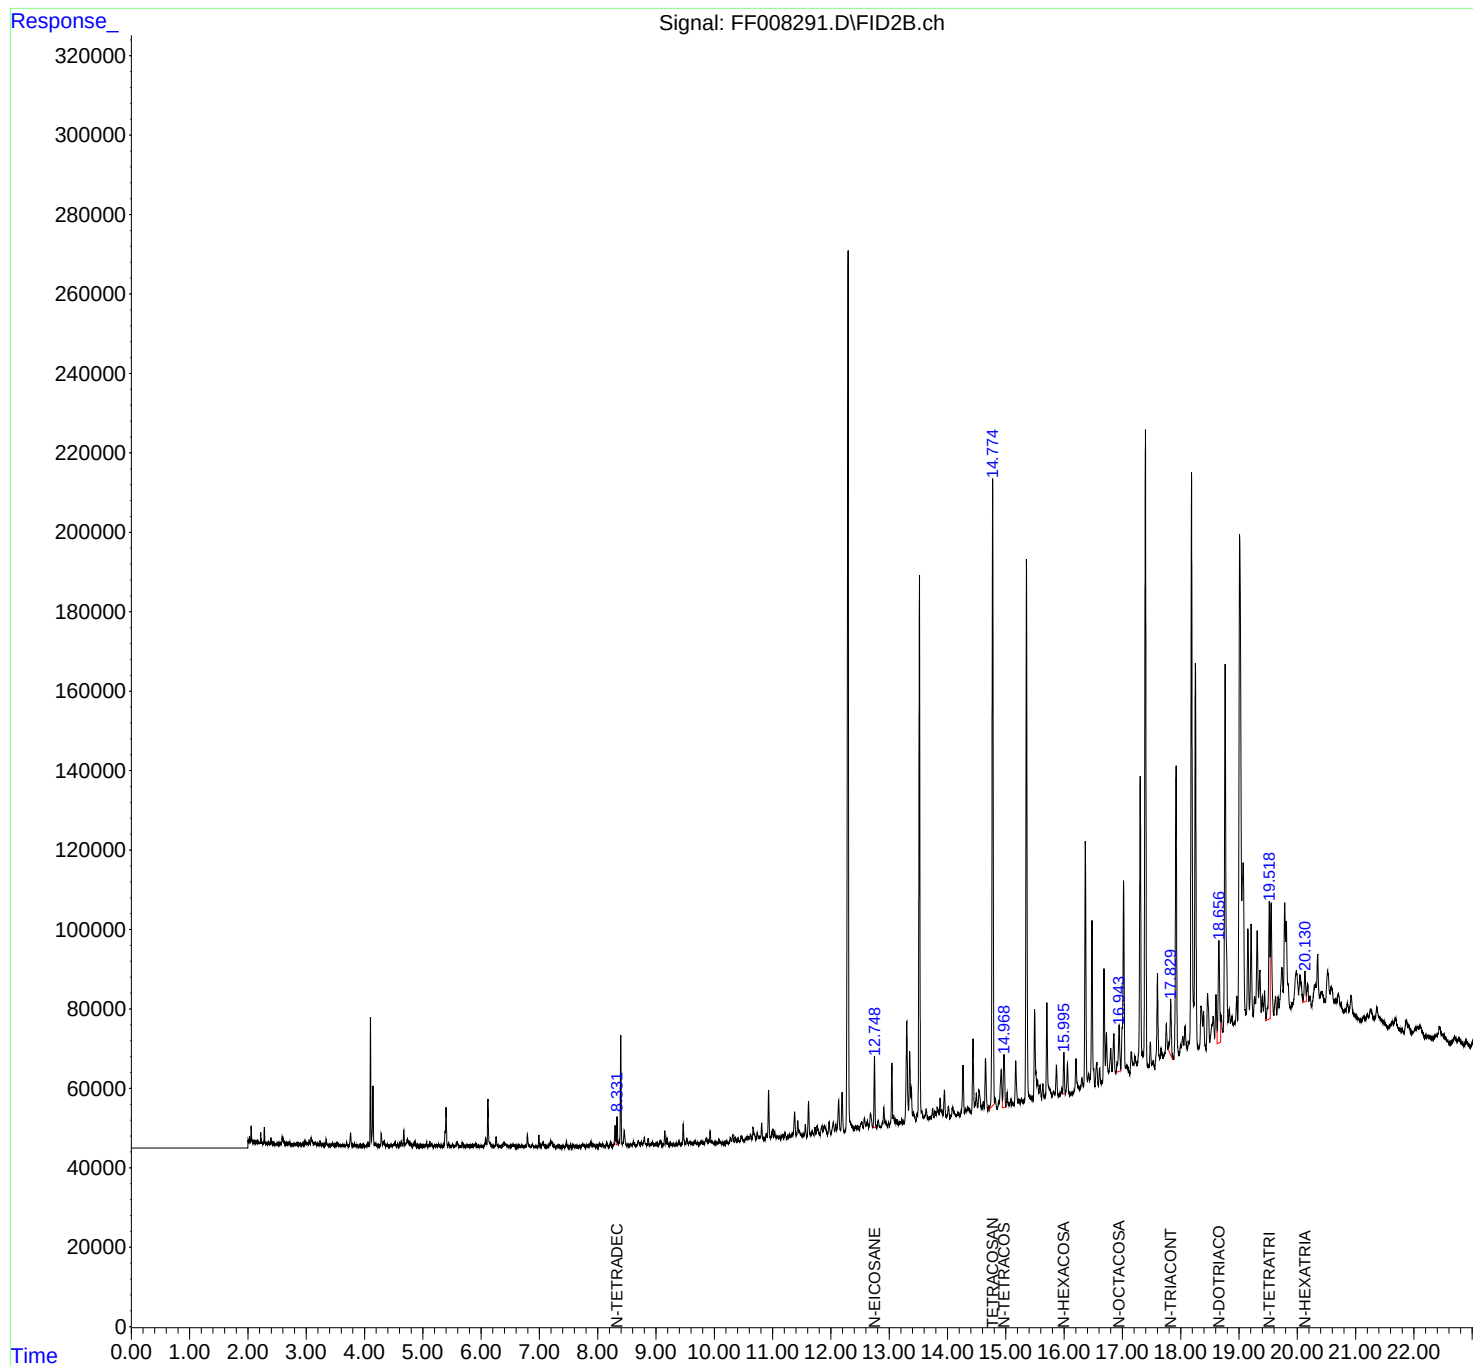


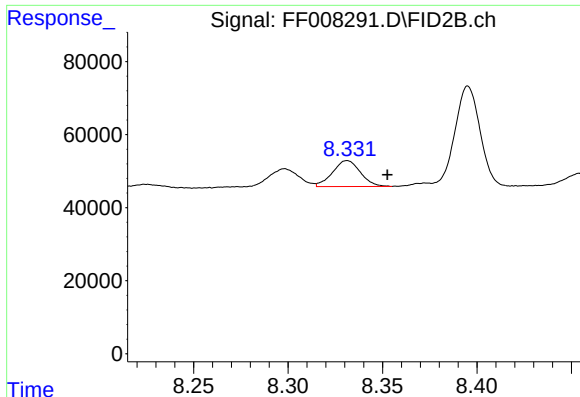

#4 N-TETRADECANE


R.T.: 8.331 min
Delta R.T.: -0.021 min
Response: 72661
Conc: 0.56 ug/ml

Instrument :
FID_F
ClientSampleId :

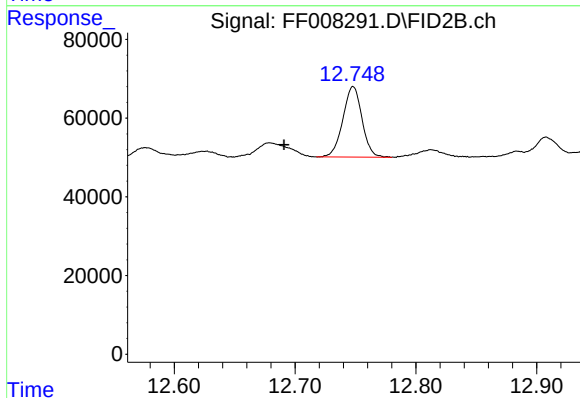


#7 N-EICOSANE

R.T.: 12.748 min
Delta R.T.: 0.057 min
Response: 197174
Conc: 1.55 ug/ml

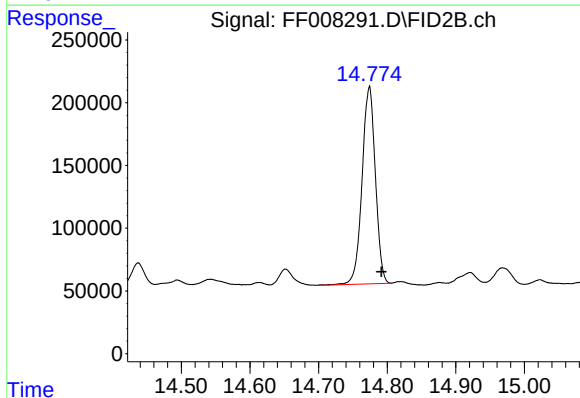


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.774 min
Delta R.T.: -0.018 min
Response: 2120131
Conc: 19.32 ug/ml

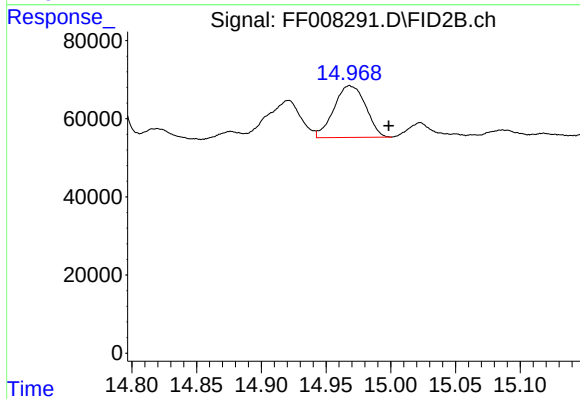

#10 N-TETRACOSANE


R.T.: 14.968 min
Delta R.T.: -0.030 min
Response: 226455
Conc: 1.82 ug/ml

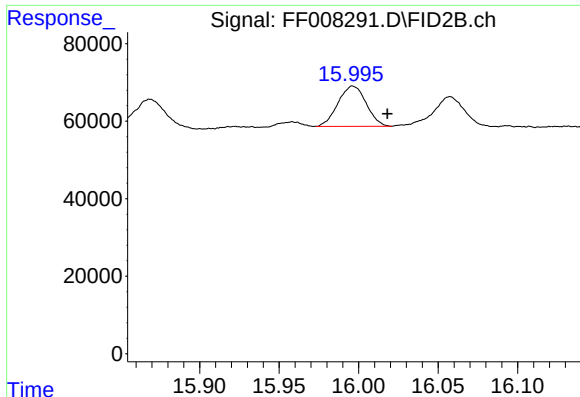

#11 N-HEXACOSANE


R.T.: 15.996 min
Delta R.T.: -0.022 min
Response: 128370
Conc: 1.05 ug/ml

Instrument :
FID_F
ClientSampleId :

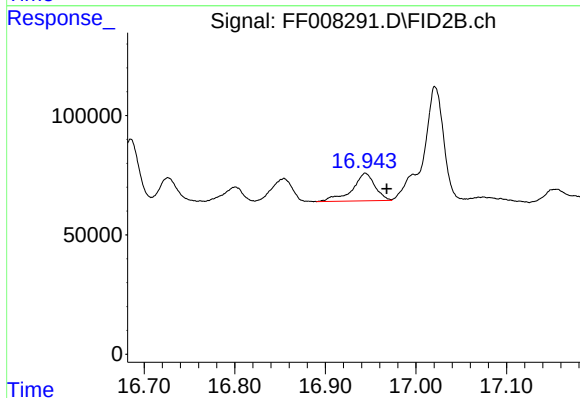


#12 N-OCTACOSANE

R.T.: 16.944 min
Delta R.T.: -0.024 min
Response: 202686
Conc: 1.66 ug/ml

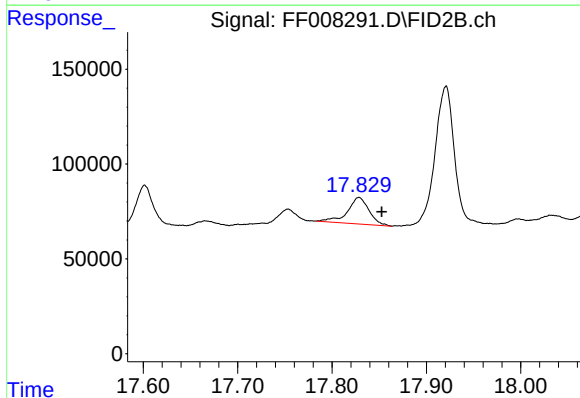


#13 N-TRIACONTANE

R.T.: 17.829 min
Delta R.T.: -0.024 min
Response: 222516
Conc: 1.82 ug/ml

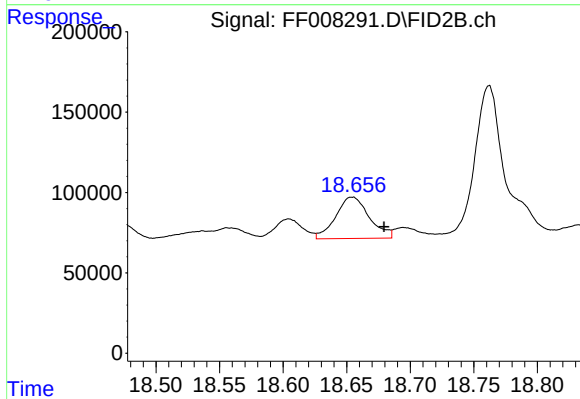

#14 N-DOTRIACONTANE


R.T.: 18.654 min
Delta R.T.: -0.025 min
Response: 473417
Conc: 3.90 ug/ml

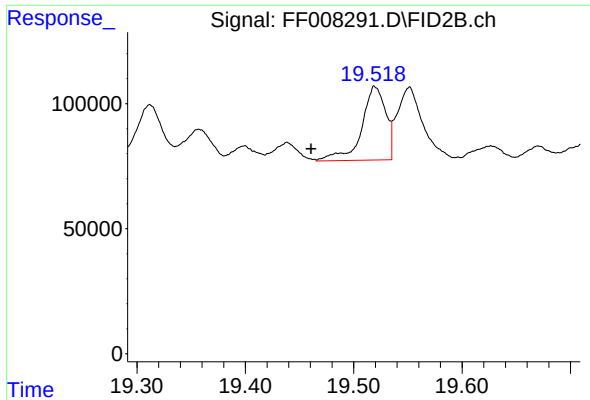

#15 N-TETRATRIACONTANE

R.T.: 19.520 min
Delta R.T.: 0.059 min
Response: 454374
Conc: 4.02 ug/ml

Instrument :
FID_F
ClientSampleId :

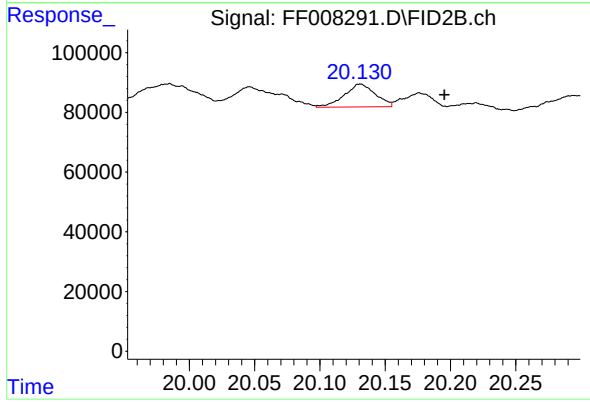

#16 N-HEXATRIACONTANE

R.T.: 20.131 min
Delta R.T.: -0.064 min
Response: 127176
Conc: 1.24 ug/ml