

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
Data File : FF008297.D
Signal(s) : FID2B.ch
Acq On : 21 Apr 2021 19:38
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 22 03:41:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
Quant Title :
QLast Update : Tue Apr 06 02:37:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.775	2148010	19.574 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.658	99189	0.818 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
Data File : FF008297.D
Signal(s) : FID2B.ch
Acq On : 21 Apr 2021 19:38
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 22 03:41:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
Quant Title :
QLast Update : Tue Apr 06 02:37:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

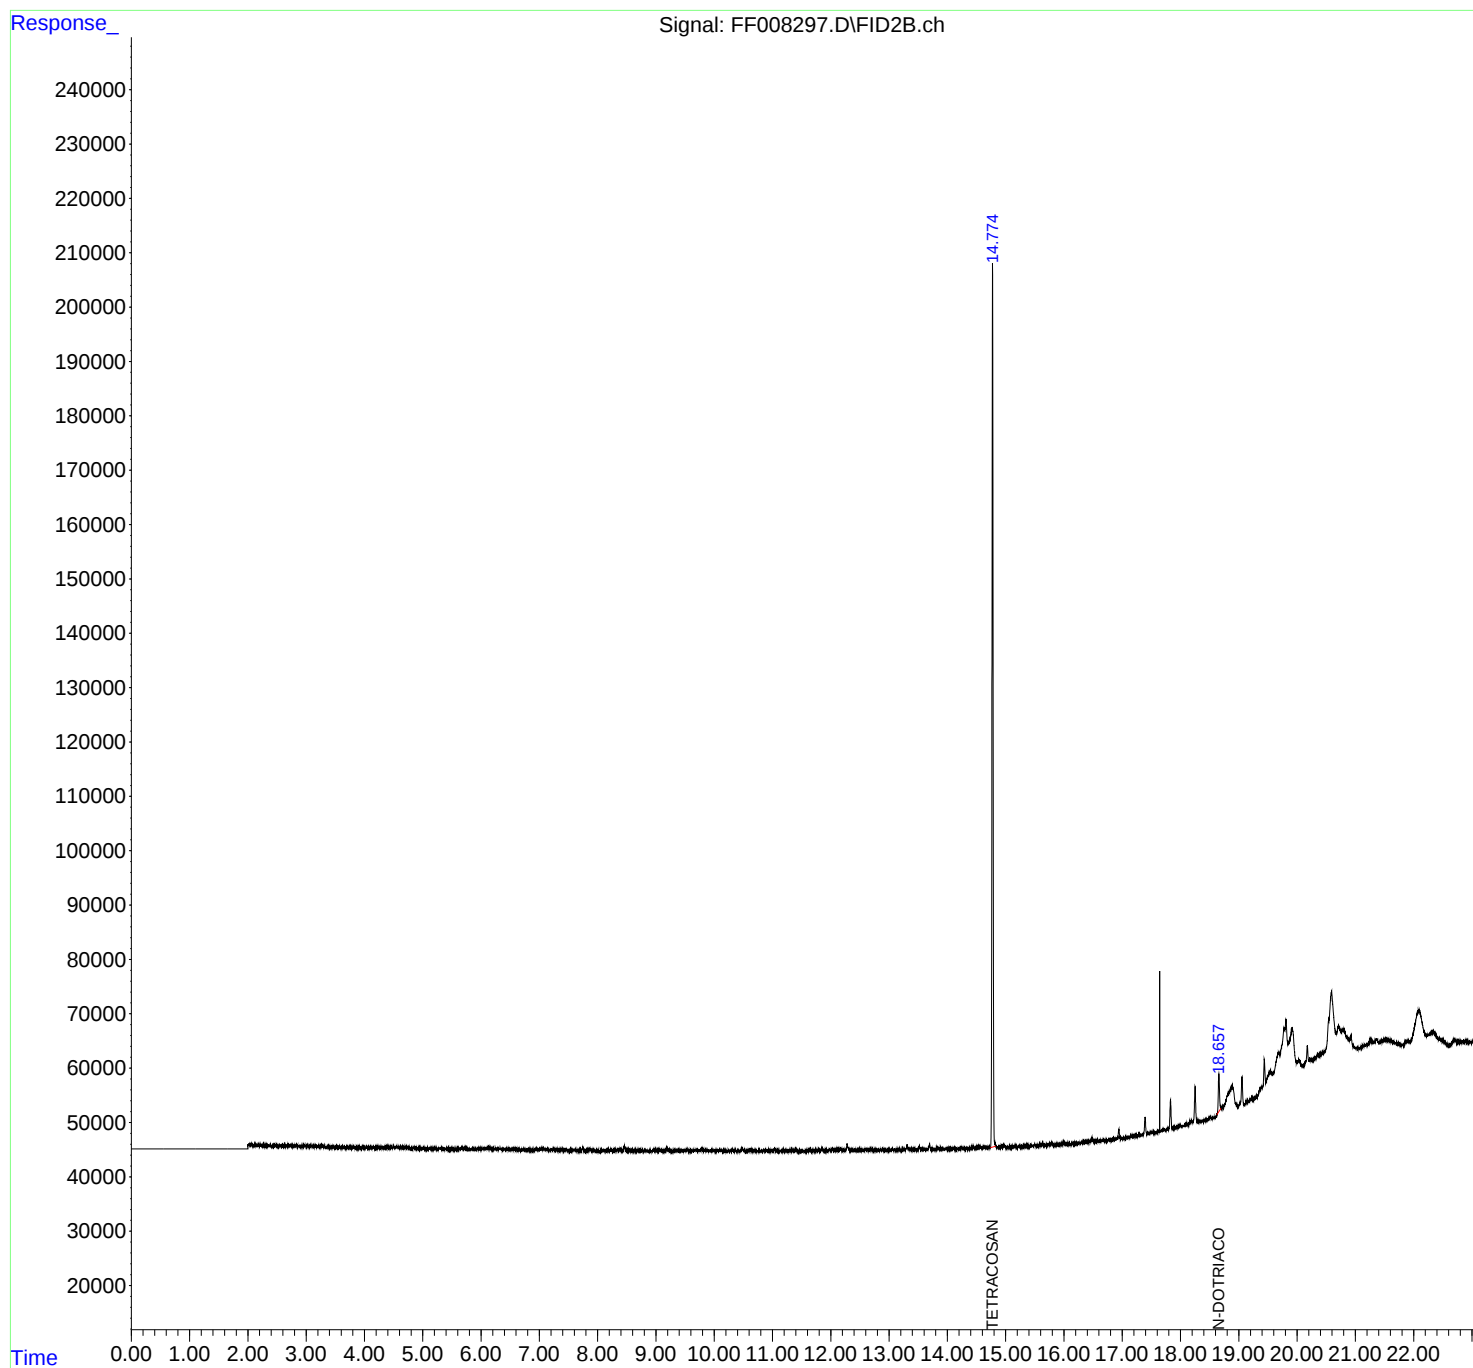


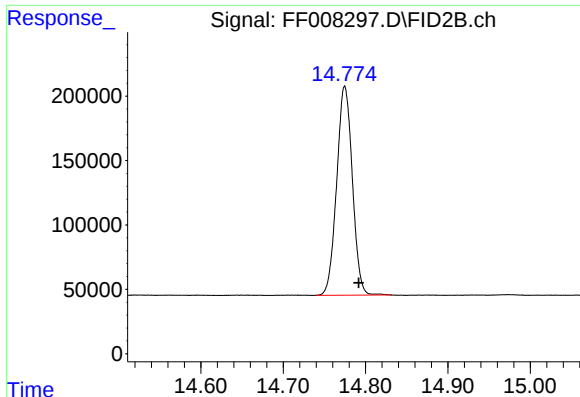

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.775 min
Delta R.T.: -0.017 min
Response: 2148010
Conc: 19.57 ug/ml

Instrument :
FID_F
ClientSampleId :

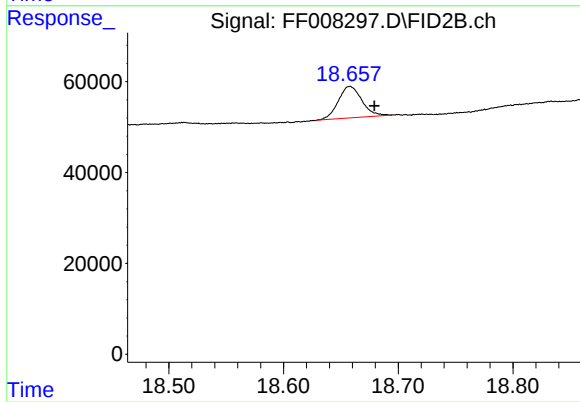

#14 N-DOTRIACONTANE

R.T.: 18.658 min
Delta R.T.: -0.021 min
Response: 99189
Conc: 0.82 ug/ml