

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
 Data File : FF008303.D
 Signal(s) : FID2B.ch
 Acq On : 21 Apr 2021 23:47
 Operator : DD\AJ
 Sample : M2106-02
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 22 03:42:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
 Quant Title :
 QLast Update : Tue Apr 06 02:37:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.777	1655070	15.082 ug/ml
Target Compounds			
4) N-TETRADECANE	8.398	155471	1.199 ug/ml
7) N-EICOSANE	12.751f	104674	0.823 ug/ml
10) N-TETRACOSANE	14.973	137148	1.101 ug/ml
11) N-HEXACOSANE	16.000	127916	1.045 ug/ml
12) N-OCTACOSANE	16.949	474747	3.888 ug/ml
13) N-TRIACONTANE	17.833	691070	5.655 ug/ml
14) N-DOTRIACONTANE	18.662	617789	5.094 ug/ml
15) N-TETRATRIACONTANE	19.444	250578	2.215 ug/ml
16) N-HEXATRIACONTANE	20.181	565295	5.493 ug/ml
17) N-OCTATRIACONTANE	20.936	293738	3.127 ug/ml
18) N-TETRACONTANE	21.885	231062	2.538 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
Data File : FF008303.D
Signal(s) : FID2B.ch
Acq On : 21 Apr 2021 23:47
Operator : DD\AJ
Sample : M2106-02
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Apr 22 03:42:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
Quant Title :
QLast Update : Tue Apr 06 02:37:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

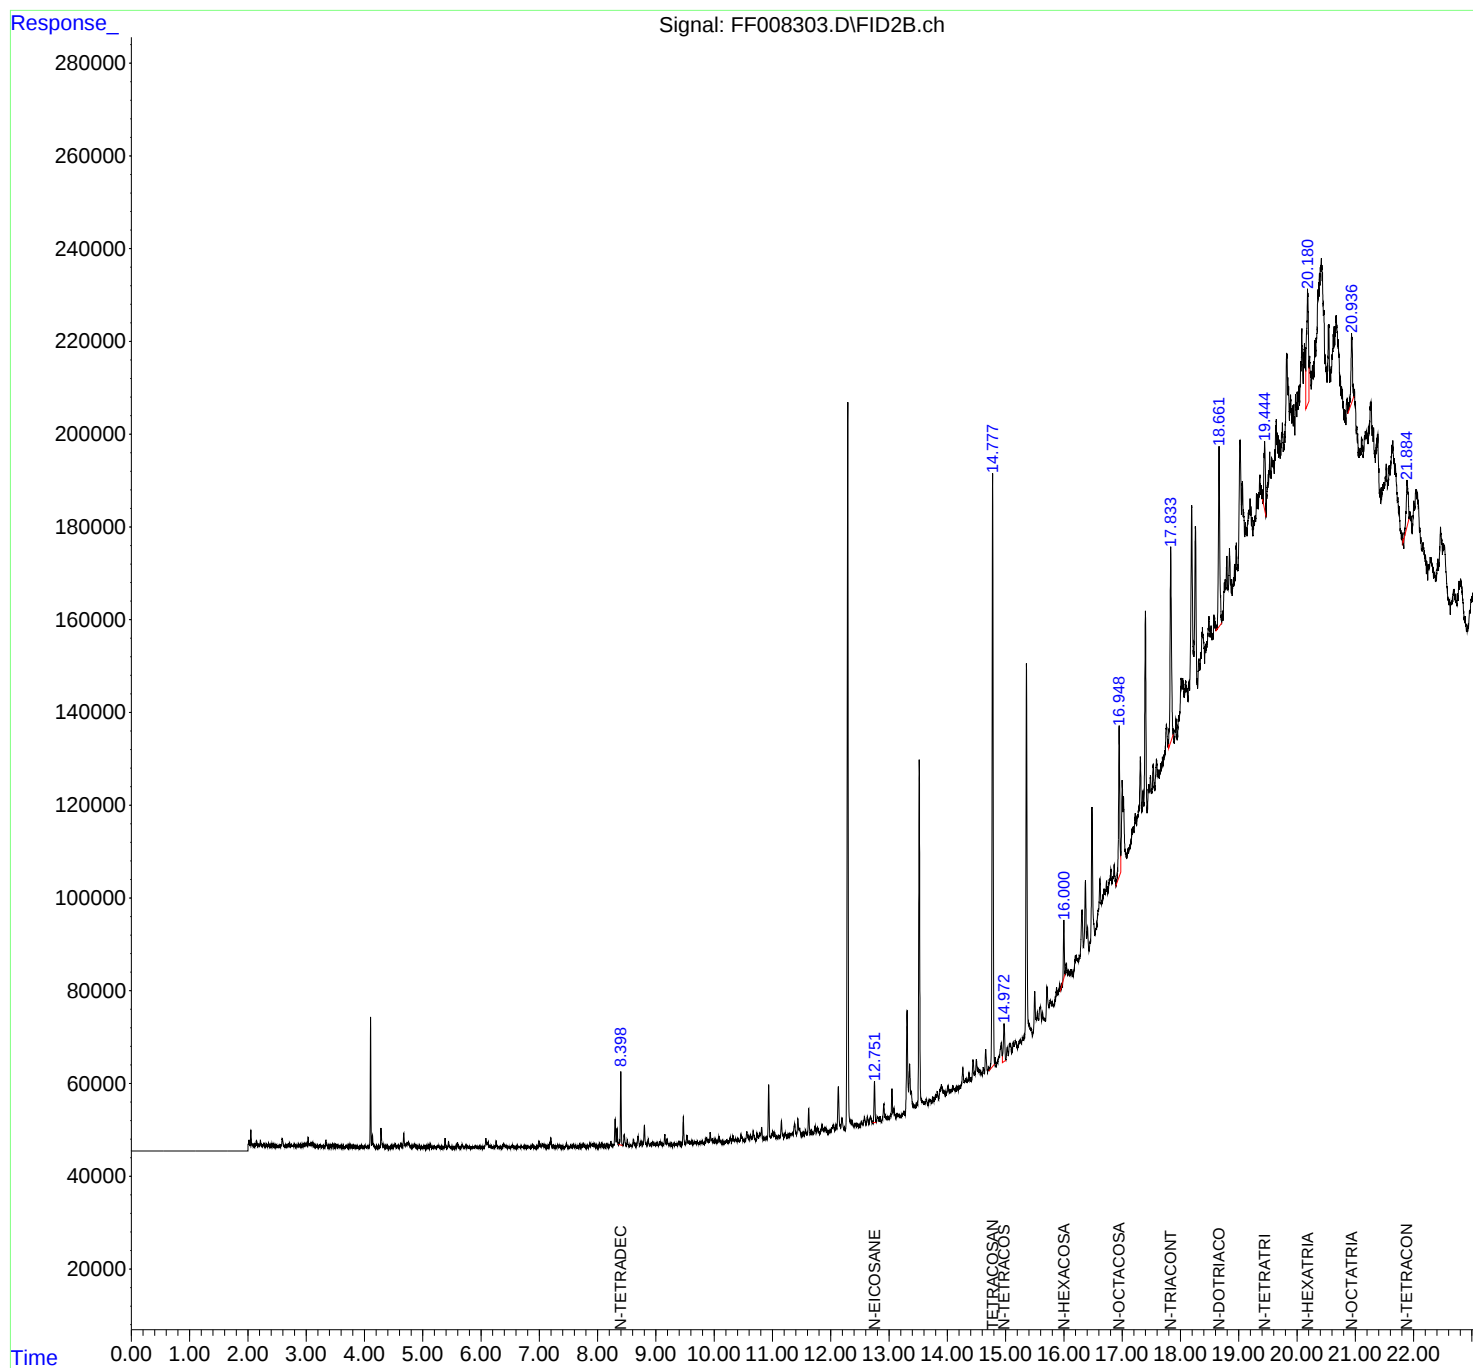


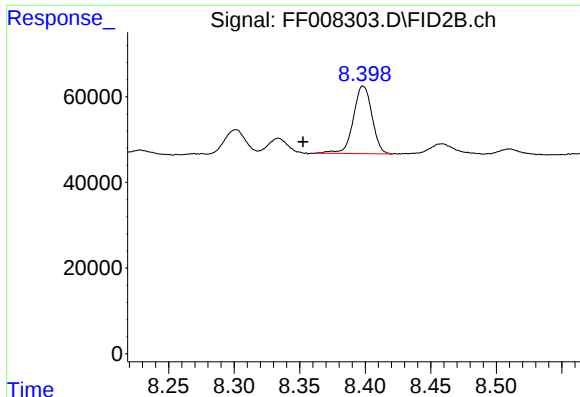

#4 N-TETRADECANE


R.T.: 8.398 min
Delta R.T.: 0.046 min
Response: 155471
Conc: 1.20 ug/ml

Instrument :
FID_F
ClientSampleId :

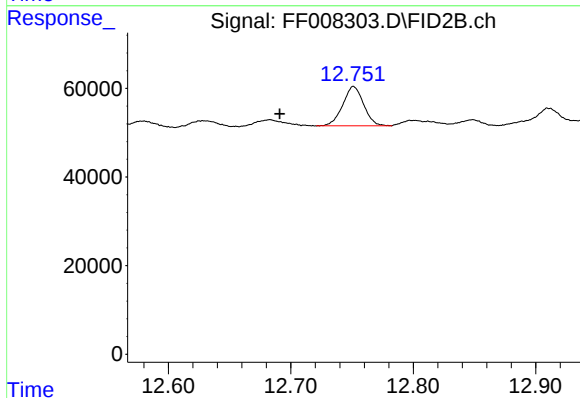


#7 N-EICOSANE

R.T.: 12.751 min
Delta R.T.: 0.060 min
Response: 104674
Conc: 0.82 ug/ml

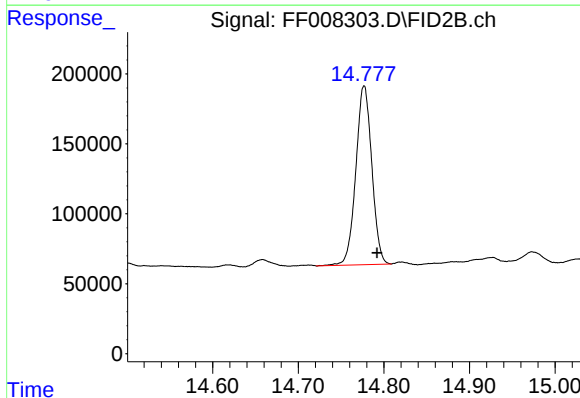


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.777 min
Delta R.T.: -0.015 min
Response: 1655070
Conc: 15.08 ug/ml

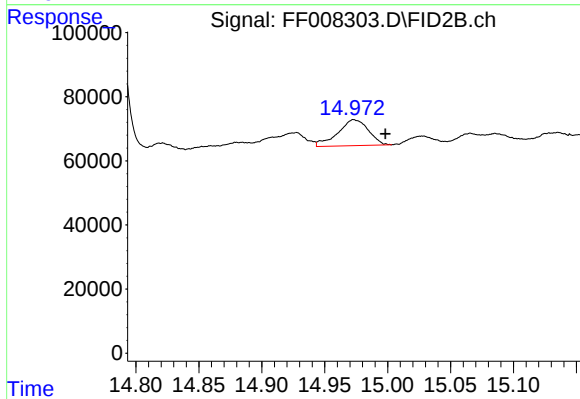

#10 N-TETRACOSANE


R.T.: 14.973 min
Delta R.T.: -0.025 min
Response: 137148
Conc: 1.10 ug/ml

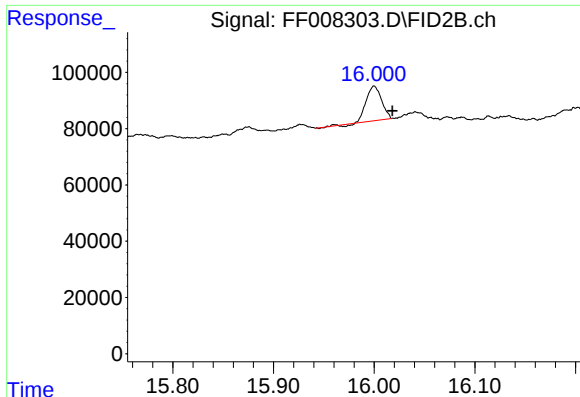

#11 N-HEXACOSANE


R.T.: 16.000 min
Delta R.T.: -0.018 min
Response: 127916
Conc: 1.05 ug/ml

Instrument :
FID_F
ClientSampleId :

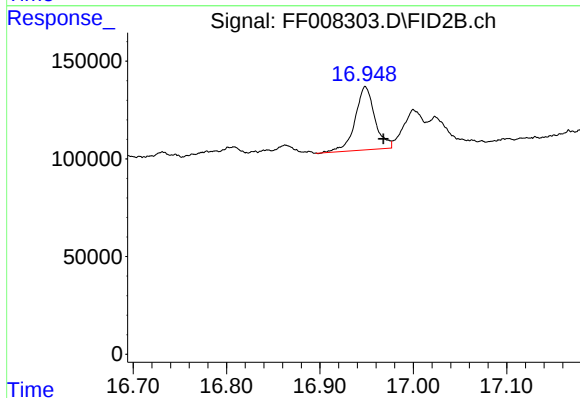


#12 N-OCTACOSANE

R.T.: 16.949 min
Delta R.T.: -0.019 min
Response: 474747
Conc: 3.89 ug/ml

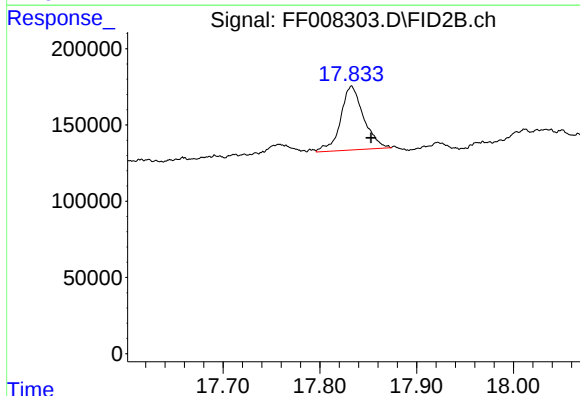


#13 N-TRIACONTANE

R.T.: 17.833 min
Delta R.T.: -0.020 min
Response: 691070
Conc: 5.66 ug/ml

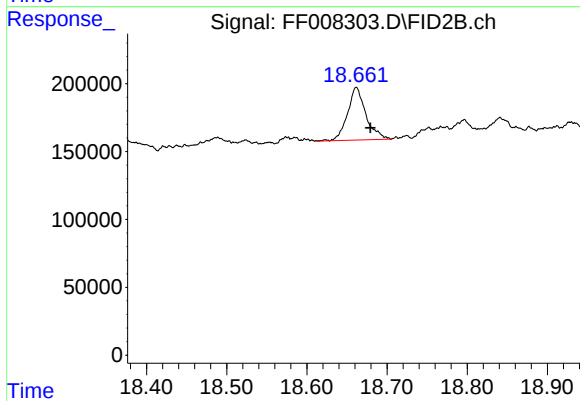

#14 N-DOTRIACONTANE

R.T.: 18.662 min
Delta R.T.: -0.018 min
Response: 617789
Conc: 5.09 ug/ml

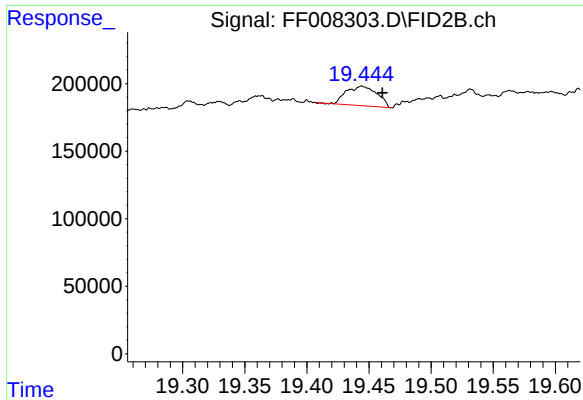

#15 N-TETRATRIACONTANE


R.T.: 19.444 min

Delta R.T.: -0.016 min

Response: 250578

Conc: 2.22 ug/ml

Instrument :
FID_F
ClientSampleId :

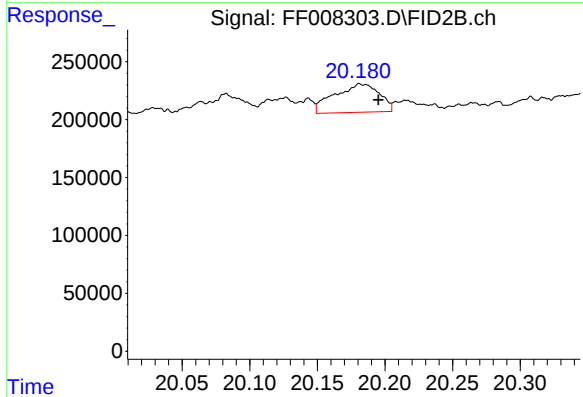


#16 N-HEXATRIACONTANE

R.T.: 20.181 min

Delta R.T.: -0.014 min

Response: 565295

Conc: 5.49 ug/ml

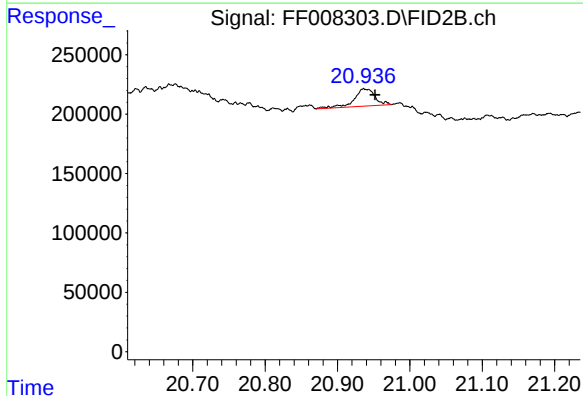


#17 N-OCTATRIACONTANE

R.T.: 20.936 min

Delta R.T.: -0.016 min

Response: 293738

Conc: 3.13 ug/ml

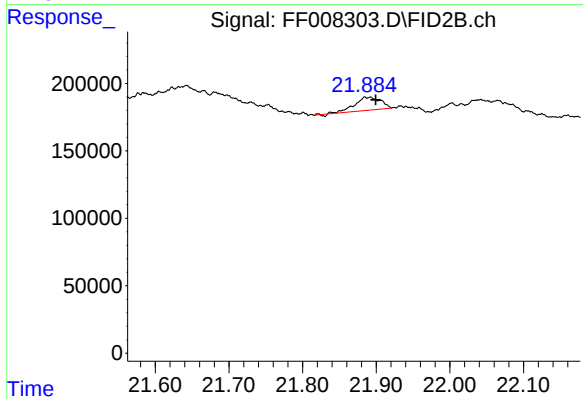

#18 N-TETRACONTANE

R.T.: 21.885 min

Delta R.T.: -0.015 min

Response: 231062

Conc: 2.54 ug/ml