

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
 Data File : FF008304.D
 Signal(s) : FID2B.ch
 Acq On : 22 Apr 2021 00:17
 Operator : DD\AJ
 Sample : M2106-05
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 22 03:43:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
 Quant Title :
 QLast Update : Tue Apr 06 02:37:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.780	1613148	14.700 ug/ml
Target Compounds			
4) N-TETRADECANE	8.400	132784	1.024 ug/ml
7) N-EICOSANE	12.756f	506504	3.980 ug/ml
10) N-TETRACOSANE	14.975	329108	2.641 ug/ml
11) N-HEXACOSANE	16.002	181364	1.482 ug/ml
12) N-OCTACOSANE	16.950	246409	2.018 ug/ml
13) N-TRIACONTANE	17.833	312324	2.556 ug/ml
14) N-DOTRIACONTANE	18.660	474403	3.912 ug/ml
15) N-TETRATRIACONTANE	19.441	174011	1.538 ug/ml
16) N-HEXATRIACONTANE	20.144f	10649	0.103 ug/ml
17) N-OCTATRIACONTANE	20.940	43718	0.465 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
Data File : FF008304.D
Signal(s) : FID2B.ch
Acq On : 22 Apr 2021 00:17
Operator : DD\AJ
Sample : M2106-05
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Apr 22 03:43:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
Quant Title :
QLast Update : Tue Apr 06 02:37:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

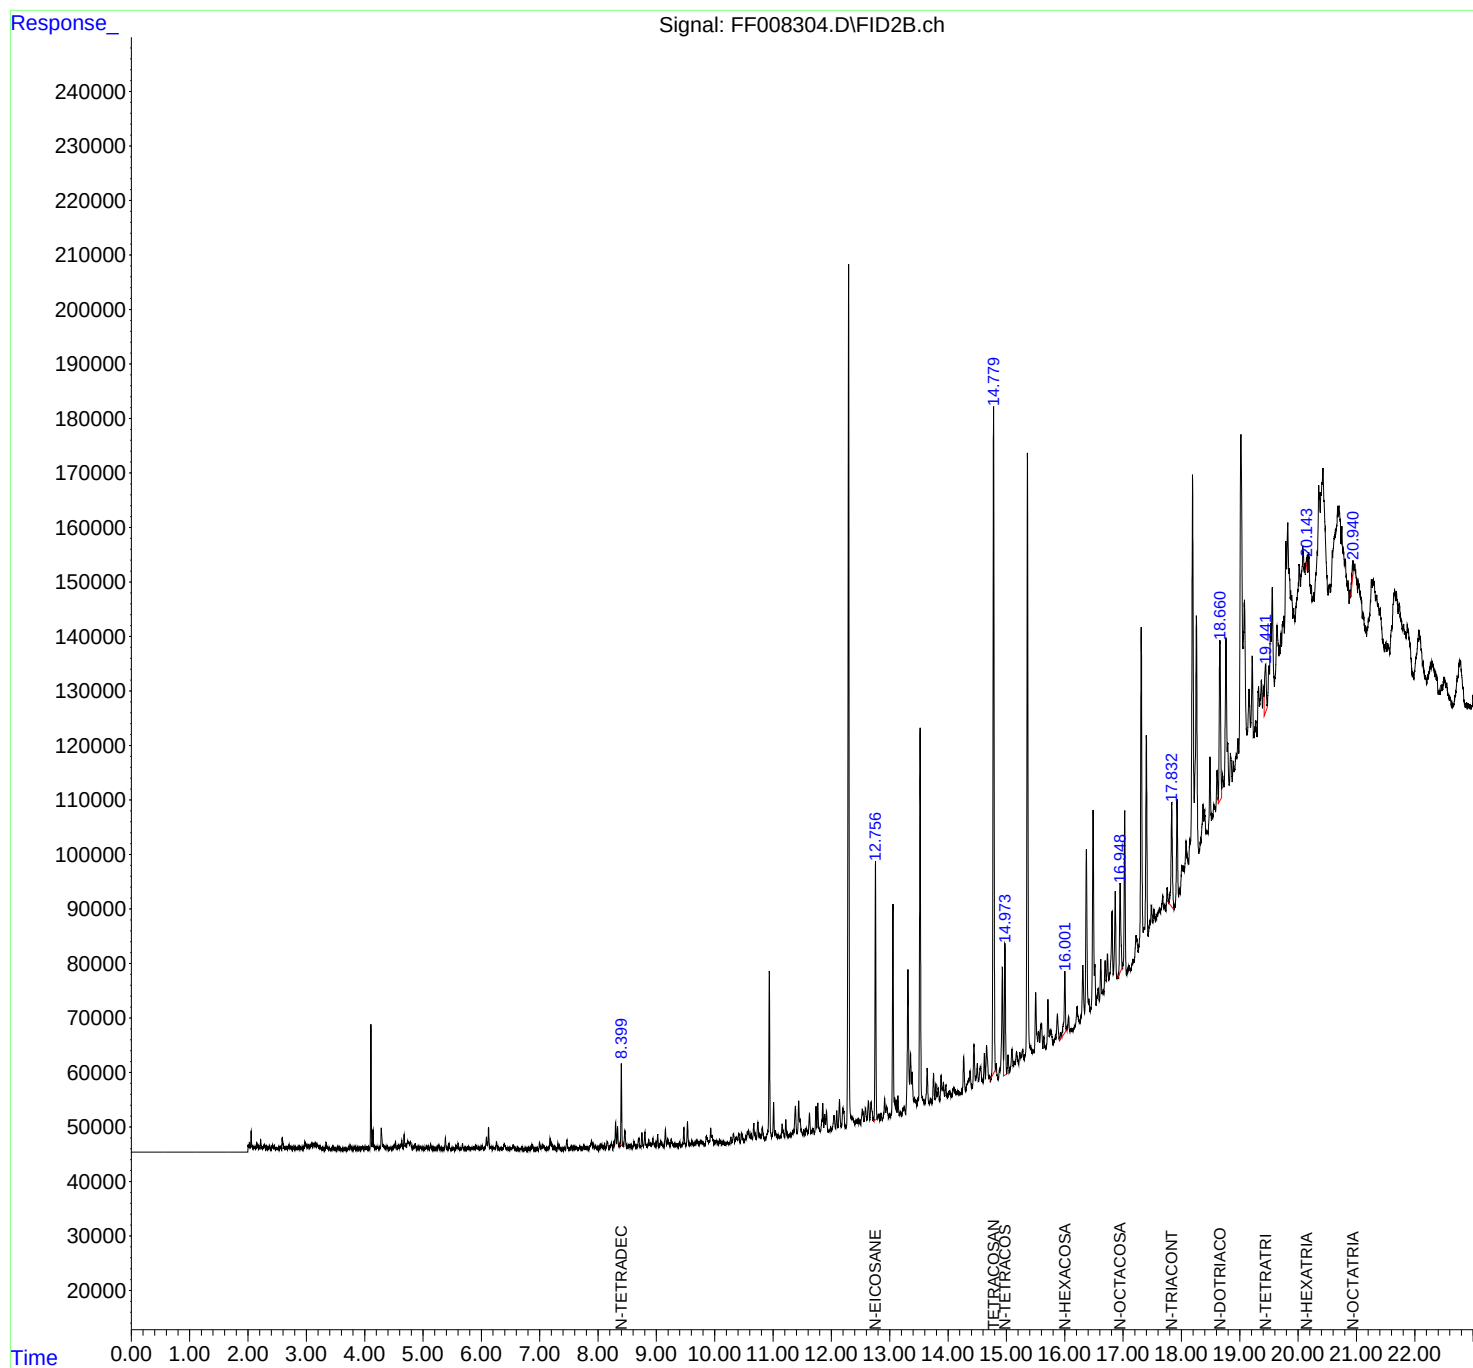


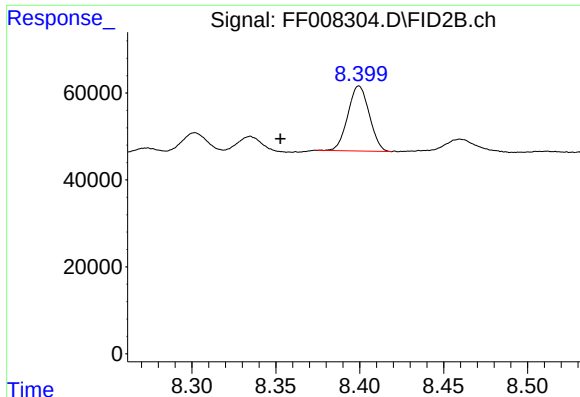

#4 N-TETRADECANE


R.T.: 8.400 min
Delta R.T.: 0.047 min
Response: 132784
Conc: 1.02 ug/ml

Instrument :
FID_F
ClientSampleId :

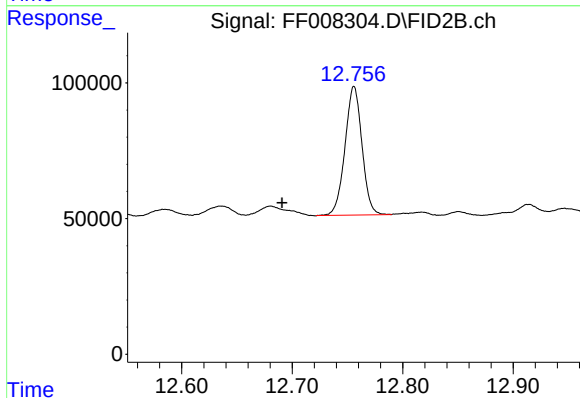


#7 N-EICOSANE

R.T.: 12.756 min
Delta R.T.: 0.065 min
Response: 506504
Conc: 3.98 ug/ml

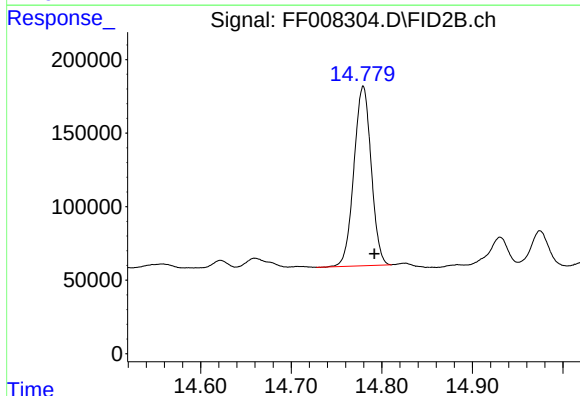


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.780 min
Delta R.T.: -0.012 min
Response: 1613148
Conc: 14.70 ug/ml

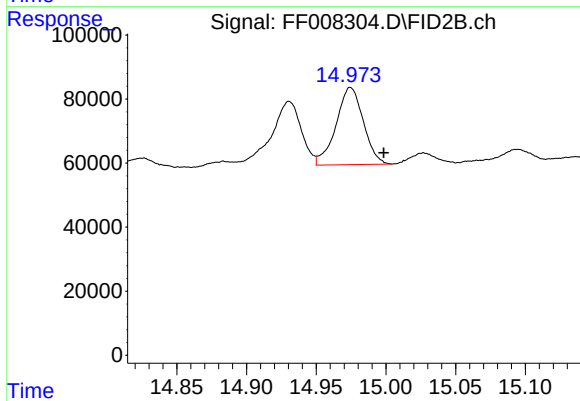

#10 N-TETRACOSANE


R.T.: 14.975 min
Delta R.T.: -0.024 min
Response: 329108
Conc: 2.64 ug/ml

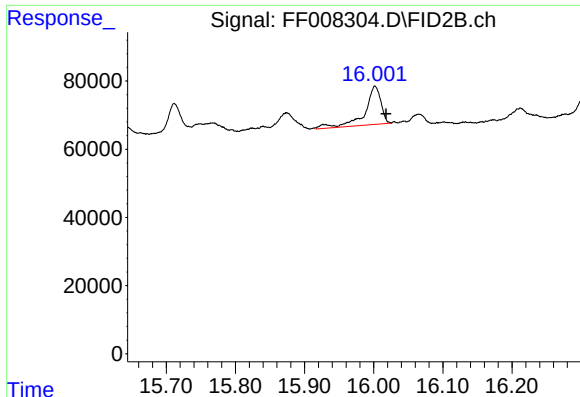

#11 N-HEXACOSANE


R.T.: 16.002 min
Delta R.T.: -0.016 min
Response: 181364
Conc: 1.48 ug/ml

Instrument :
FID_F
ClientSampleId :

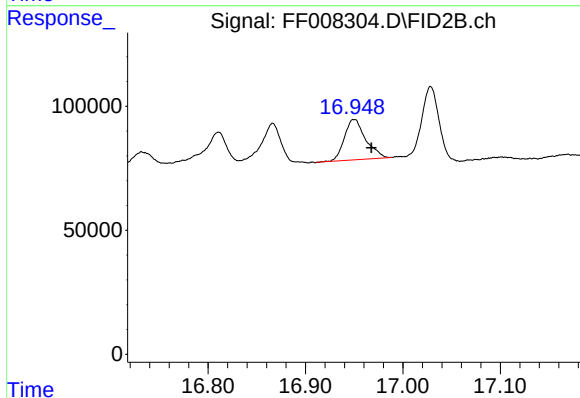


#12 N-OCTACOSANE

R.T.: 16.950 min
Delta R.T.: -0.018 min
Response: 246409
Conc: 2.02 ug/ml

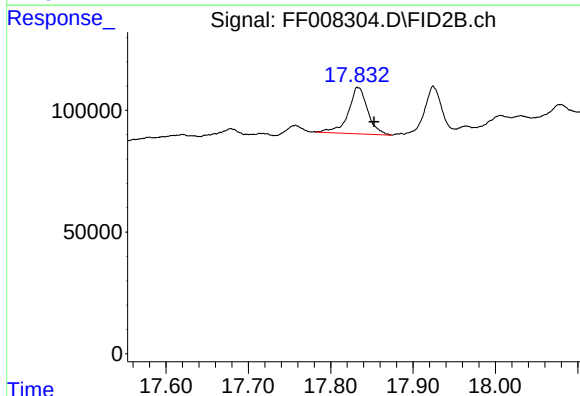


#13 N-TRIACONTANE

R.T.: 17.833 min
Delta R.T.: -0.020 min
Response: 312324
Conc: 2.56 ug/ml

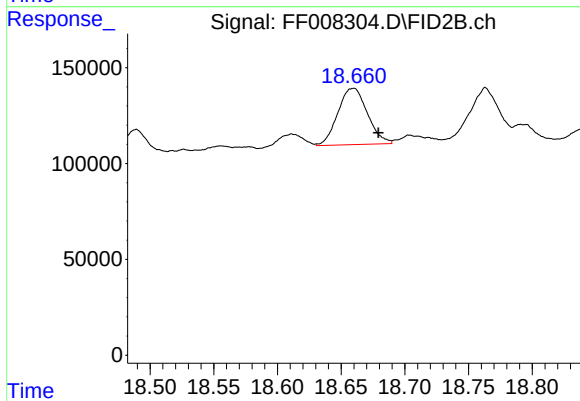

#14 N-DOTRIACONTANE


R.T.: 18.660 min
Delta R.T.: -0.020 min
Response: 474403
Conc: 3.91 ug/ml

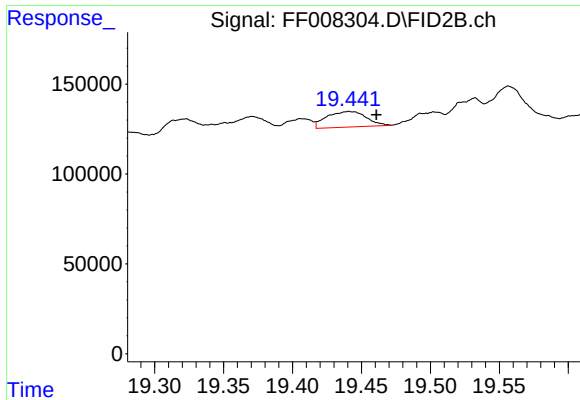

#15 N-TETRATRIACONTANE


R.T.: 19.441 min
Delta R.T.: -0.020 min
Response: 174011
Conc: 1.54 ug/ml

Instrument :
FID_F
ClientSampleId :

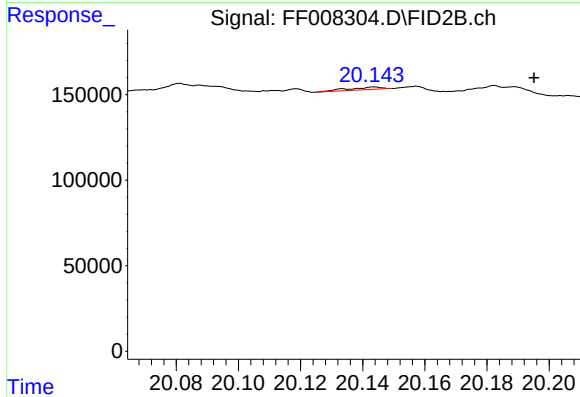

#16 N-HEXATRIACONTANE

R.T.: 20.144 min
Delta R.T.: -0.051 min
Response: 10649
Conc: 0.10 ug/ml

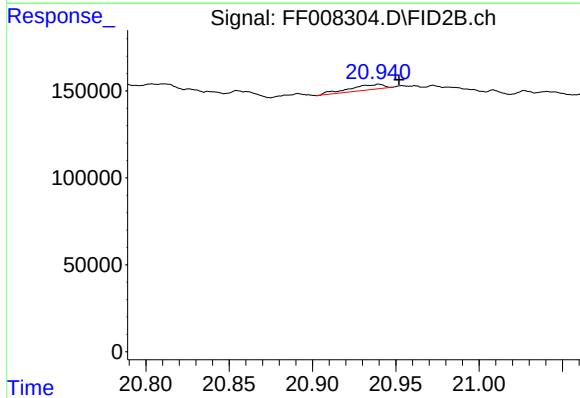

#17 N-OCTATRIACONTANE

R.T.: 20.940 min
Delta R.T.: -0.012 min
Response: 43718
Conc: 0.47 ug/ml