

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
 Data File : FF008307.D
 Signal(s) : FID2B.ch
 Acq On : 22 Apr 2021 01:51
 Operator : DD\AJ
 Sample : M2107-12
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 22 03:44:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
 Quant Title :
 QLast Update : Tue Apr 06 02:37:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.781	2147549	19.570 ug/ml
Target Compounds			
4) N-TETRADECANE	8.400	160973	1.241 ug/ml
7) N-EICOSANE	12.757f	166087	1.305 ug/ml
10) N-TETRACOSANE	14.979	205308	1.647 ug/ml
11) N-HEXACOSANE	16.003	166531	1.361 ug/ml
12) N-OCTACOSANE	16.951	251328	2.059 ug/ml
13) N-TRIACONTANE	17.835	256046	2.095 ug/ml
14) N-DOTRIACONTANE	18.660	308274	2.542 ug/ml
16) N-HEXATRIACONTANE	20.181	184065	1.789 ug/ml
18) N-TETRACONTANE	21.909	245829	2.700 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
Data File : FF008307.D
Signal(s) : FID2B.ch
Acq On : 22 Apr 2021 01:51
Operator : DD\AJ
Sample : M2107-12
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Apr 22 03:44:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
Quant Title :
QLast Update : Tue Apr 06 02:37:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

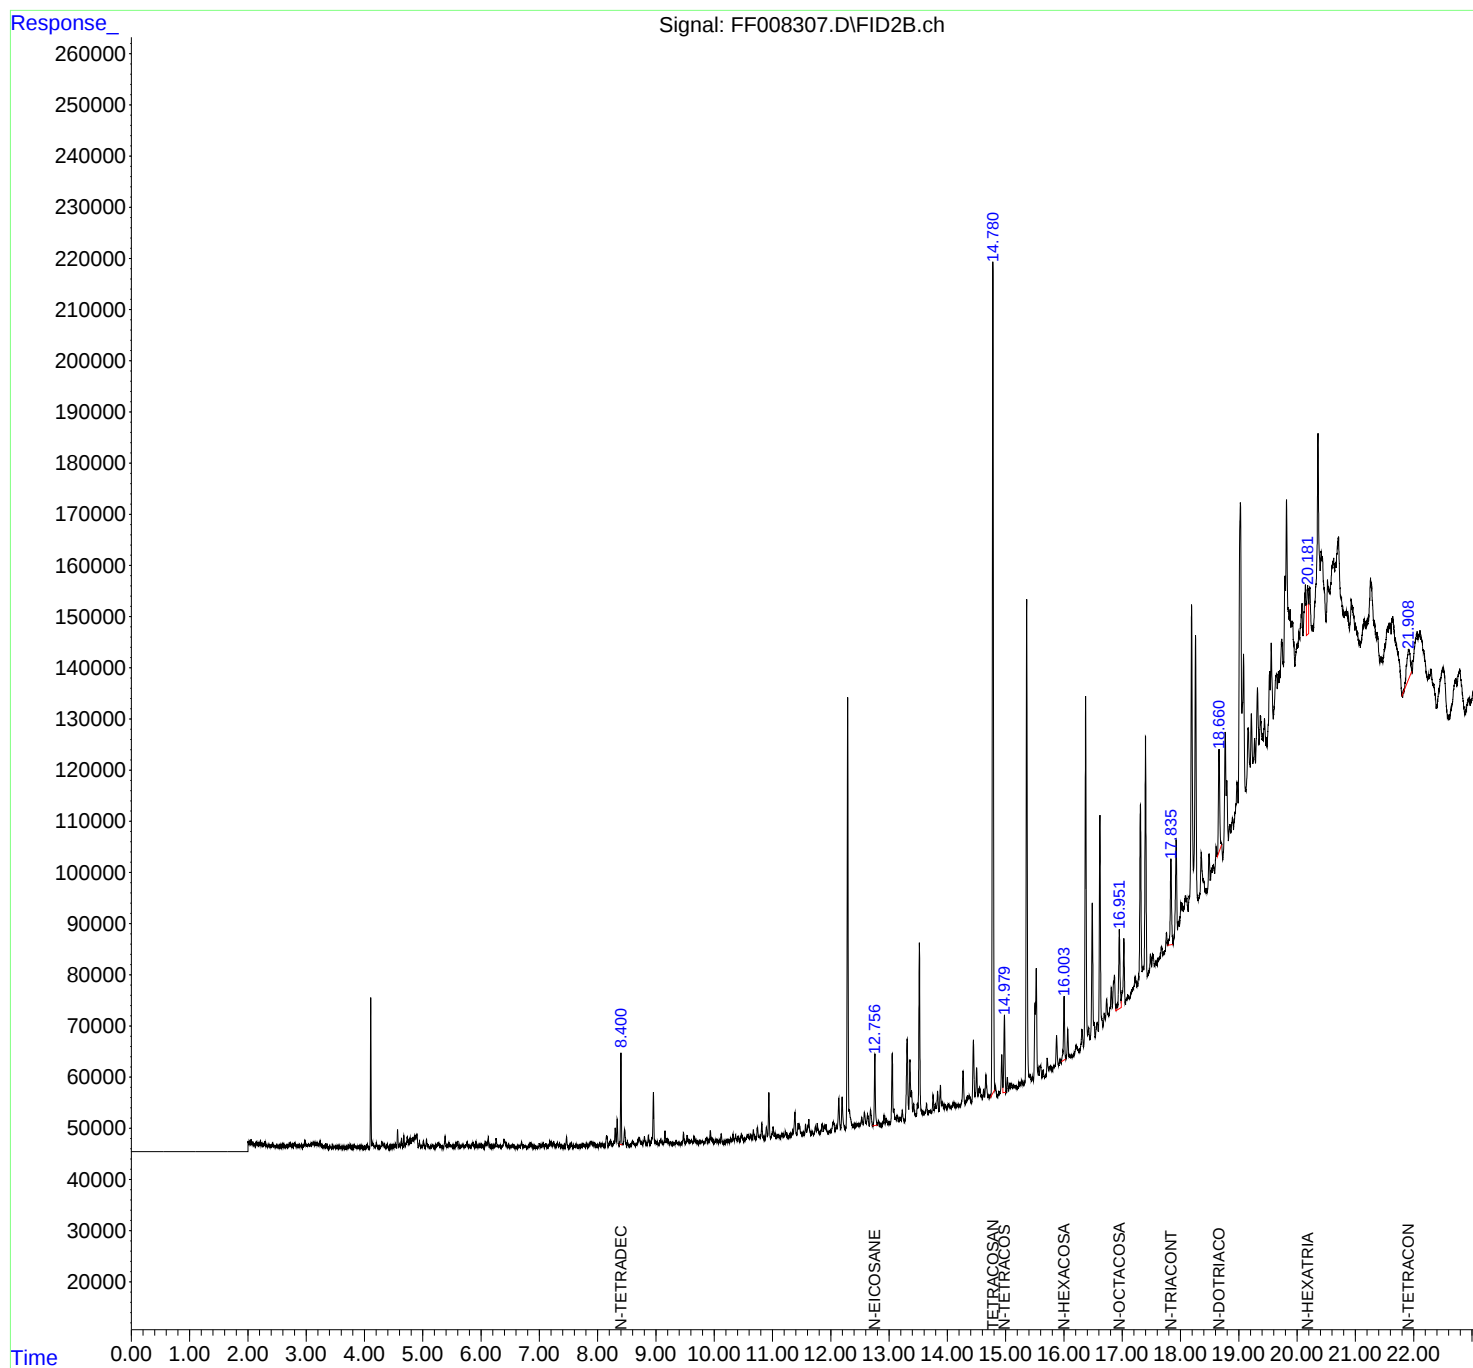


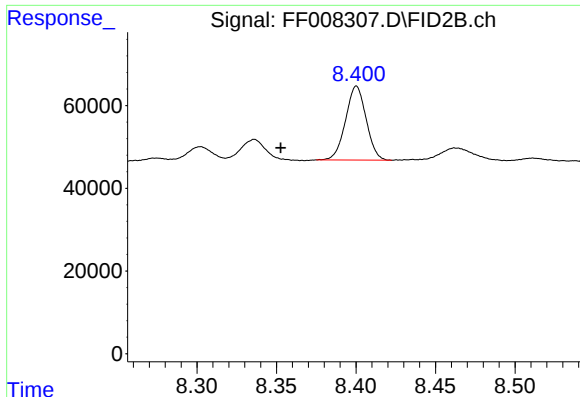

#4 N-TETRADECANE


R.T.: 8.400 min
Delta R.T.: 0.048 min
Response: 160973
Conc: 1.24 ug/ml

Instrument :
FID_F
ClientSampleId :

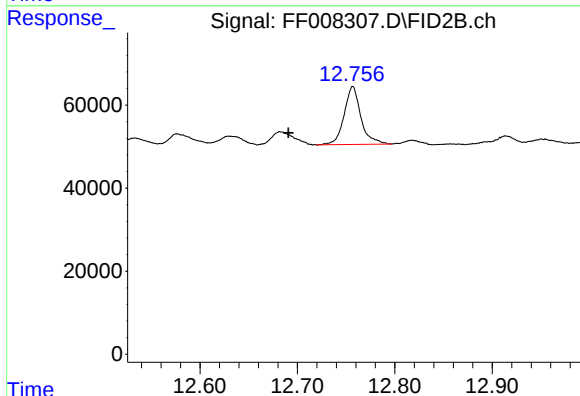


#7 N-EICOSANE

R.T.: 12.757 min
Delta R.T.: 0.066 min
Response: 166087
Conc: 1.31 ug/ml

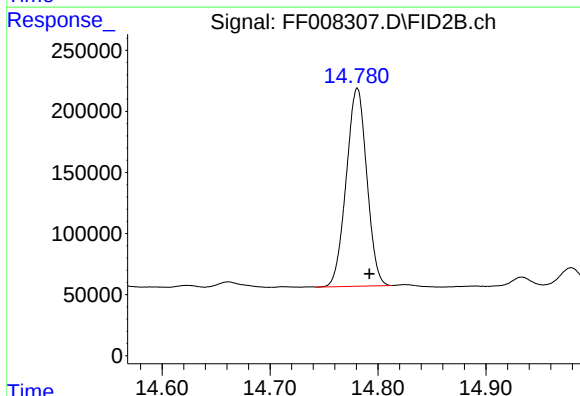


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.781 min
Delta R.T.: -0.011 min
Response: 2147549
Conc: 19.57 ug/ml

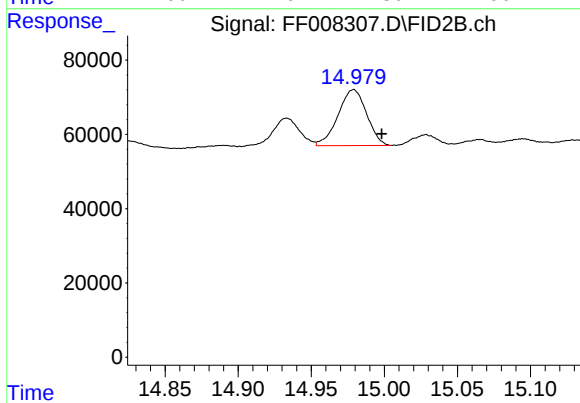

#10 N-TETRACOSANE


R.T.: 14.979 min
Delta R.T.: -0.019 min
Response: 205308
Conc: 1.65 ug/ml

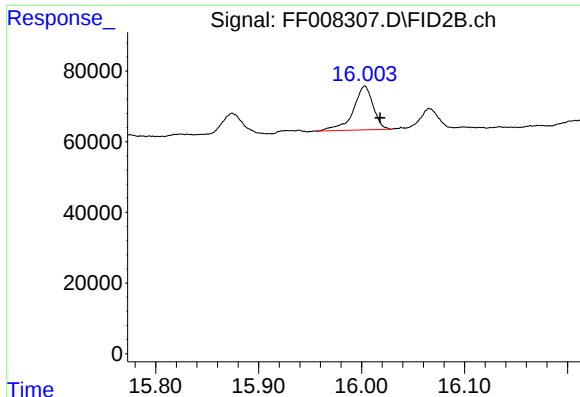

#11 N-HEXACOSANE


R.T.: 16.003 min
Delta R.T.: -0.015 min
Response: 166531
Conc: 1.36 ug/ml

Instrument :
FID_F
ClientSampleId :

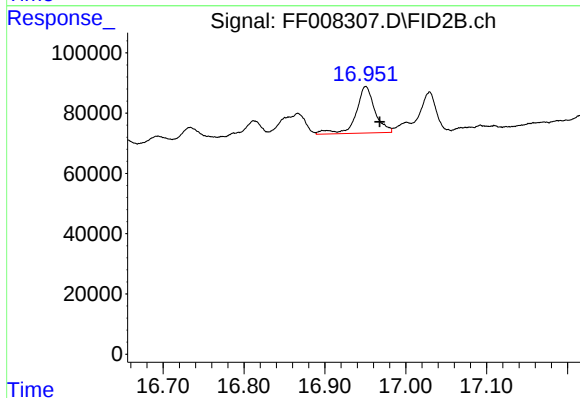


#12 N-OCTACOSANE

R.T.: 16.951 min
Delta R.T.: -0.017 min
Response: 251328
Conc: 2.06 ug/ml

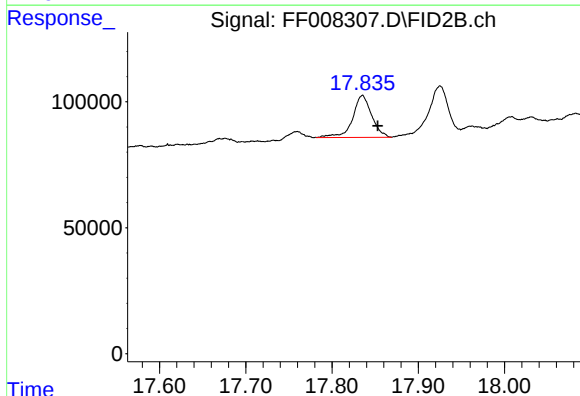


#13 N-TRIACONTANE

R.T.: 17.835 min
Delta R.T.: -0.018 min
Response: 256046
Conc: 2.10 ug/ml

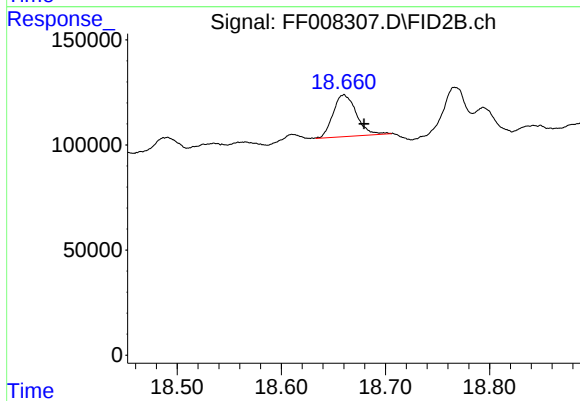

#14 N-DOTRIACONTANE


R.T.: 18.660 min
Delta R.T.: -0.019 min
Response: 308274
Conc: 2.54 ug/ml

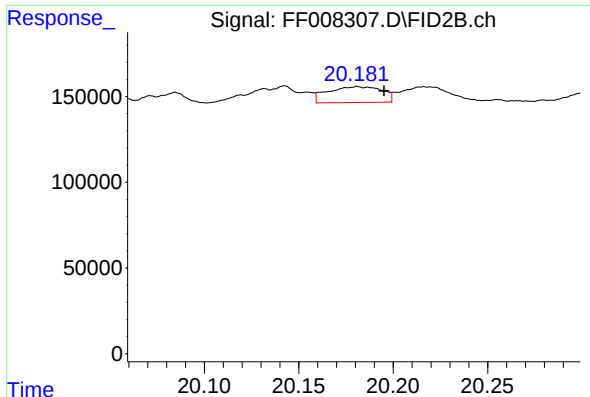

#16 N-HEXATRIACONTANE

R.T.: 20.181 min
Delta R.T.: -0.014 min
Response: 184065
Conc: 1.79 ug/ml

Instrument :
FID_F
ClientSampleId :

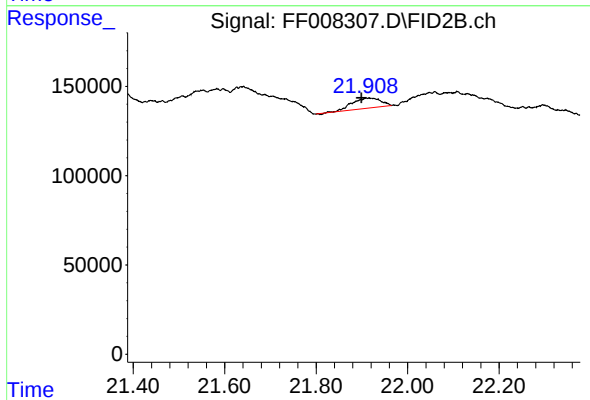

#18 N-TETRACONTANE

R.T.: 21.909 min
Delta R.T.: 0.010 min
Response: 245829
Conc: 2.70 ug/ml