

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
 Data File : FF008311.D
 Signal(s) : FID2B.ch
 Acq On : 22 Apr 2021 03:55
 Operator : DD\AJ
 Sample : M2107-05
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 22 07:16:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
 Quant Title :
 QLast Update : Tue Apr 06 02:37:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.780	1745269	15.904 ug/ml
Target Compounds			
4) N-TETRADECANE	8.401	93042	0.717 ug/ml
7) N-EICOSANE	12.757f	252950	1.988 ug/ml
10) N-TETRACOSANE	14.976	175231	1.406 ug/ml
12) N-OCTACOSANE	16.950	134392	1.101 ug/ml
13) N-TRIACONTANE	17.835	189079	1.547 ug/ml
14) N-DOTRIACONTANE	18.661	185758	1.532 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
Data File : FF008311.D
Signal(s) : FID2B.ch
Acq On : 22 Apr 2021 03:55
Operator : DD\AJ
Sample : M2107-05
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 22 07:16:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
Quant Title :
QLast Update : Tue Apr 06 02:37:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

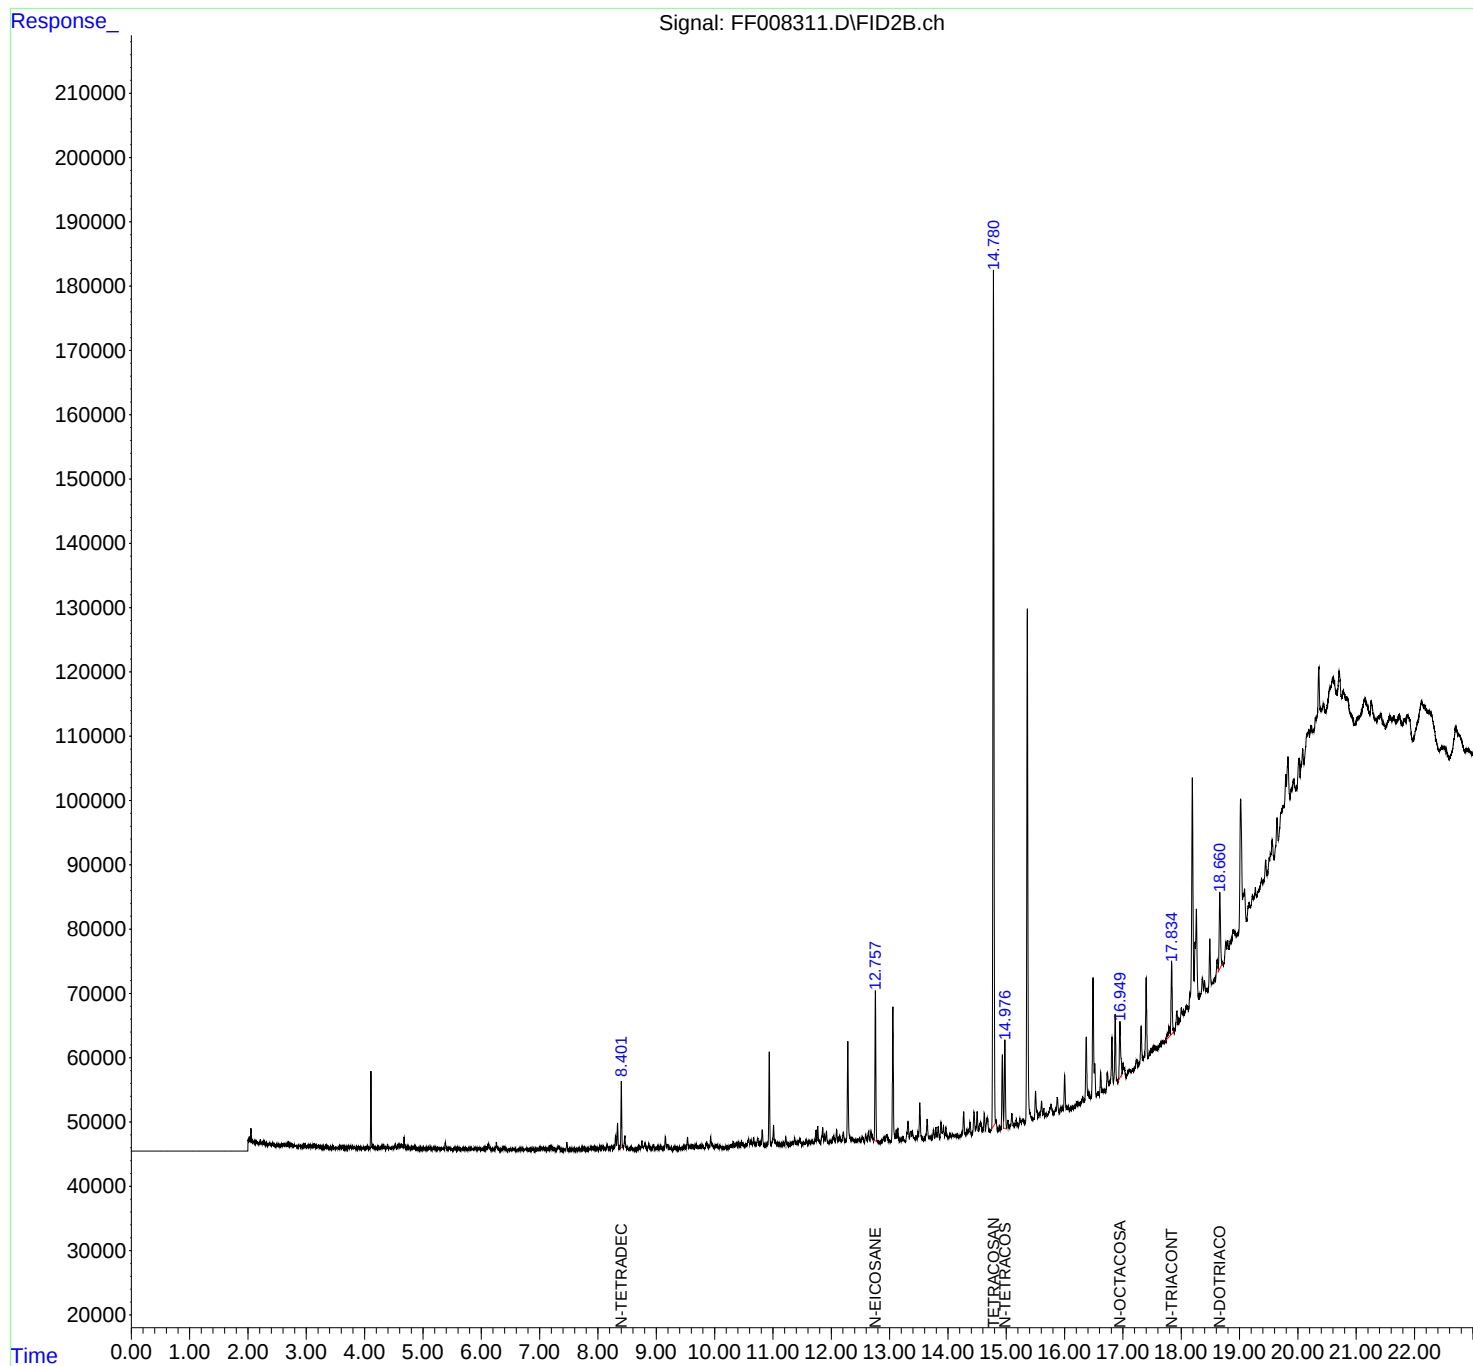


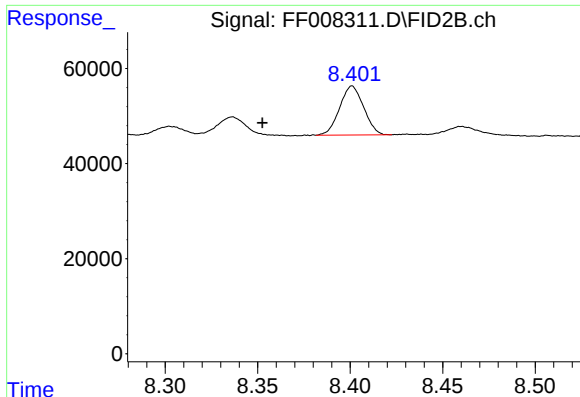

#4 N-TETRADECANE


R.T.: 8.401 min
Delta R.T.: 0.049 min
Response: 93042
Conc: 0.72 ug/ml

Instrument :
FID_F
ClientSampleId :

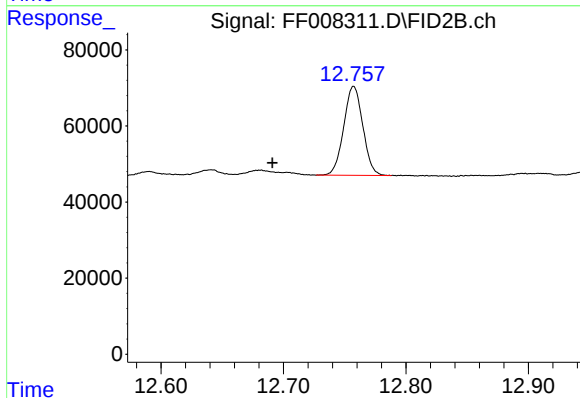


#7 N-EICOSANE

R.T.: 12.757 min
Delta R.T.: 0.066 min
Response: 252950
Conc: 1.99 ug/ml

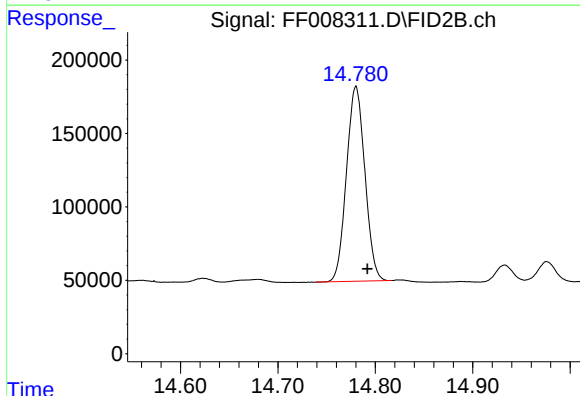


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.780 min
Delta R.T.: -0.012 min
Response: 1745269
Conc: 15.90 ug/ml

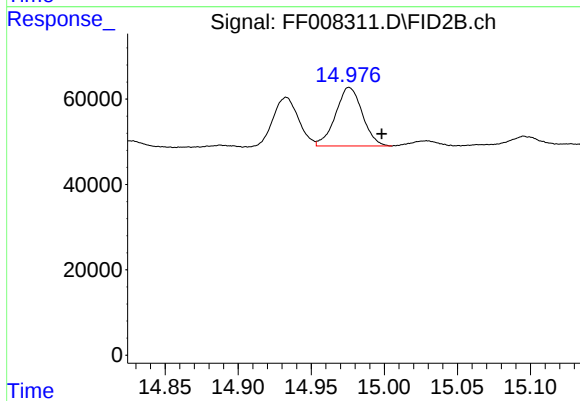

#10 N-TETRACOSANE


R.T.: 14.976 min
Delta R.T.: -0.022 min
Response: 175231
Conc: 1.41 ug/ml

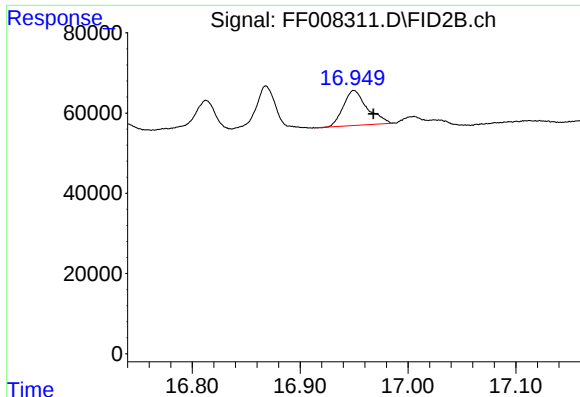

#12 N-OCTACOSANE


R.T.: 16.950 min
Delta R.T.: -0.018 min
Response: 134392
Conc: 1.10 ug/ml

Instrument :
FID_F
ClientSampleId :

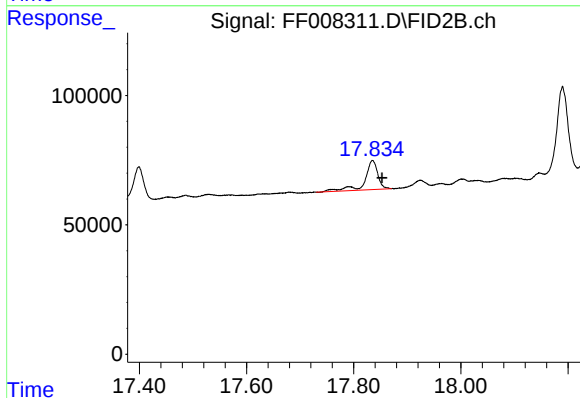

#13 N-TRIACONTANE

R.T.: 17.835 min
Delta R.T.: -0.018 min
Response: 189079
Conc: 1.55 ug/ml

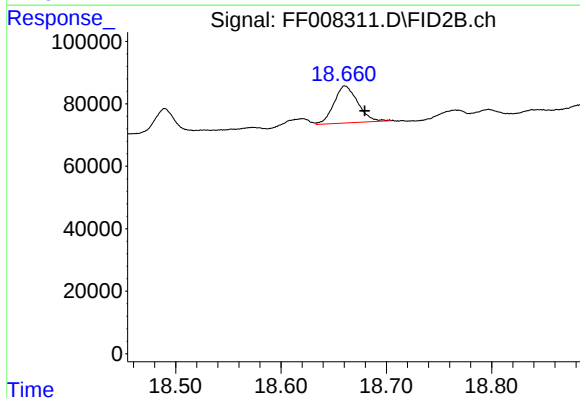

#14 N-DOTRIACONTANE

R.T.: 18.661 min
Delta R.T.: -0.019 min
Response: 185758
Conc: 1.53 ug/ml