

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
 Data File : FF008312.D
 Signal(s) : FID2B.ch
 Acq On : 22 Apr 2021 04:26
 Operator : DD\AJ
 Sample : M2106-11
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 22 07:16:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
 Quant Title :
 QLast Update : Tue Apr 06 02:37:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.780	1755088	15.994 ug/ml
Target Compounds			
4) N-TETRADECANE	8.401	152186	1.173 ug/ml
7) N-EICOSANE	12.757f	615999	4.841 ug/ml
10) N-TETRACOSANE	14.975	286327	2.298 ug/ml
11) N-HEXACOSANE	16.004	65258	0.533 ug/ml
12) N-OCTACOSANE	16.951	151574	1.241 ug/ml
13) N-TRIACONTANE	17.836	207531	1.698 ug/ml
14) N-DOTRIACONTANE	18.662	192279	1.585 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
Data File : FF008312.D
Signal(s) : FID2B.ch
Acq On : 22 Apr 2021 04:26
Operator : DD\AJ
Sample : M2106-11
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 22 07:16:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
Quant Title :
QLast Update : Tue Apr 06 02:37:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

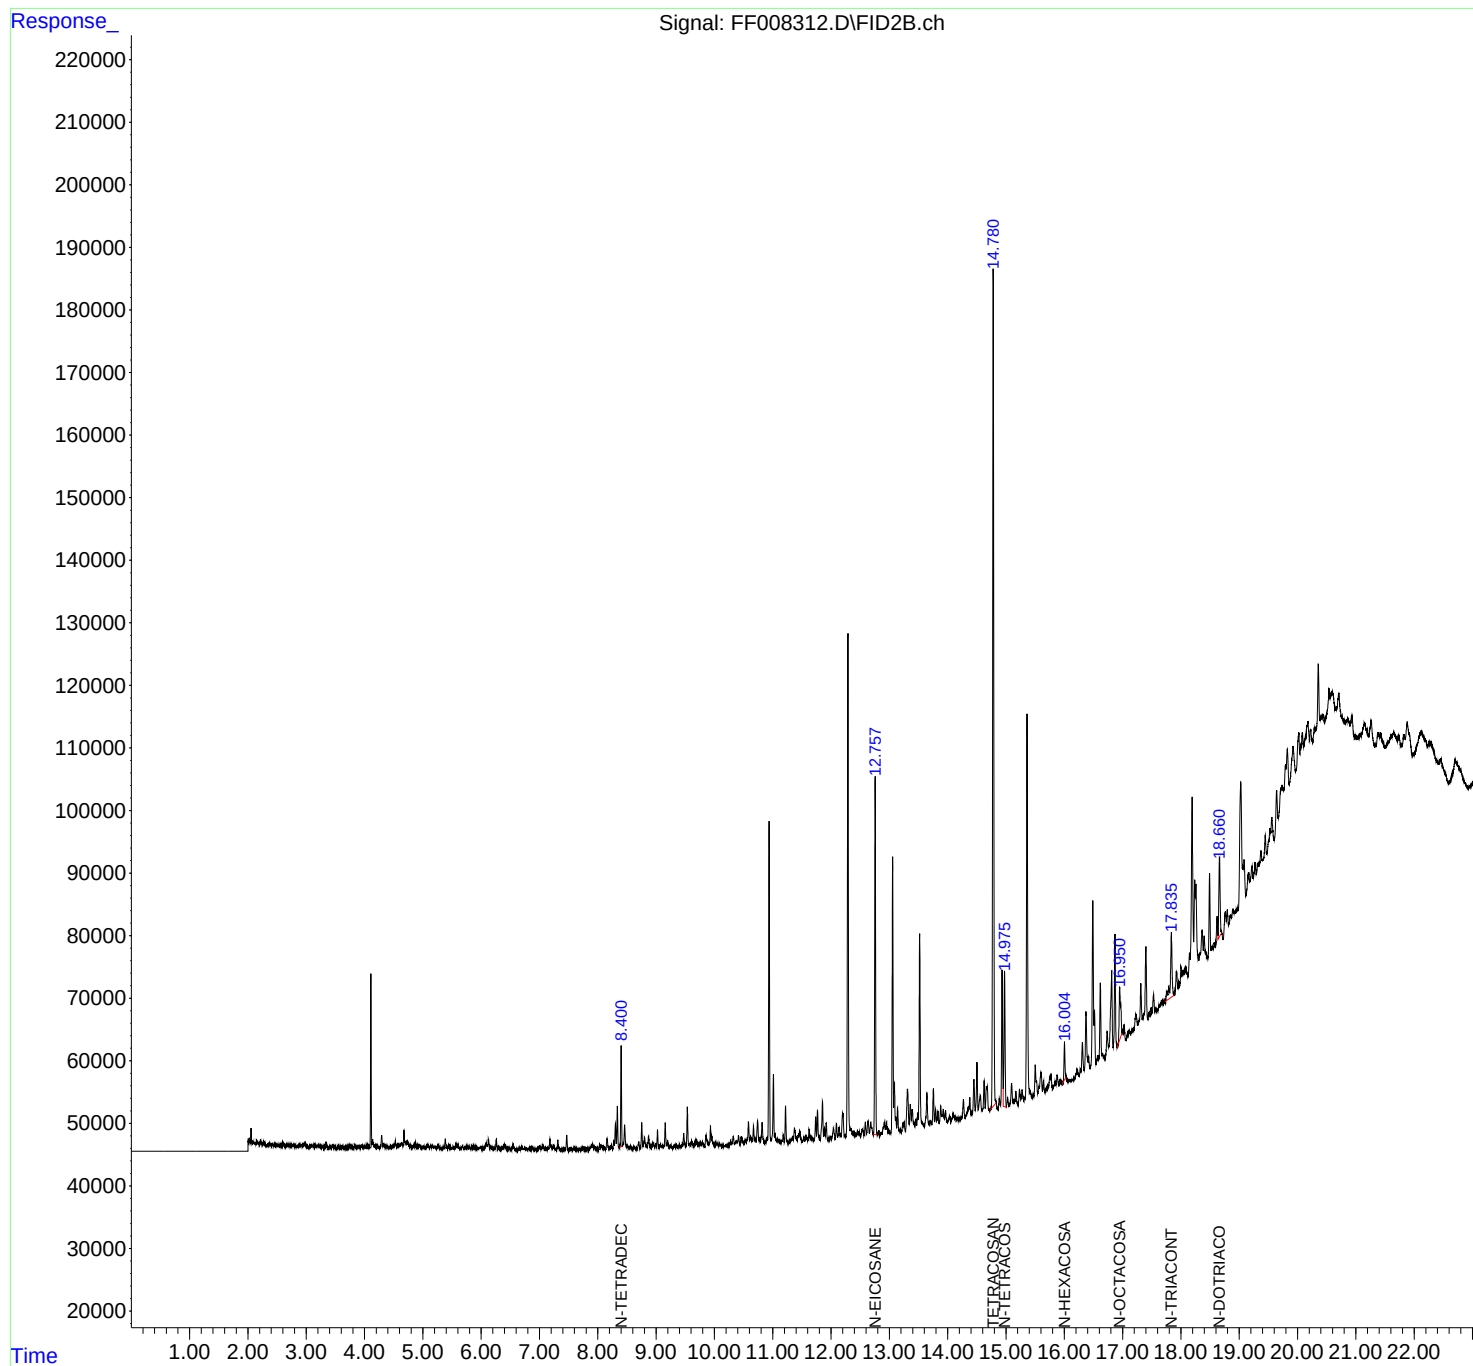


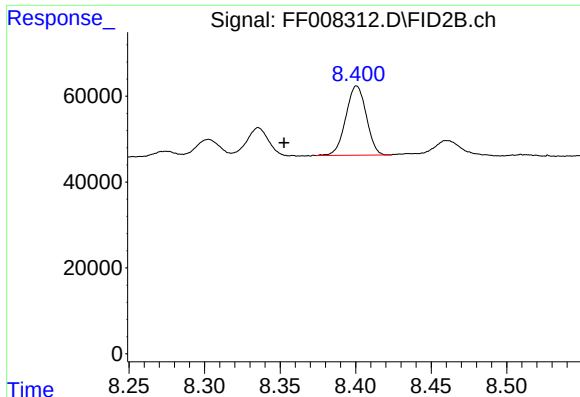

#4 N-TETRADECANE


R.T.: 8.401 min
Delta R.T.: 0.048 min
Response: 152186
Conc: 1.17 ug/ml

Instrument :
FID_F
ClientSampleId :

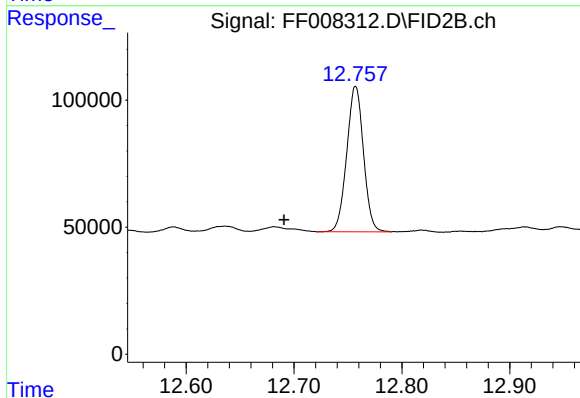


#7 N-EICOSANE

R.T.: 12.757 min
Delta R.T.: 0.066 min
Response: 615999
Conc: 4.84 ug/ml

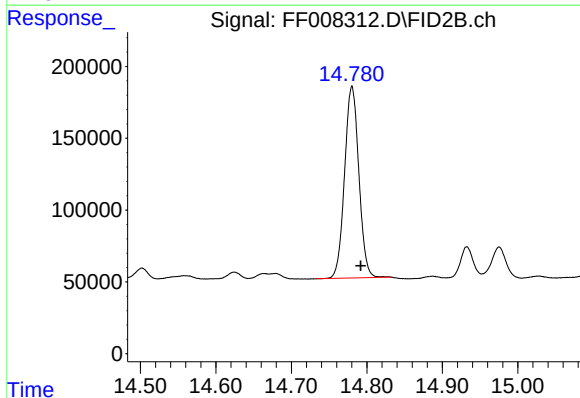


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.780 min
Delta R.T.: -0.012 min
Response: 1755088
Conc: 15.99 ug/ml

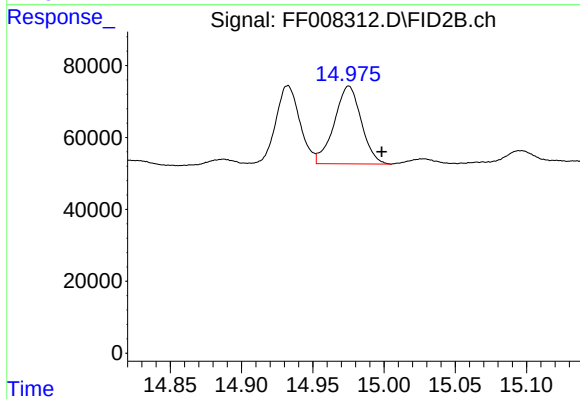

#10 N-TETRACOSANE


R.T.: 14.975 min
Delta R.T.: -0.023 min
Response: 286327
Conc: 2.30 ug/ml

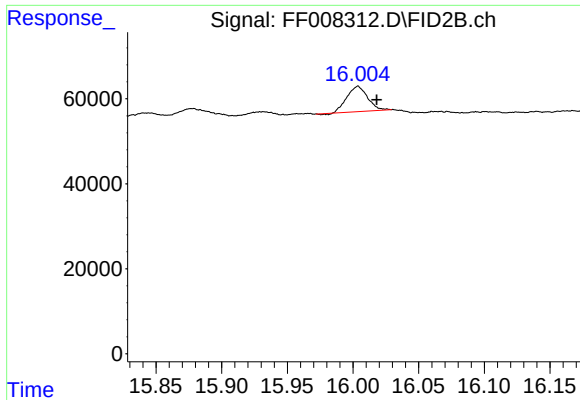

#11 N-HEXACOSANE


R.T.: 16.004 min
Delta R.T.: -0.014 min
Response: 65258
Conc: 0.53 ug/ml

Instrument :
FID_F
ClientSampleId :

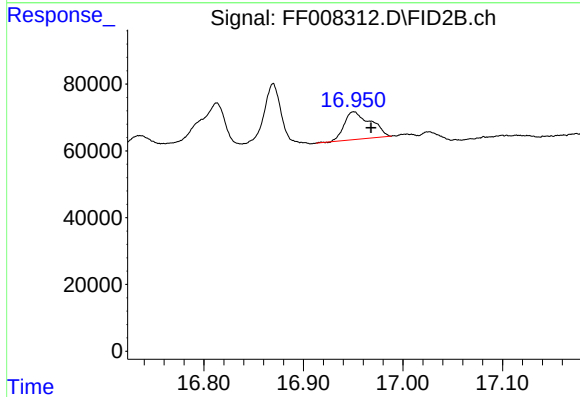


#12 N-OCTACOSANE

R.T.: 16.951 min
Delta R.T.: -0.017 min
Response: 151574
Conc: 1.24 ug/ml

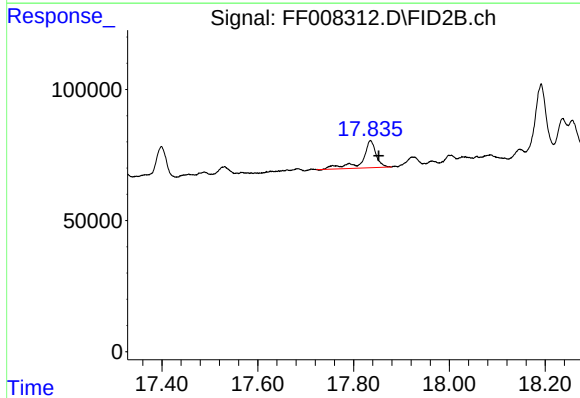

#13 N-TRIACONTANE

R.T.: 17.836 min
Delta R.T.: -0.017 min
Response: 207531
Conc: 1.70 ug/ml

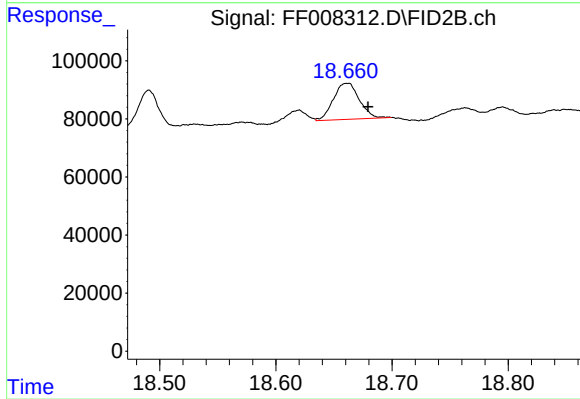

#14 N-DOTRIACONTANE

R.T.: 18.662 min
Delta R.T.: -0.018 min
Response: 192279
Conc: 1.59 ug/ml