

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
 Data File : FF008313.D
 Signal(s) : FID2B.ch
 Acq On : 22 Apr 2021 04:57
 Operator : DD\AJ
 Sample : M2106-14
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 22 07:16:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
 Quant Title :
 QLast Update : Tue Apr 06 02:37:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.781	2177304	19.841 ug/ml
Target Compounds			
4) N-TETRADECANE	8.401	193260	1.490 ug/ml
7) N-EICOSANE	12.757f	101218	0.795 ug/ml
10) N-TETRACOSANE	14.978	141013	1.132 ug/ml
11) N-HEXACOSANE	16.020	4733090	38.669 ug/ml
12) N-OCTACOSANE	16.950	182259	1.493 ug/ml
13) N-TRIACONTANE	17.835	233909	1.914 ug/ml
14) N-DOTRIACONTANE	18.662	299824	2.472 ug/ml
15) N-TETRATRIACONTANE	19.530f	120105	1.062 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042121\
Data File : FF008313.D
Signal(s) : FID2B.ch
Acq On : 22 Apr 2021 04:57
Operator : DD\AJ
Sample : M2106-14
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 22 07:16:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
Quant Title :
QLast Update : Tue Apr 06 02:37:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

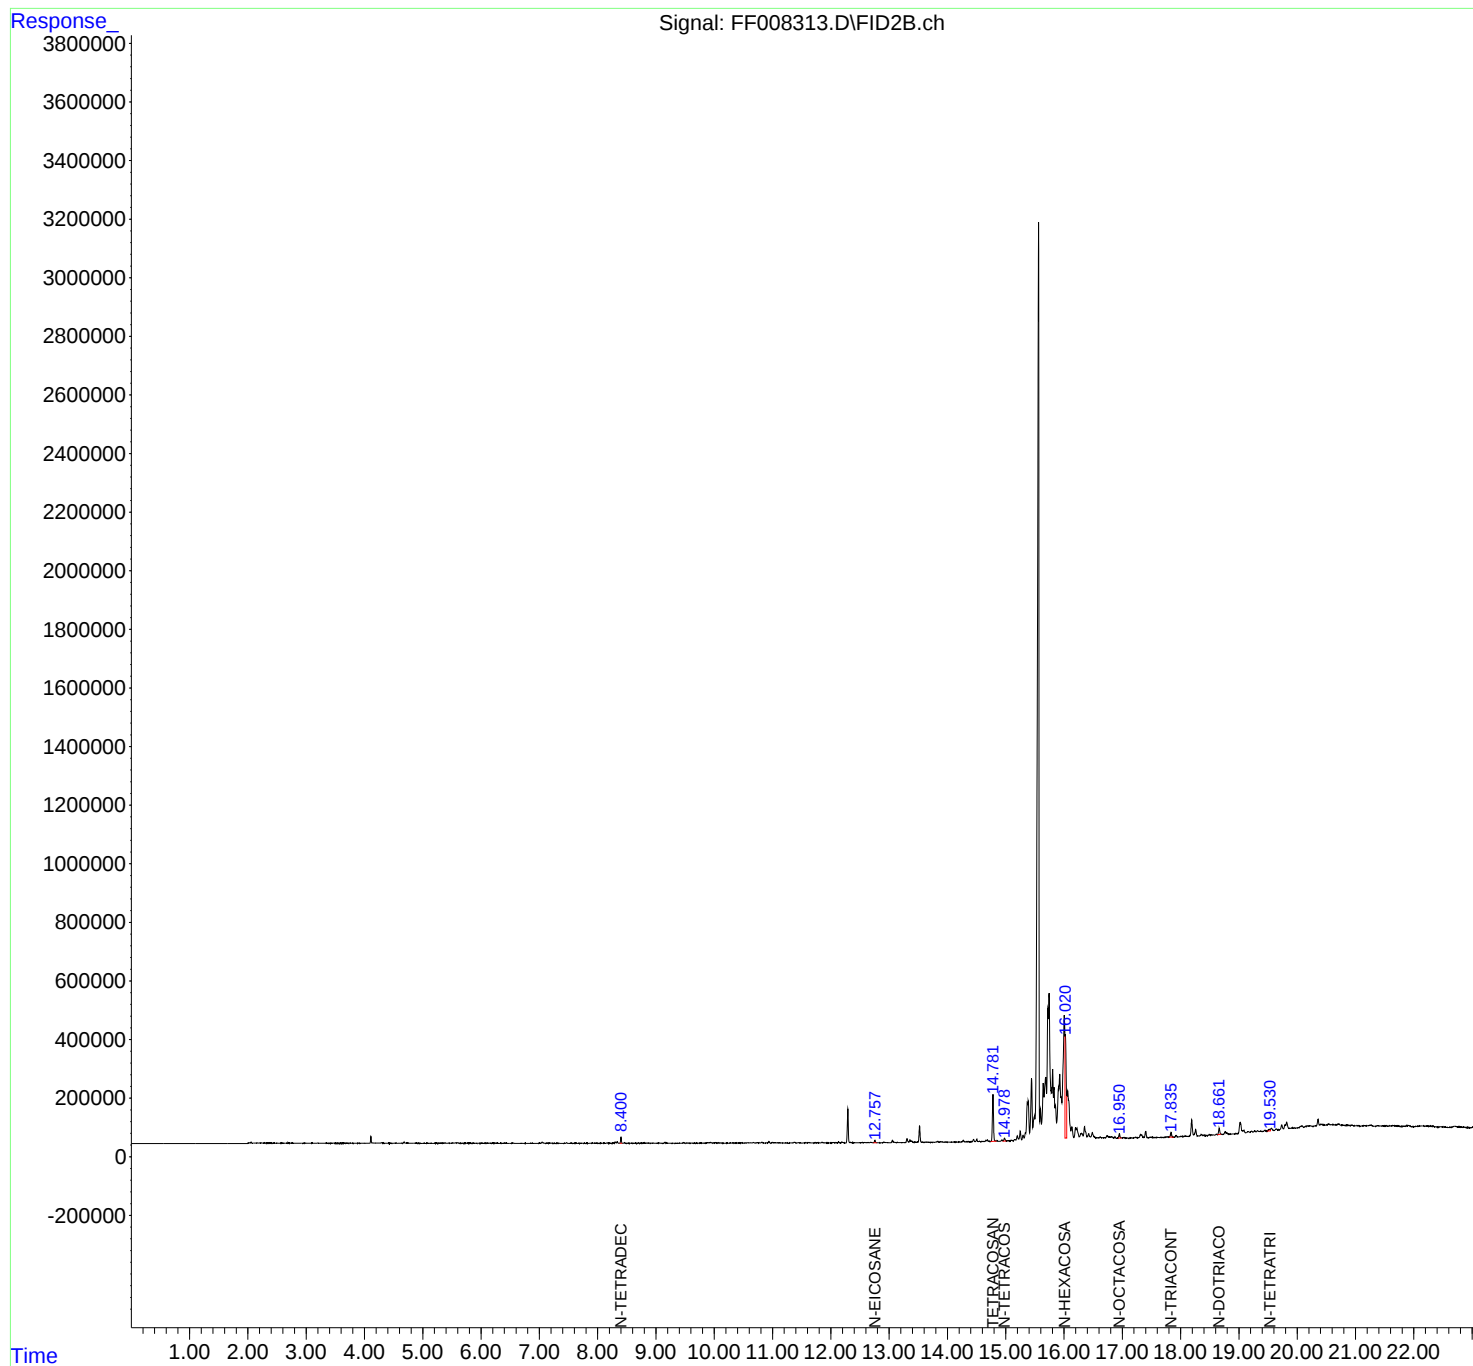


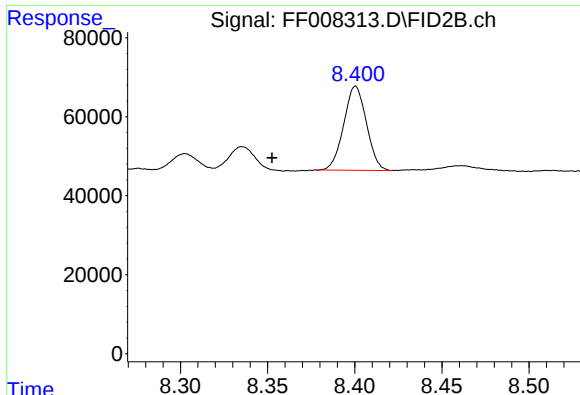

#4 N-TETRADECANE


R.T.: 8.401 min
Delta R.T.: 0.048 min
Response: 193260
Conc: 1.49 ug/ml

Instrument :
FID_F
ClientSampleId :

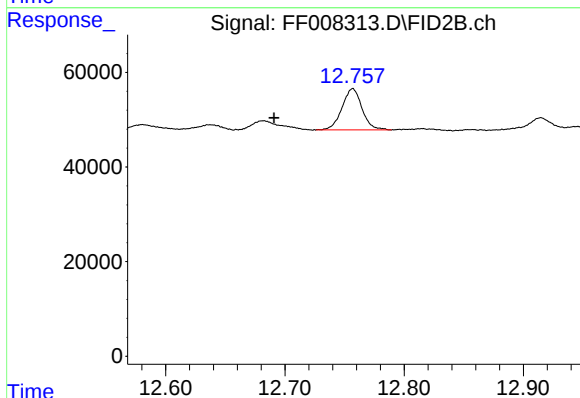


#7 N-EICOSANE

R.T.: 12.757 min
Delta R.T.: 0.066 min
Response: 101218
Conc: 0.80 ug/ml

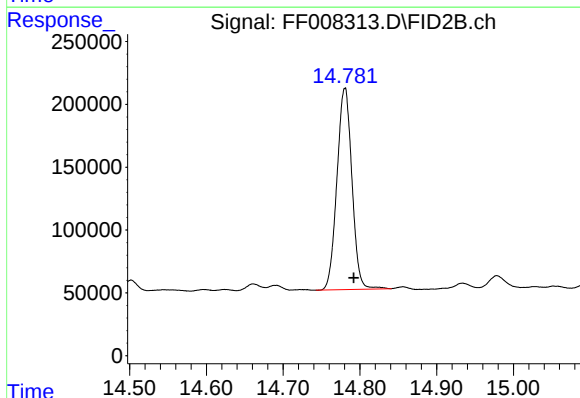


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.781 min
Delta R.T.: -0.011 min
Response: 2177304
Conc: 19.84 ug/ml

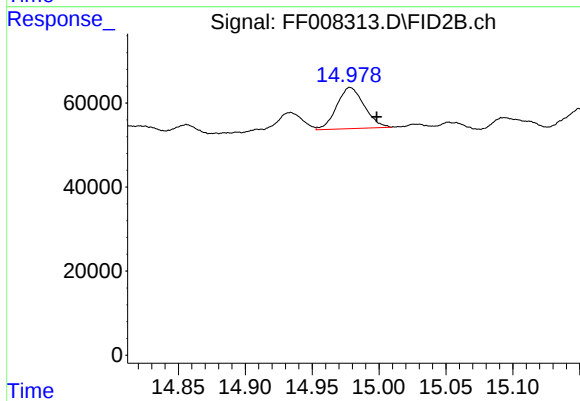

#10 N-TETRACOSANE


R.T.: 14.978 min
Delta R.T.: -0.020 min
Response: 141013
Conc: 1.13 ug/ml

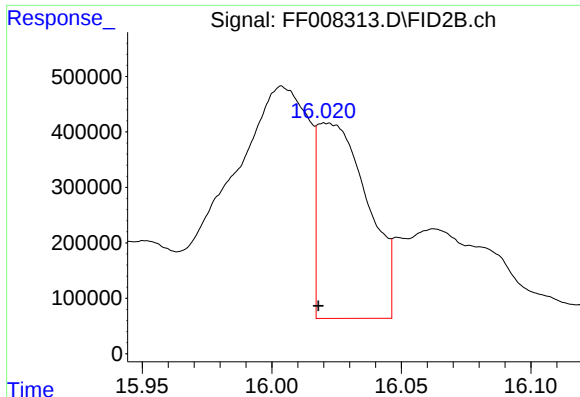

#11 N-HEXACOSANE


R.T.: 16.020 min
Delta R.T.: 0.002 min
Response: 4733090
Conc: 38.67 ug/ml

Instrument :
FID_F
ClientSampleId :

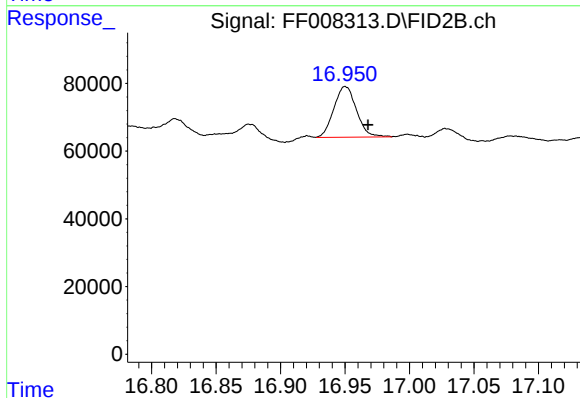


#12 N-OCTACOSANE

R.T.: 16.950 min
Delta R.T.: -0.018 min
Response: 182259
Conc: 1.49 ug/ml

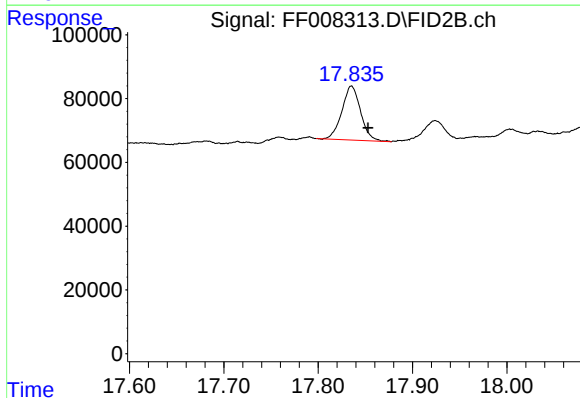


#13 N-TRIACONTANE

R.T.: 17.835 min
Delta R.T.: -0.017 min
Response: 233909
Conc: 1.91 ug/ml

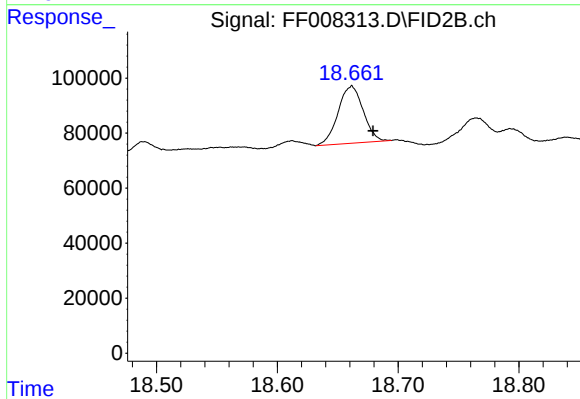

#14 N-DOTRIACONTANE

R.T.: 18.662 min
Delta R.T.: -0.018 min
Response: 299824
Conc: 2.47 ug/ml

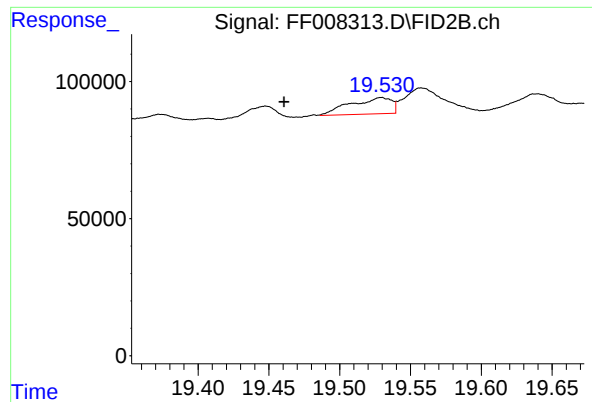

#15 N-TETRATRIACONTANE

R.T.: 19.530 min
Delta R.T.: 0.069 min
Response: 120105
Conc: 1.06 ug/ml

Instrument :
FID_F
ClientSampleId :