

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042219\
 Data File : FF004293.D
 Signal(s) : FID2B.ch
 Acq On : 22 Apr 2019 14:51
 Operator : AJ\SJ
 Sample : K2465-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 Q-COMP-4.18.19

Integration File: autoint1.e
 Quant Time: Apr 22 21:51:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.531	1588255	12.217 ug/ml
Target Compounds			
4) N-TETRADECANE	8.153	197623	1.390 ug/ml
10) N-TETRACOSANE	14.734	312425	2.121 ug/ml
11) N-HEXACOSANE	15.755	331851	2.286 ug/ml
12) N-OCTACOSANE	16.709	369636	2.571 ug/ml
13) N-TRIACONTANE	17.596	345229	2.417 ug/ml
14) N-DOTRIACONTANE	18.431	251409	1.781 ug/ml
15) N-TETRATRIACONTANE	19.241	117194	0.879 ug/ml
16) N-HEXATRIACONTANE	19.973	144562	1.139 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042219\
Data File : FF004293.D
Signal(s) : FID2B.ch
Acq On : 22 Apr 2019 14:51
Operator : AJ\SJ
Sample : K2465-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
Q-COMP-4.18.19

Integration File: autoint1.e
Quant Time: Apr 22 21:51:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

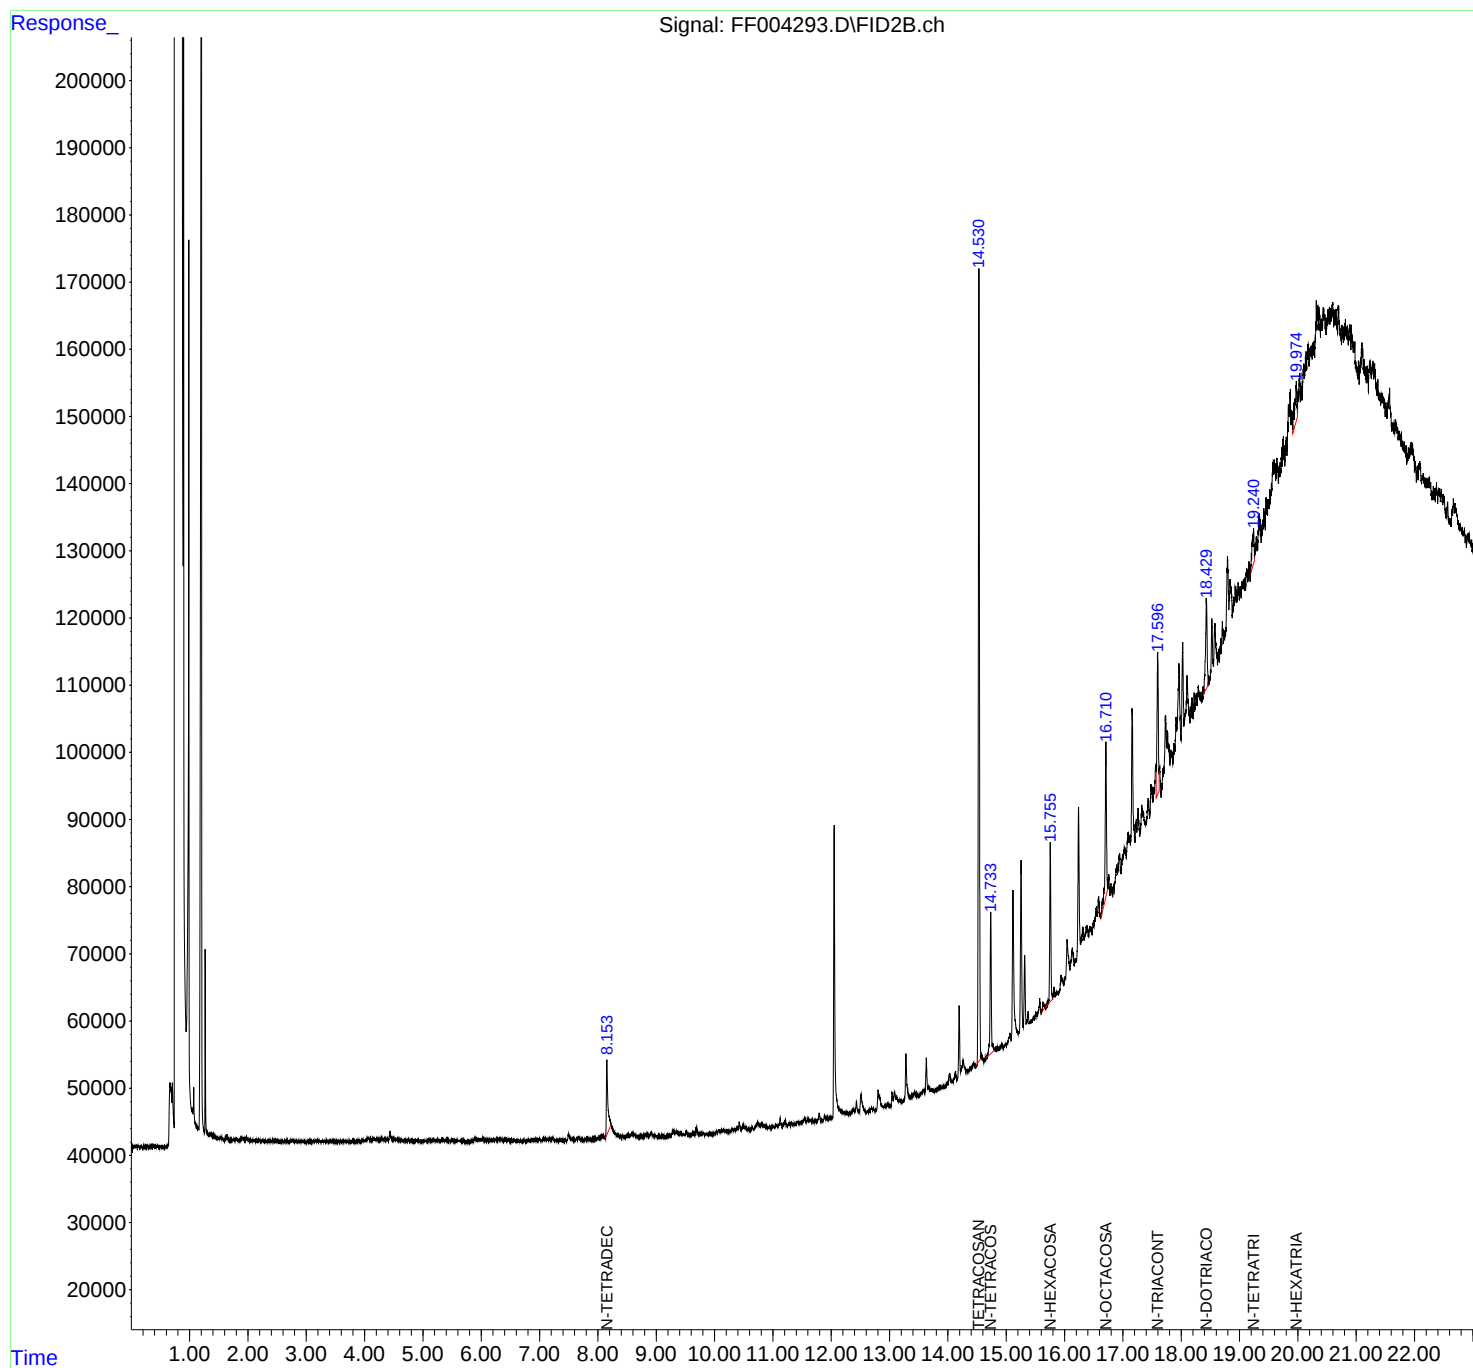


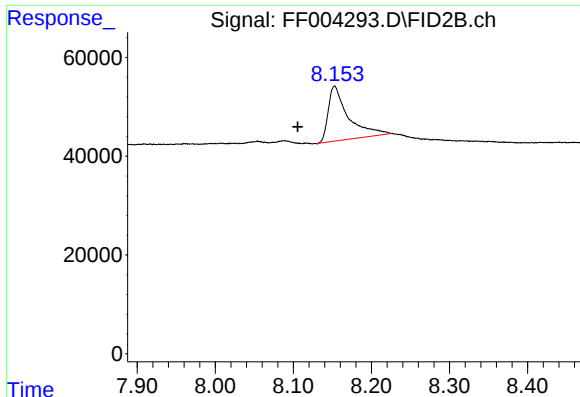

#4 N-TETRADECANE


R.T.: 8.153 min
Delta R.T.: 0.047 min
Response: 197623
Conc: 1.39 ug/ml

Instrument :
FID_F
ClientSampleId :
Q-COMP-4.18.19

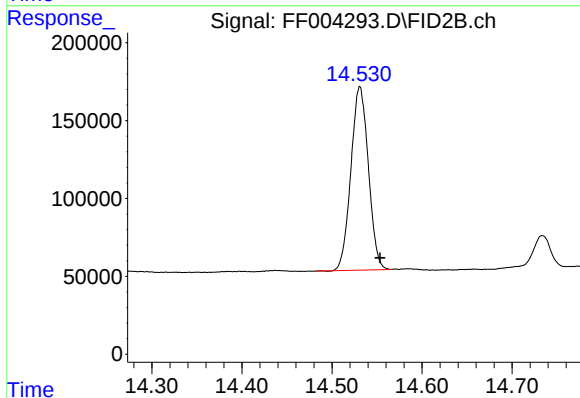


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.531 min
Delta R.T.: -0.022 min
Response: 1588255
Conc: 12.22 ug/ml

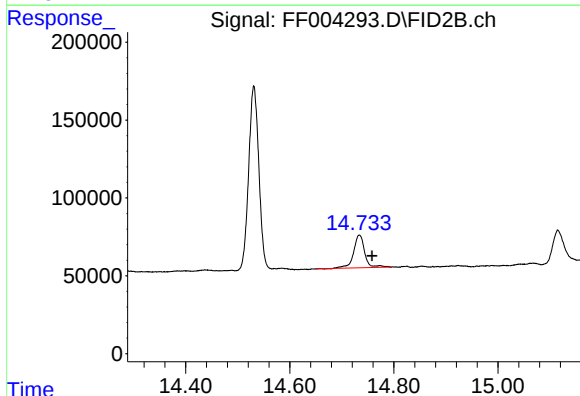


#10 N-TETRACOSANE

R.T.: 14.734 min
Delta R.T.: -0.024 min
Response: 312425
Conc: 2.12 ug/ml

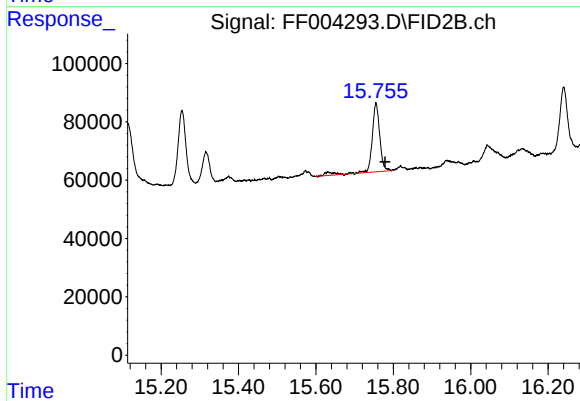

#11 N-HEXACOSANE


R.T.: 15.755 min
Delta R.T.: -0.023 min
Response: 331851
Conc: 2.29 ug/ml

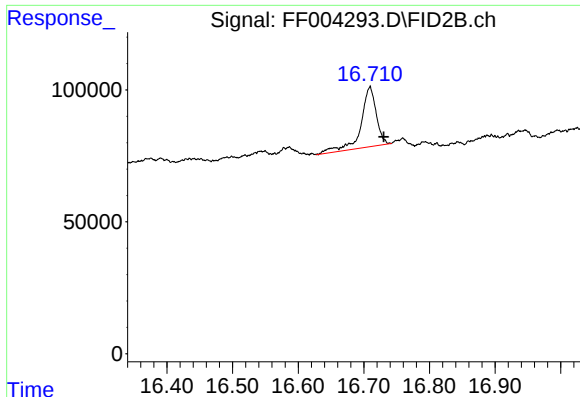

#12 N-OCTACOSANE


R.T.: 16.709 min
Delta R.T.: -0.021 min
Response: 369636
Conc: 2.57 ug/ml

Instrument :
FID_F
ClientSampleId :
Q-COMP-4.18.19

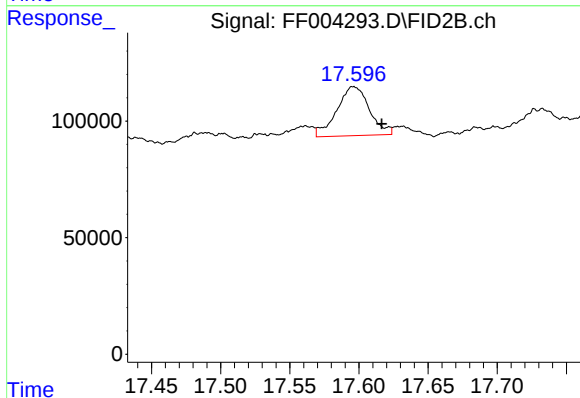


#13 N-TRIACONTANE

R.T.: 17.596 min
Delta R.T.: -0.020 min
Response: 345229
Conc: 2.42 ug/ml

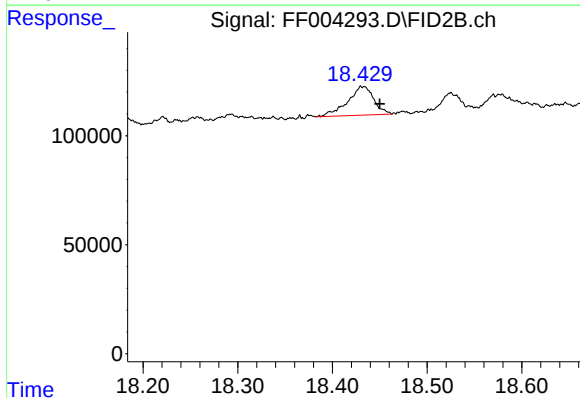


#14 N-DOTRIACONTANE

R.T.: 18.431 min
Delta R.T.: -0.019 min
Response: 251409
Conc: 1.78 ug/ml

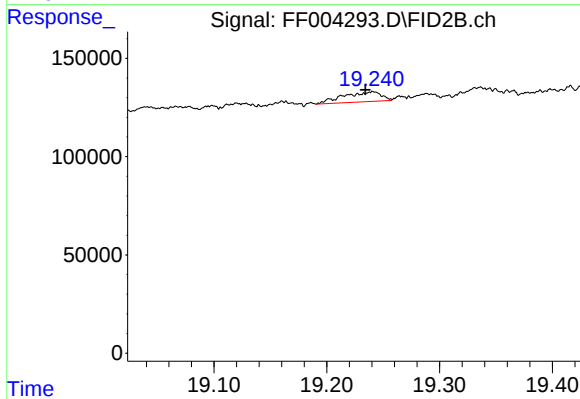

#15 N-TETRATRIACONTANE

R.T.: 19.241 min
Delta R.T.: 0.007 min
Response: 117194
Conc: 0.88 ug/ml

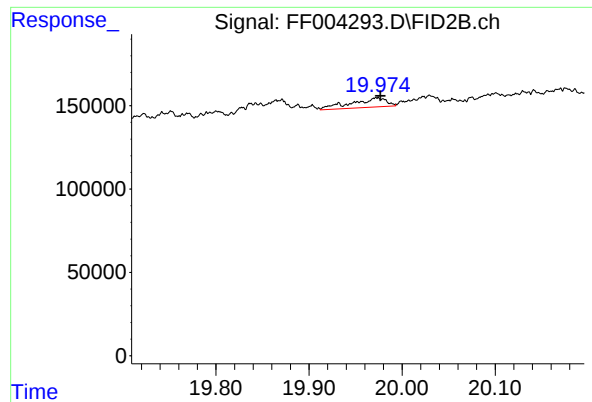

#16 N-HEXATRIACONTANE

R.T.: 19.973 min
Delta R.T.: -0.003 min
Response: 144562
Conc: 1.14 ug/ml

Instrument :
FID_F
ClientSampleId :
Q-COMP-4.18.19