

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042219\
 Data File : FF004305.D
 Signal(s) : FID2B.ch
 Acq On : 22 Apr 2019 20:43
 Operator : AJ\SJ
 Sample : K2464-01 5X
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 M-COMP-4.18.19

Integration File: autoint1.e
 Quant Time: Apr 22 21:54:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.528	470287	3.618 ug/ml
Target Compounds			
7) N-EICOSANE	12.496	554317	3.689 ug/ml
10) N-TETRACOSANE	14.730	358245	2.432 ug/ml
12) N-OCTACOSANE	16.703	93464	0.650 ug/ml
13) N-TRIACONTANE	17.590	128669	0.901 ug/ml
14) N-DOTRIACONTANE	18.429	135147	0.957 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042219\
Data File : FF004305.D
Signal(s) : FID2B.ch
Acq On : 22 Apr 2019 20:43
Operator : AJ\SJ
Sample : K2464-01 5X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
M-COMP-4.18.19

Integration File: autoint1.e
Quant Time: Apr 22 21:54:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

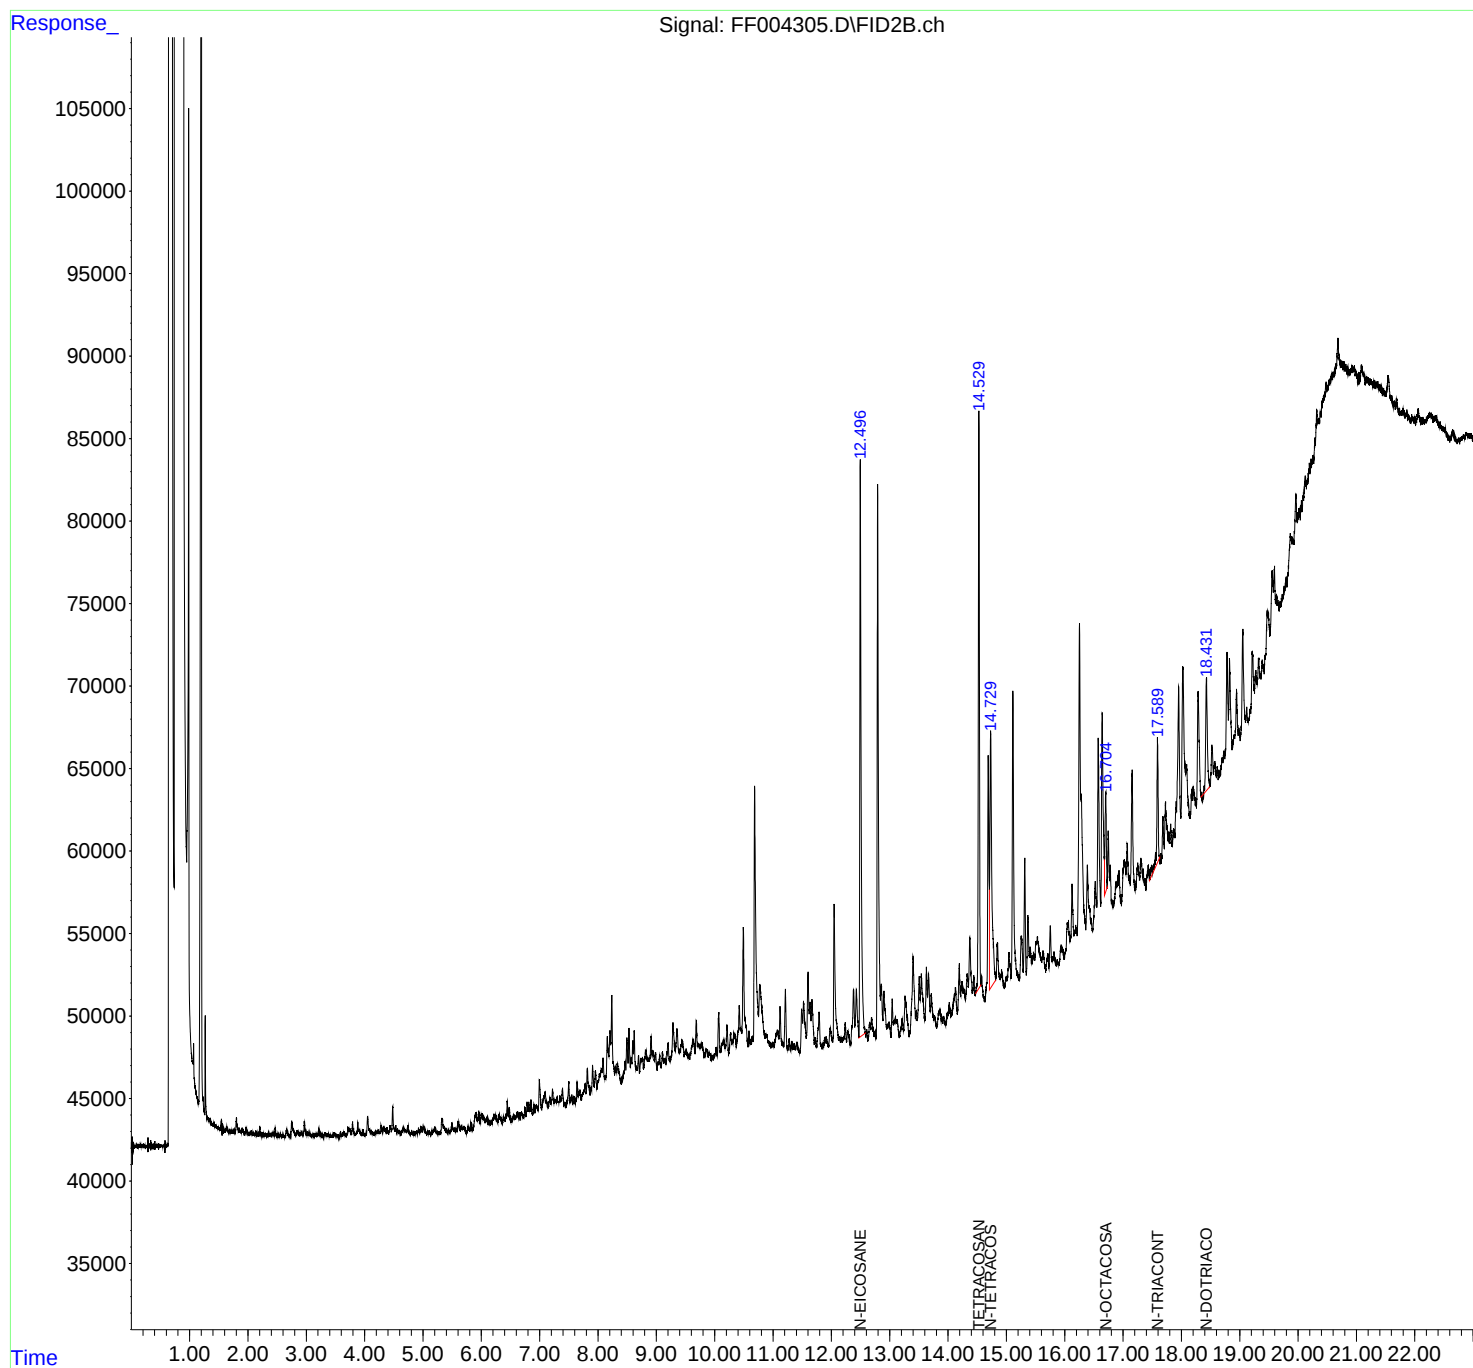


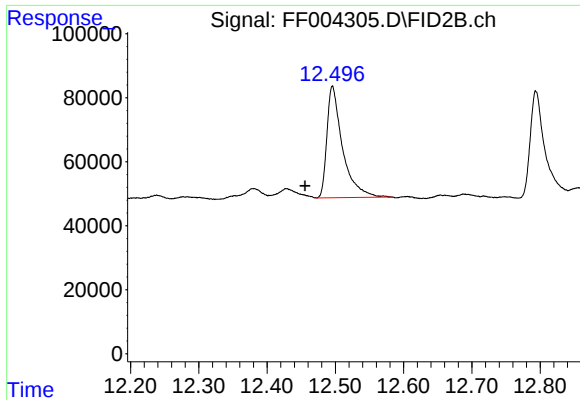

#7 N-EICOSANE


R.T.: 12.496 min
Delta R.T.: 0.040 min
Response: 554317
Conc: 3.69 ug/ml

Instrument :
FID_F
ClientSampleId :
M-COMP-4.18.19

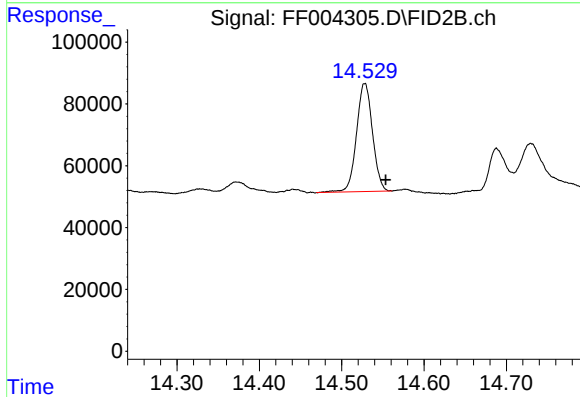


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.528 min
Delta R.T.: -0.025 min
Response: 470287
Conc: 3.62 ug/ml

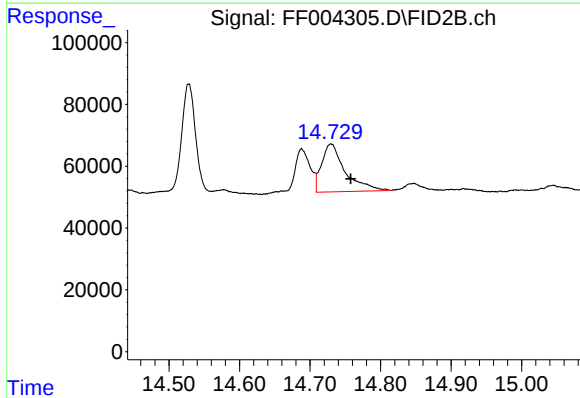


#10 N-TETRACOSANE

R.T.: 14.730 min
Delta R.T.: -0.028 min
Response: 358245
Conc: 2.43 ug/ml

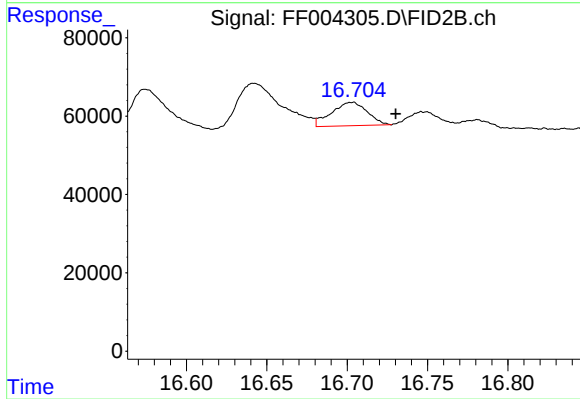

#12 N-OCTACOSANE


R.T.: 16.703 min
Delta R.T.: -0.027 min
Response: 93464
Conc: 0.65 ug/ml

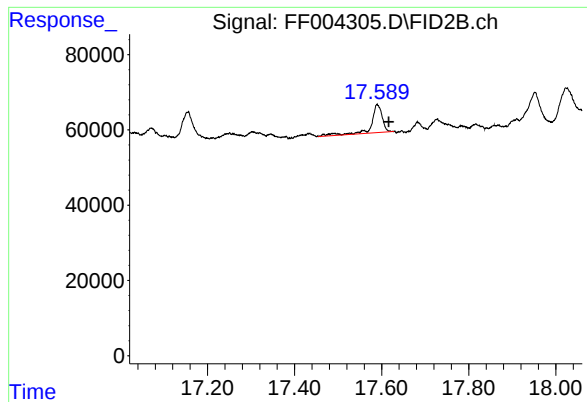

#13 N-TRIACONTANE

R.T.: 17.590 min
Delta R.T.: -0.027 min
Response: 128669
Conc: 0.90 ug/ml

Instrument :
FID_F
ClientSampleId :
M-COMP-4.18.19

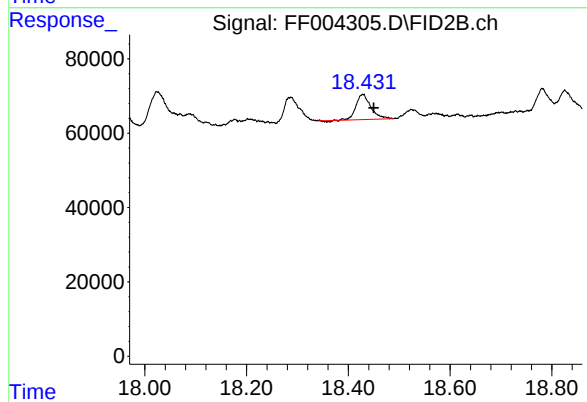

#14 N-DOTRIACONTANE

R.T.: 18.429 min
Delta R.T.: -0.021 min
Response: 135147
Conc: 0.96 ug/ml