

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042219\
Data File : FF004292.D
Signal(s) : FID2B.ch
Acq On : 22 Apr 2019 14:21
Operator : AJ\SJ
Sample : K2464-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
M-COMP-4.18.19

Integration File: autoint1.e
Quant Time: Apr 22 21:50:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.534	2393016	18.408 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042219\
Data File : FF04292.D
Signal(s) : FID2B.ch
Acq On : 22 Apr 2019 14:21
Operator : AJ\SJ
Sample : K2464-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
M-COMP-4.18.19

Integration File: autoint1.e
Quant Time: Apr 22 21:50:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

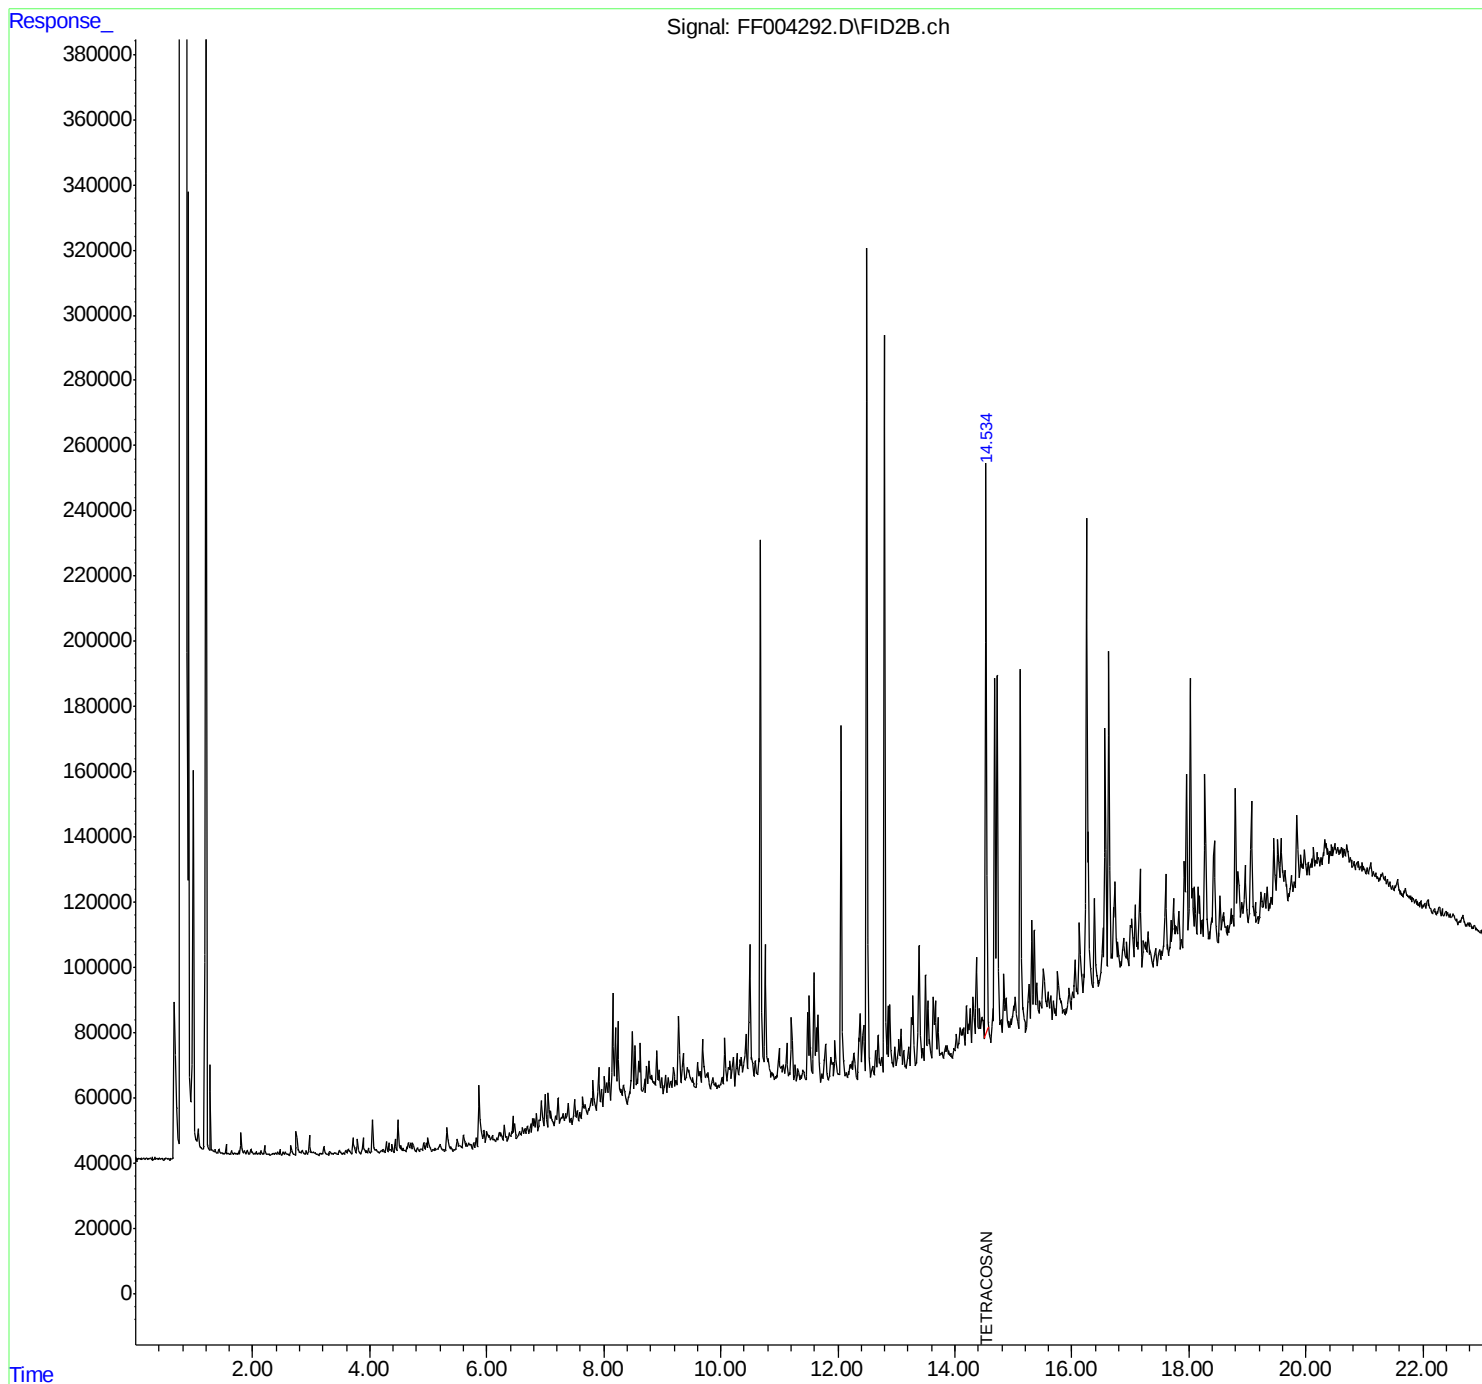

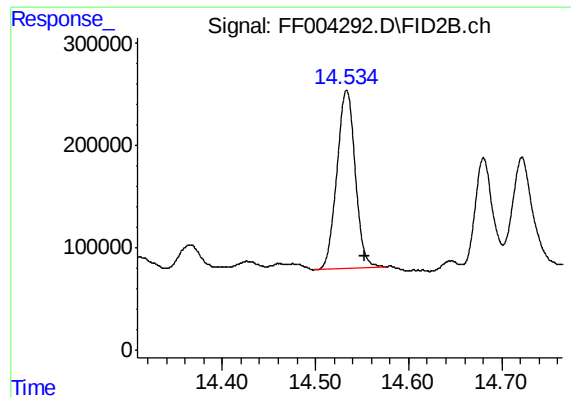

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.534 min
Delta R.T.: -0.020 min
Response: 2393016
Conc: 18.41 ug/ml

Instrument :
FID_F
ClientSampleId :
M-COMP-4.18.19