

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042221\
 Data File : FF008323.D
 Signal(s) : FID2B.ch
 Acq On : 22 Apr 2021 10:43
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 23 01:30:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
 Quant Title :
 QLast Update : Tue Apr 06 02:37:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.778	2154935	19.638 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.833	90456	0.740 ug/ml
14) N-DOTRIACONTANE	18.664	133694	1.102 ug/ml
15) N-TETRATRIACONTANE	19.443	88937	0.786 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042221\
Data File : FF008323.D
Signal(s) : FID2B.ch
Acq On : 22 Apr 2021 10:43
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 23 01:30:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
Quant Title :
QLast Update : Tue Apr 06 02:37:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

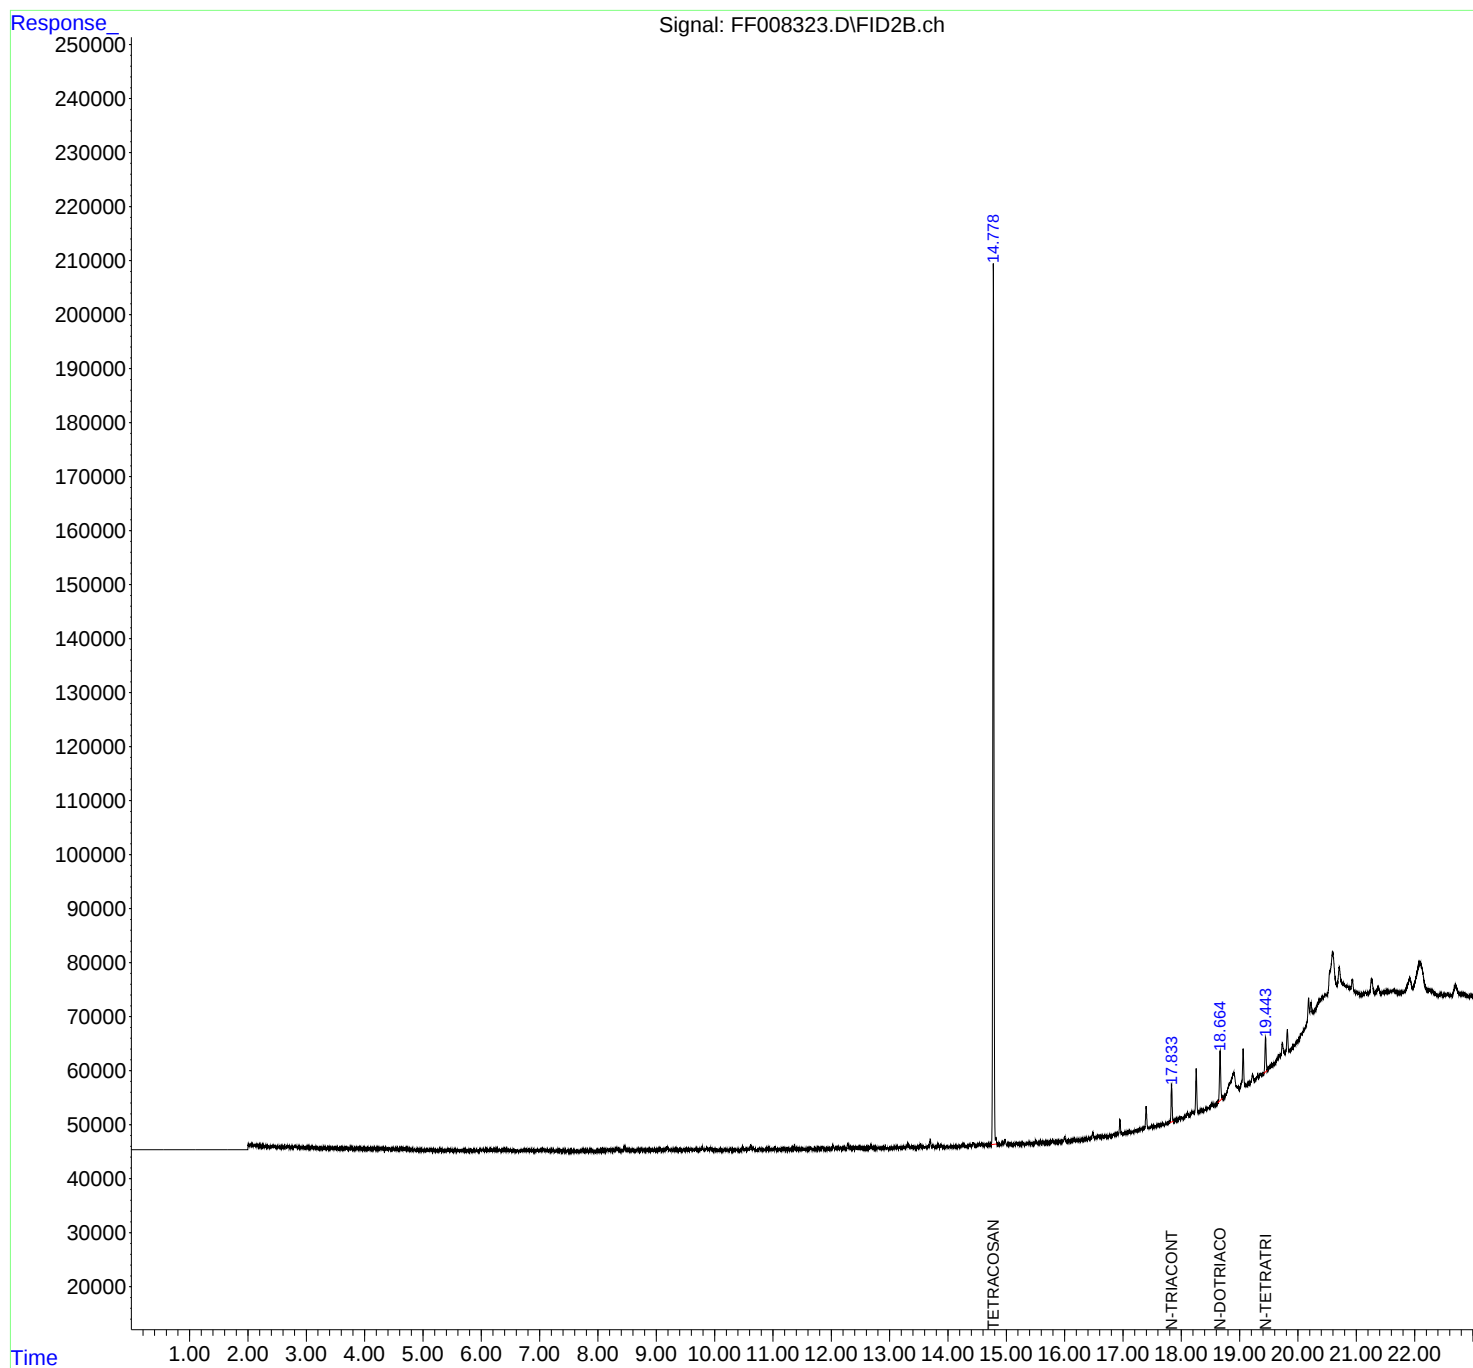


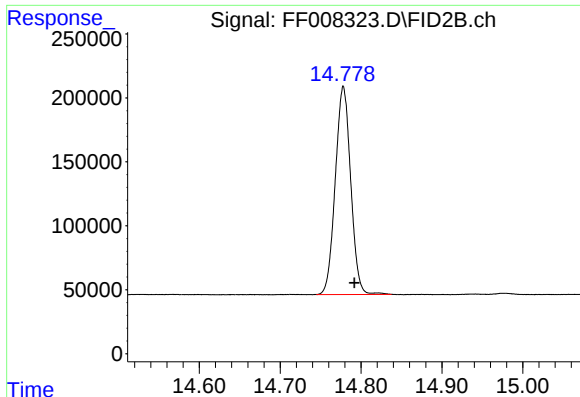

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.778 min
Delta R.T.: -0.014 min
Response: 2154935
Conc: 19.64 ug/ml

Instrument :
FID_F
ClientSampleId :

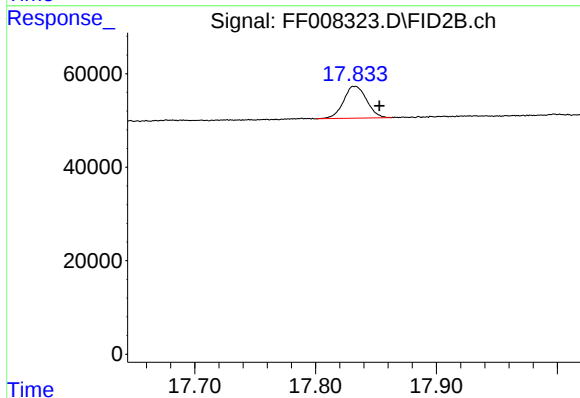


#13 N-TRIACONTANE

R.T.: 17.833 min
Delta R.T.: -0.020 min
Response: 90456
Conc: 0.74 ug/ml

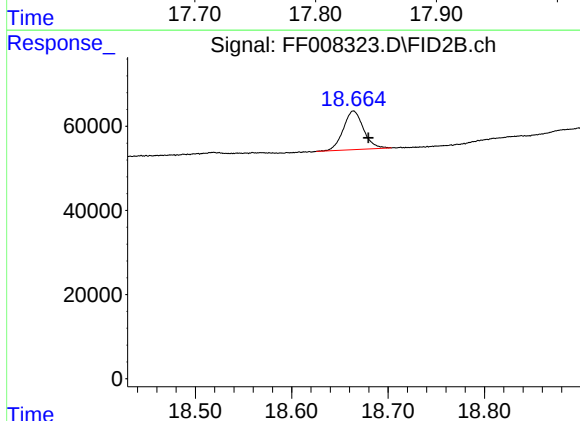

#14 N-DOTRIACONTANE

R.T.: 18.664 min
Delta R.T.: -0.015 min
Response: 133694
Conc: 1.10 ug/ml

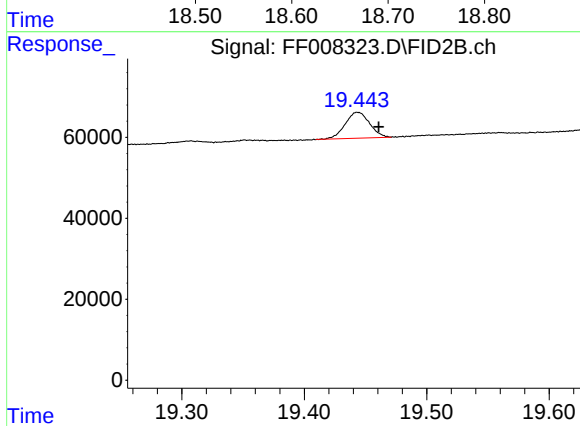

#15 N-TETRATRIACONTANE

R.T.: 19.443 min
Delta R.T.: -0.018 min
Response: 88937
Conc: 0.79 ug/ml