

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042221\
 Data File : FF008332.D
 Signal(s) : FID2B.ch
 Acq On : 22 Apr 2021 19:25
 Operator : DD\AJ
 Sample : M2107-18 2X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 23 01:45:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
 Quant Title :
 QLast Update : Tue Apr 06 02:37:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.778	773355	7.047 ug/ml
Target Compounds			
7) N-EICOSANE	12.755f	243062	1.910 ug/ml
10) N-TETRACOSANE	14.977	181816	1.459 ug/ml
11) N-HEXACOSANE	16.001	91946	0.751 ug/ml
12) N-OCTACOSANE	16.950	131819	1.080 ug/ml
13) N-TRIACONTANE	17.834	220662	1.806 ug/ml
14) N-DOTRIACONTANE	18.662	194347	1.602 ug/ml
15) N-TETRATRIACONTANE	19.443	111234	0.983 ug/ml
16) N-HEXATRIACONTANE	20.181	76847	0.747 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042221\
Data File : FF008332.D
Signal(s) : FID2B.ch
Acq On : 22 Apr 2021 19:25
Operator : DD\AJ
Sample : M2107-18 2X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Apr 23 01:45:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
Quant Title :
QLast Update : Tue Apr 06 02:37:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

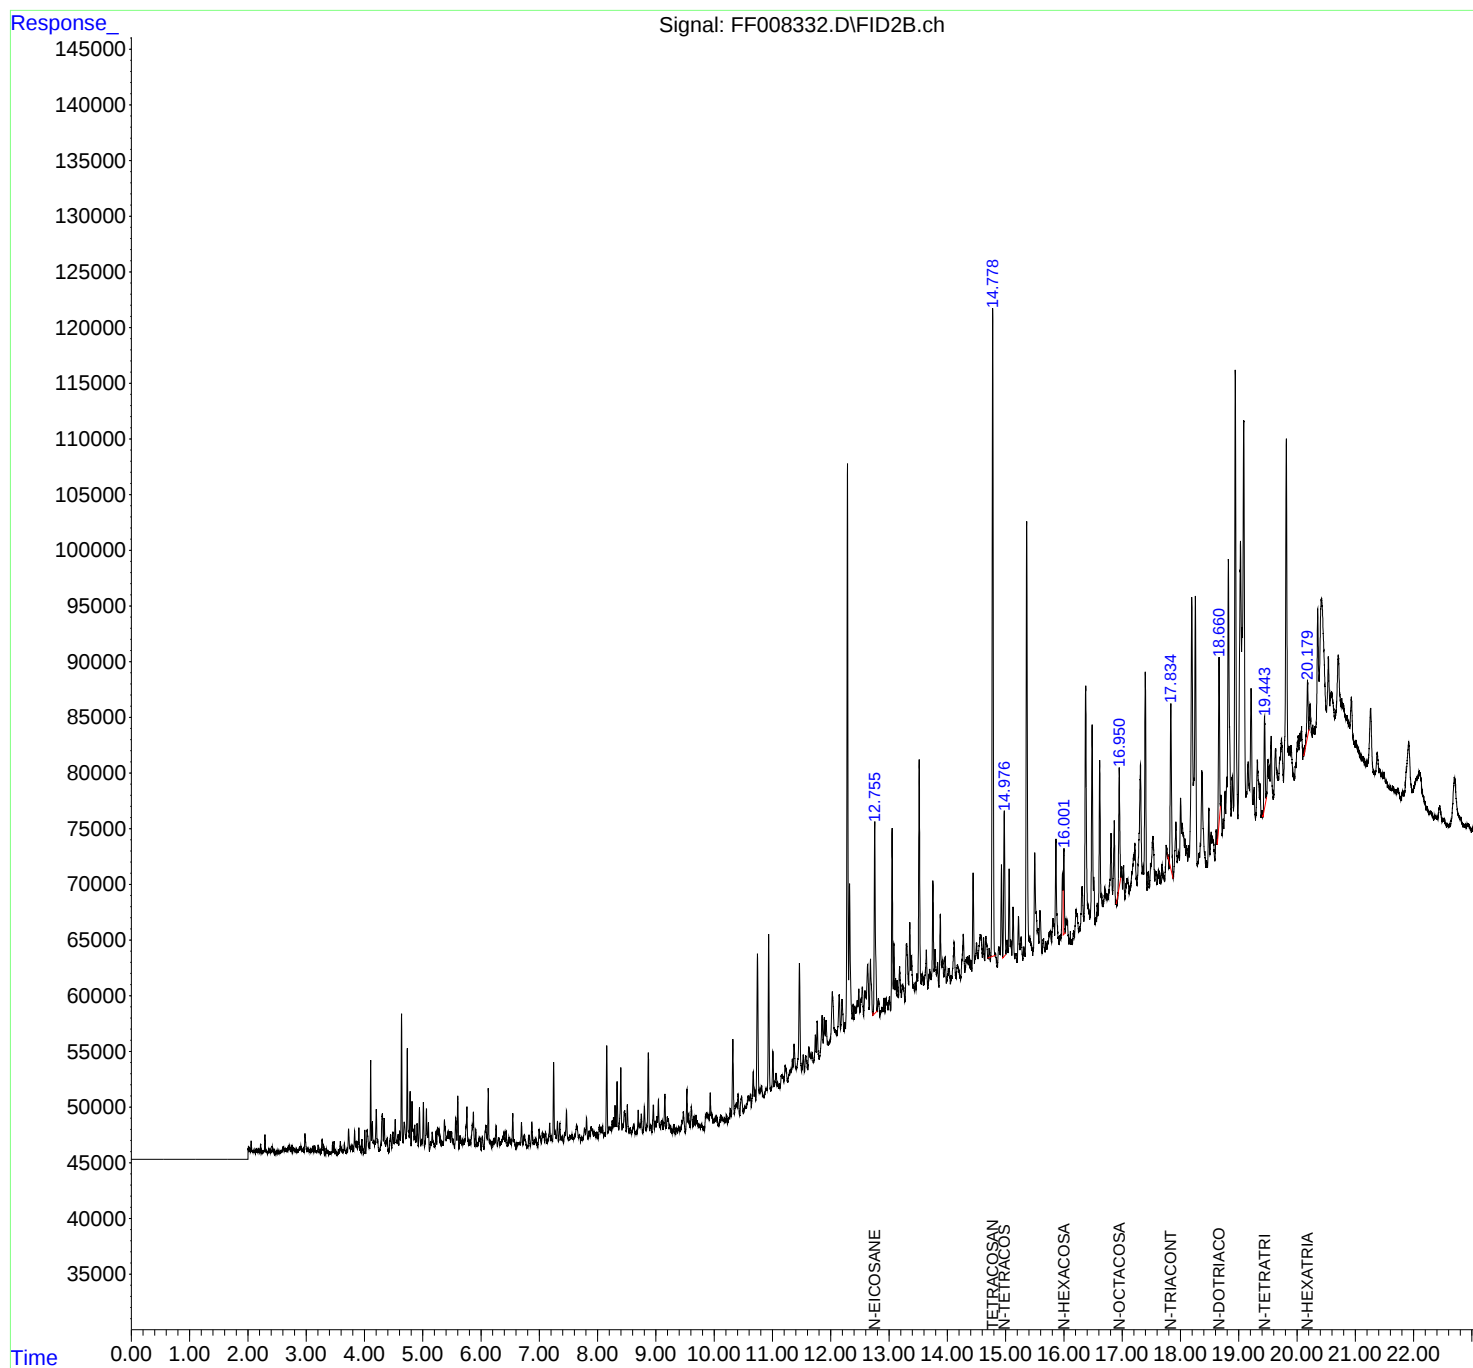


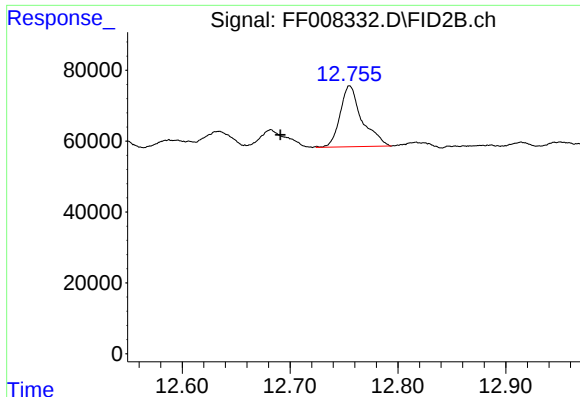

#7 N-EICOSANE


R.T.: 12.755 min
Delta R.T.: 0.065 min
Response: 243062
Conc: 1.91 ug/ml

Instrument :
FID_F
ClientSampleId :

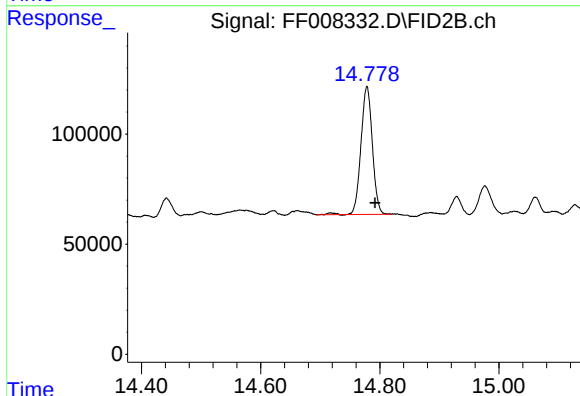


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.778 min
Delta R.T.: -0.013 min
Response: 773355
Conc: 7.05 ug/ml

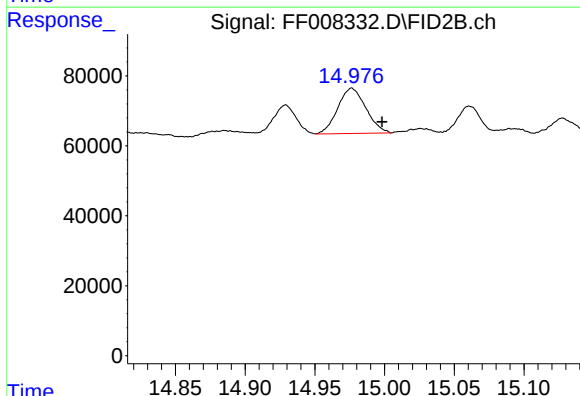


#10 N-TETRACOSANE

R.T.: 14.977 min
Delta R.T.: -0.022 min
Response: 181816
Conc: 1.46 ug/ml

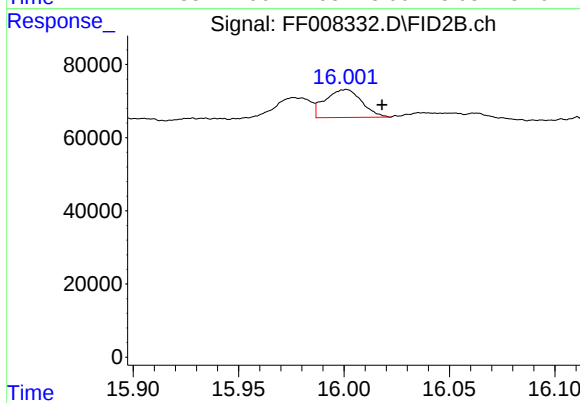

#11 N-HEXACOSANE


R.T.: 16.001 min
Delta R.T.: -0.017 min
Response: 91946
Conc: 0.75 ug/ml

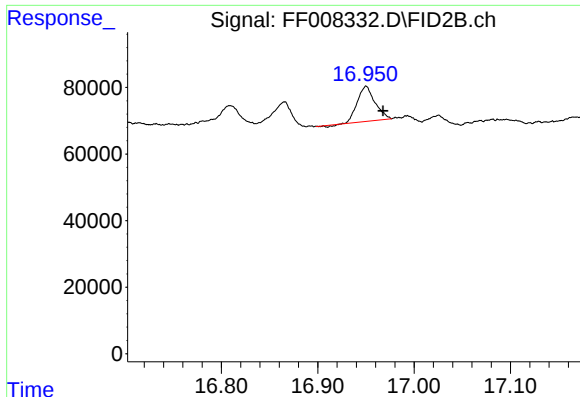

#12 N-OCTACOSANE


R.T.: 16.950 min
Delta R.T.: -0.018 min
Response: 131819
Conc: 1.08 ug/ml

Instrument :
FID_F
ClientSampleId :

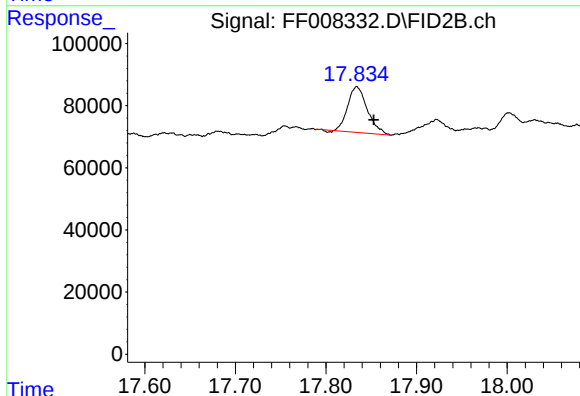


#13 N-TRIACONTANE

R.T.: 17.834 min
Delta R.T.: -0.019 min
Response: 220662
Conc: 1.81 ug/ml

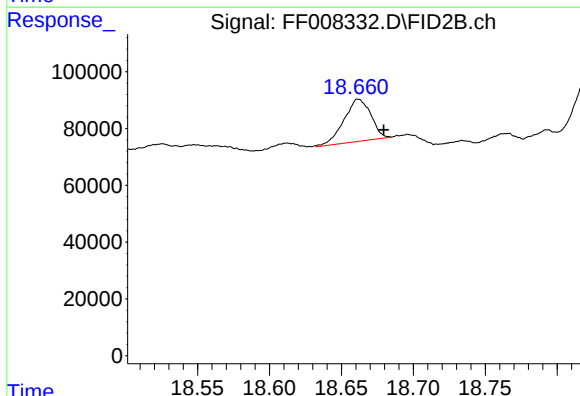


#14 N-DOTRIACONTANE

R.T.: 18.662 min
Delta R.T.: -0.018 min
Response: 194347
Conc: 1.60 ug/ml

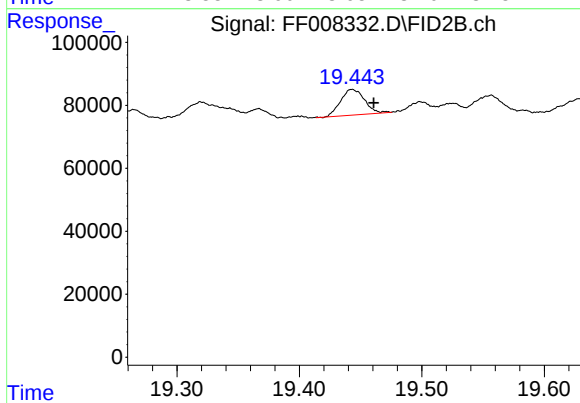

#15 N-TETRATRIACONTANE

R.T.: 19.443 min
Delta R.T.: -0.018 min
Response: 111234
Conc: 0.98 ug/ml

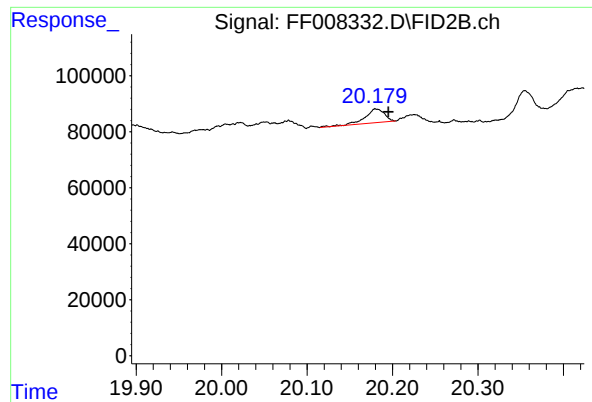

#16 N-HEXATRIACONTANE

R.T.: 20.181 min
Delta R.T.: -0.015 min
Response: 76847
Conc: 0.75 ug/ml

Instrument :
FID_F
ClientSampleId :