

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042221\
Data File : FF008334.D
Signal(s) : FID2B.ch
Acq On : 22 Apr 2021 20:27
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 23 01:45:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
Quant Title :
QLast Update : Tue Apr 06 02:37:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.779	2113089	19.256 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.832	98385	0.805 ug/ml
14) N-DOTRIACONTANE	18.663	165630	1.366 ug/ml
15) N-TETRATRIACONTANE	19.445	98349	0.869 ug/ml
18) N-TETRACONTANE	21.913	279731	3.073 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042221\
Data File : FF008334.D
Signal(s) : FID2B.ch
Acq On : 22 Apr 2021 20:27
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 23 01:45:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
Quant Title :
QLast Update : Tue Apr 06 02:37:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

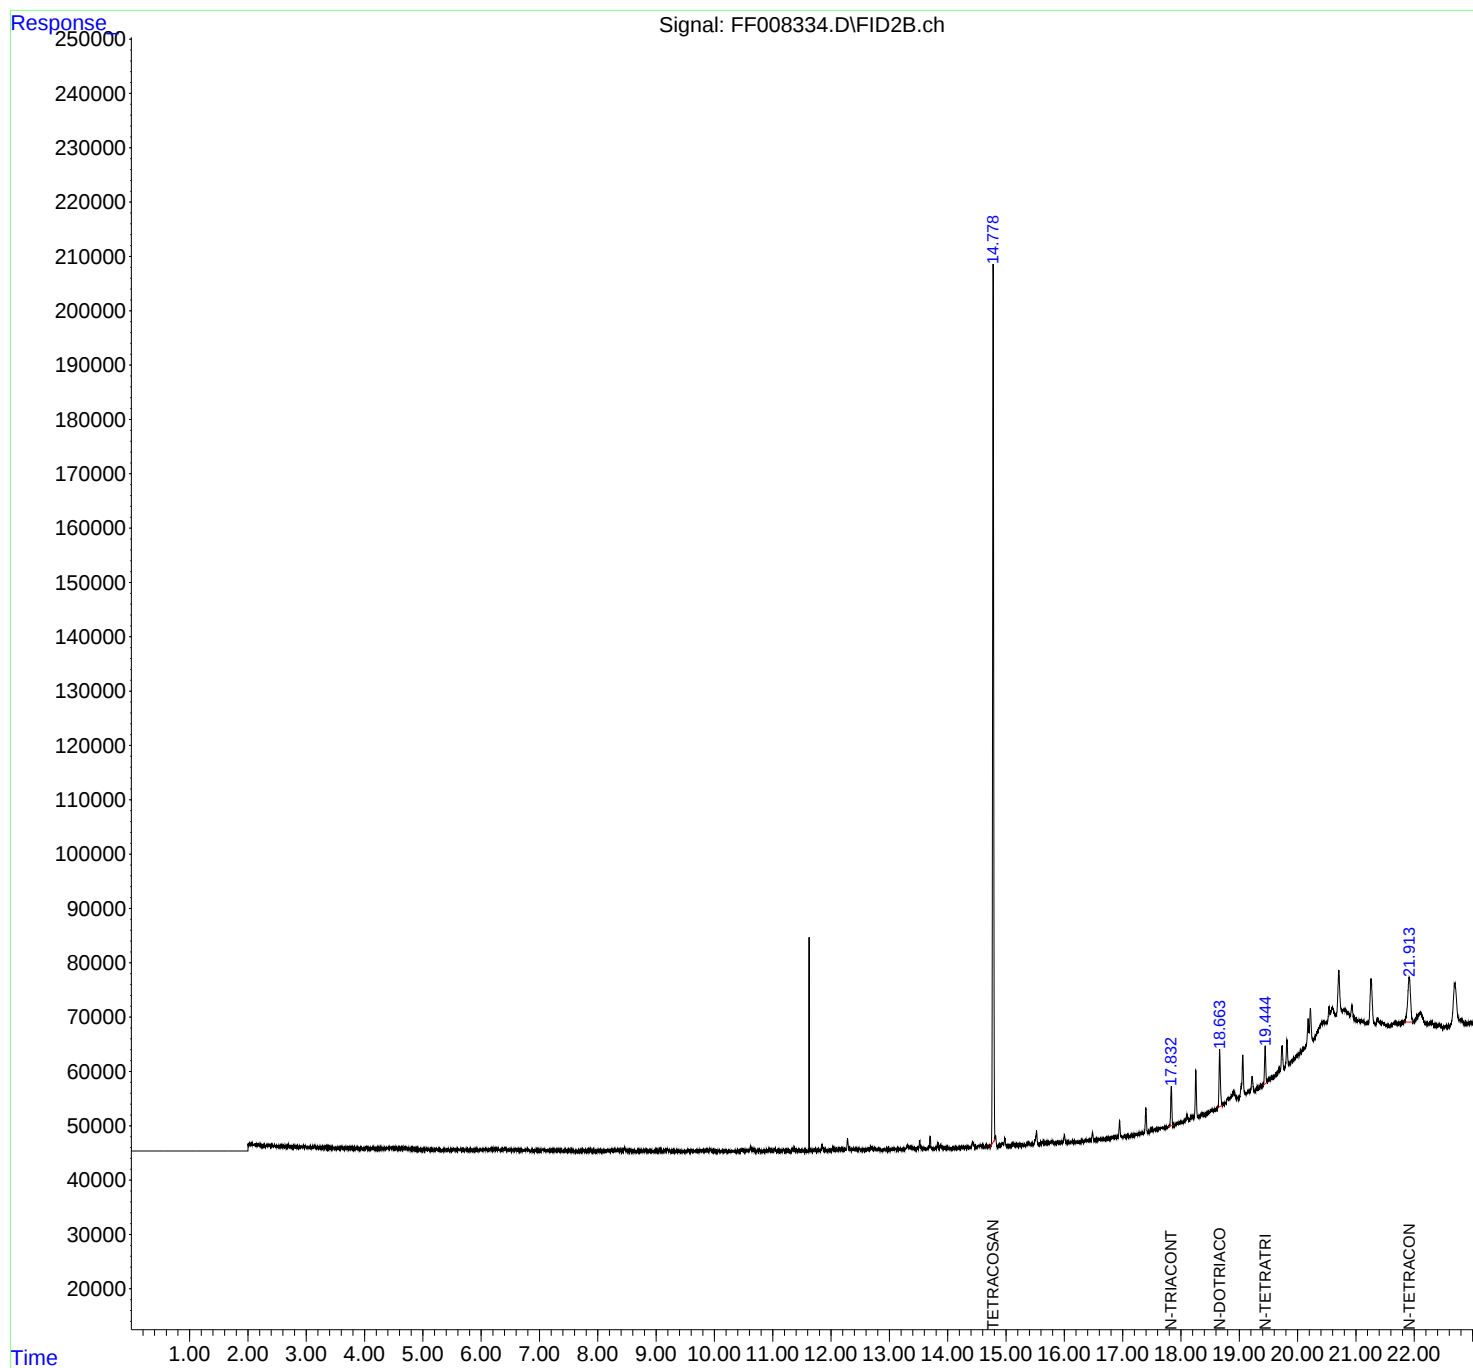


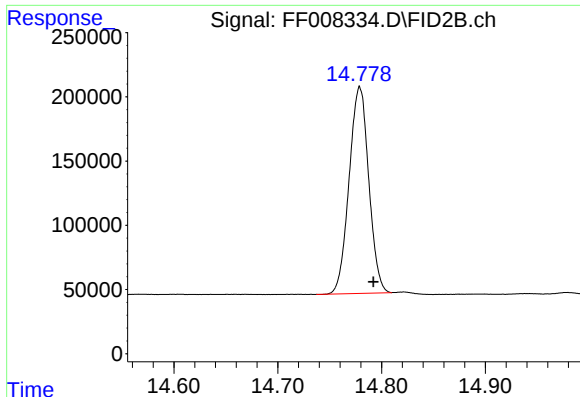

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.779 min
Delta R.T.: -0.013 min
Response: 2113089
Conc: 19.26 ug/ml

Instrument :
FID_F
ClientSampleId :

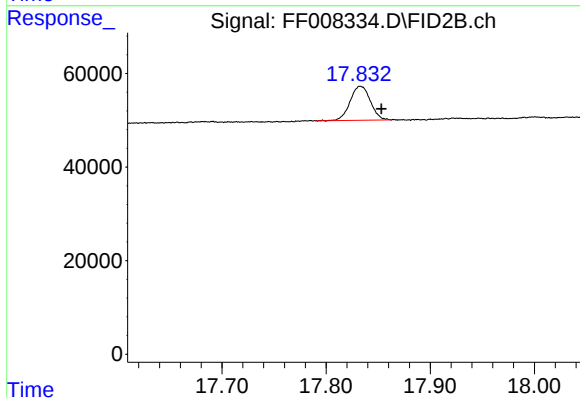


#13 N-TRIACONTANE

R.T.: 17.832 min
Delta R.T.: -0.020 min
Response: 98385
Conc: 0.81 ug/ml

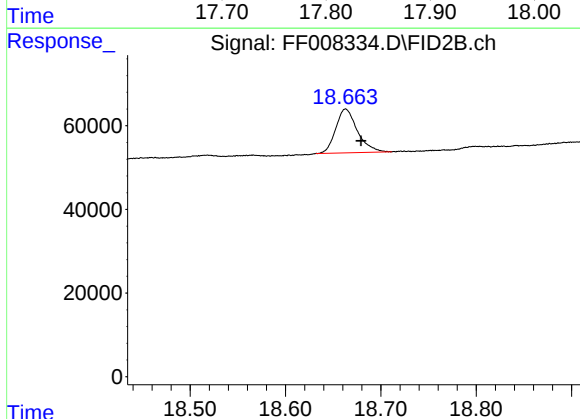


#14 N-DOTRIACONTANE

R.T.: 18.663 min
Delta R.T.: -0.016 min
Response: 165630
Conc: 1.37 ug/ml

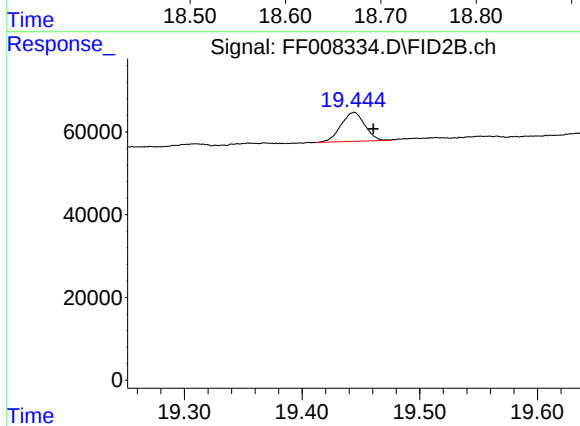

#15 N-TETRATRIACONTANE

R.T.: 19.445 min
Delta R.T.: -0.016 min
Response: 98349
Conc: 0.87 ug/ml

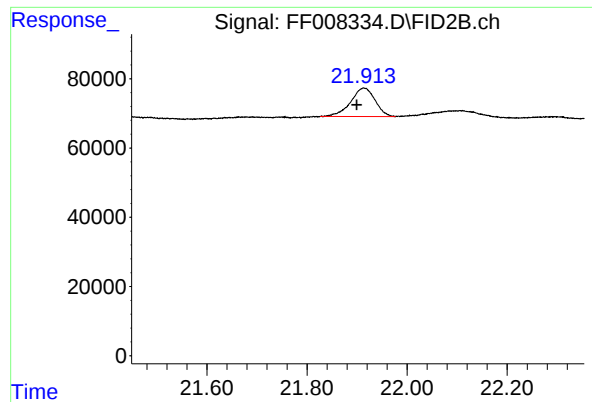

#18 N-TETRACONTANE

R.T.: 21.913 min
Delta R.T.: 0.014 min
Response: 279731
Conc: 3.07 ug/ml

Instrument :
FID_F
ClientSampleId :