

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042221\
Data File : FF008332.D
Signal(s) : FID2B.ch
Acq On : 22 Apr 2021 19:25
Operator : DD\AJ
Sample : M2107-18 2X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-34-COMP

Integration File: autoint1.e
Quant Time: Apr 23 01:45:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
Quant Title :
QLast Update : Tue Apr 06 02:37:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.778	773355	7.047 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042221\
Data File : FF008332.D
Signal(s) : FID2B.ch
Acq On : 22 Apr 2021 19:25
Operator : DD\AJ
Sample : M2107-18 2X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-34-COMP

Integration File: autoint1.e
Quant Time: Apr 23 01:45:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040521.M
Quant Title :
QLast Update : Tue Apr 06 02:37:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

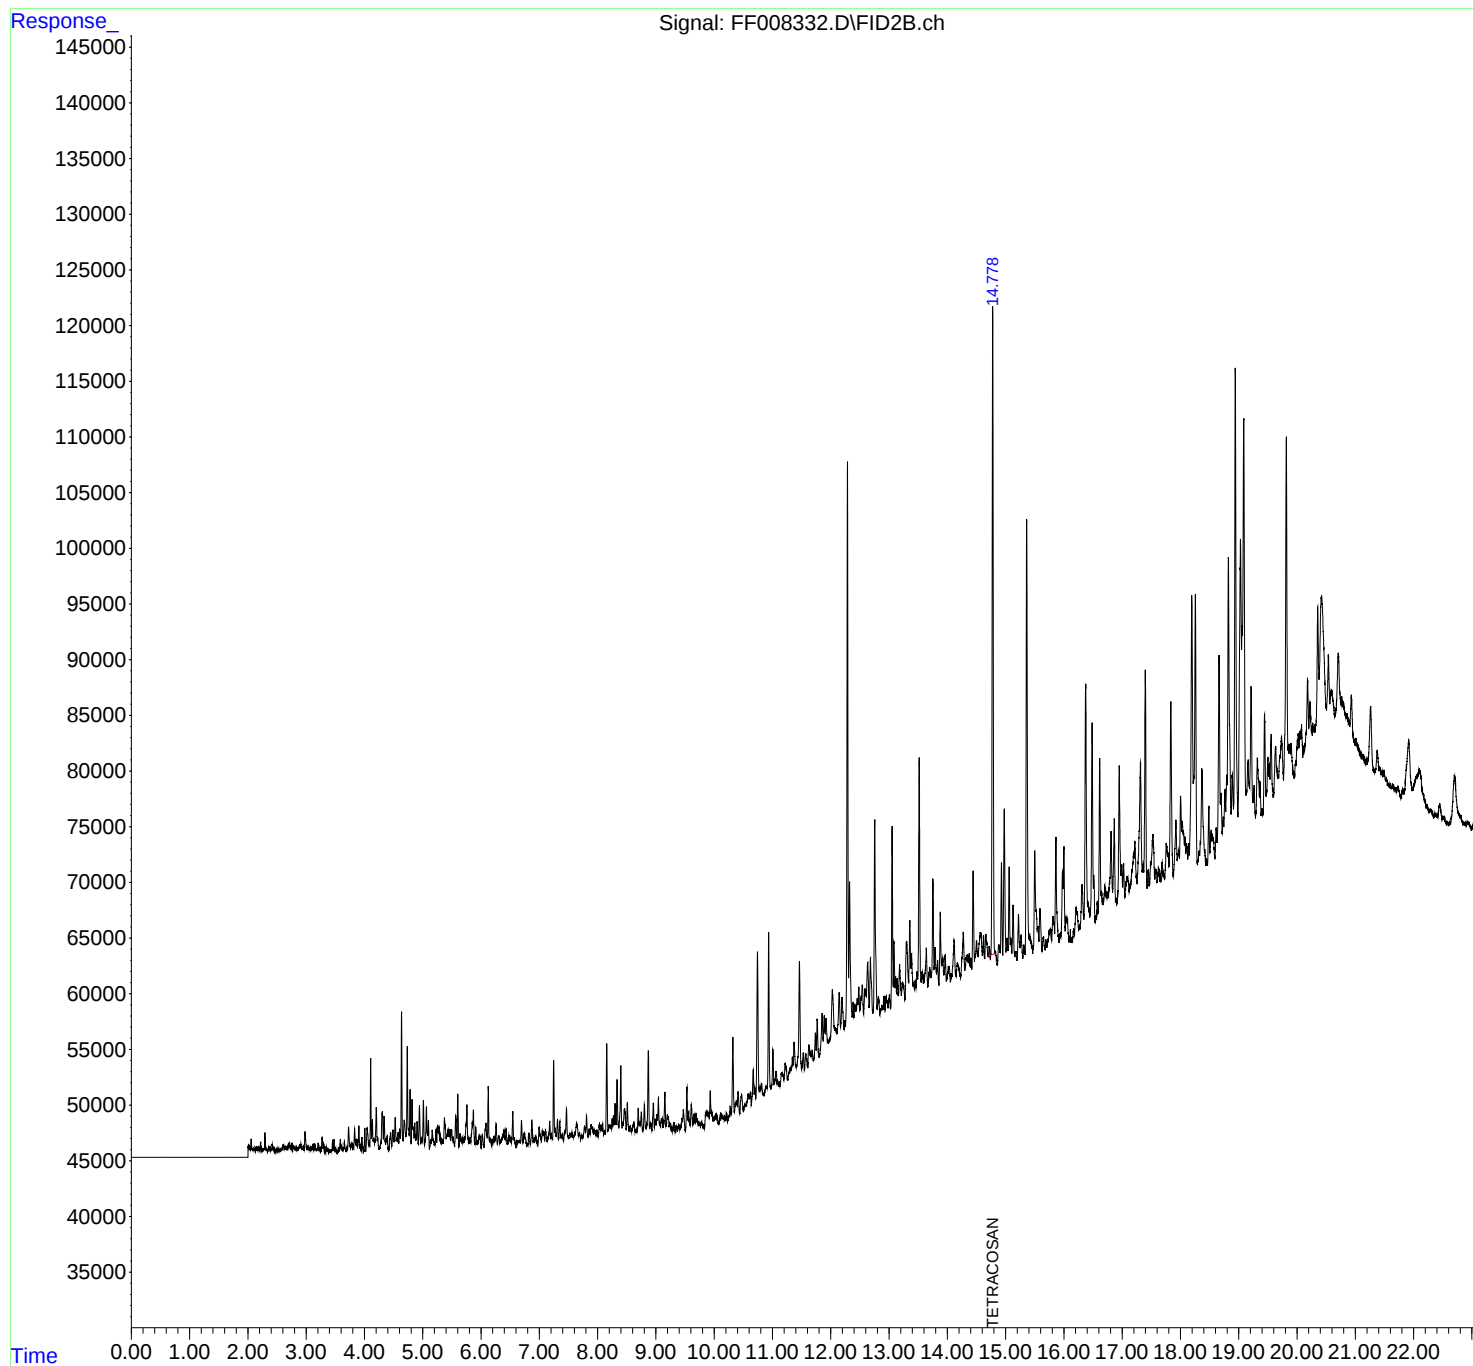

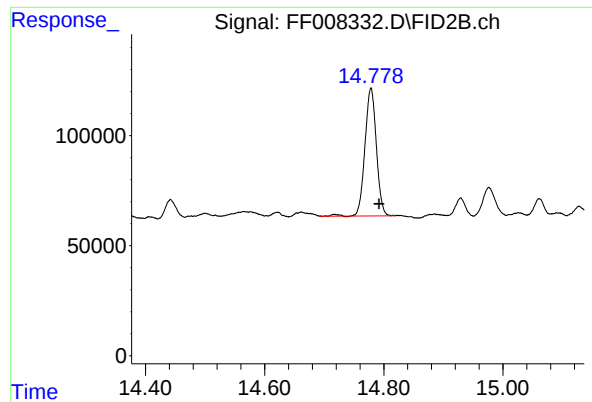

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.778 min
Delta R.T.: -0.013 min
Response: 773355
Conc: 7.05 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-34-COMP