

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF042222\  
Data File : FF010371.D  
Signal(s) : FID2B.ch  
Acq On : 22 Apr 2022 12:21  
Operator : AJ\MA  
Sample : MECL2  
Misc :  
ALS Vial : 51 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Apr 22 23:03:54 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF040122.M  
Quant Title :  
QLast Update : Fri Apr 01 11:58:56 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |                   | R.T.   | Response | Conc Units  |
|-----------------------------|-------------------|--------|----------|-------------|
| -----                       |                   |        |          |             |
| System Monitoring Compounds |                   |        |          |             |
| Target Compounds            |                   |        |          |             |
| 14)                         | N-DOTRIACONTANE   | 18.517 | 160760   | 1.245 ug/ml |
| 16)                         | N-HEXATRIACONTANE | 20.064 | 538446   | 5.162 ug/ml |
| 18)                         | N-TETRACONTANE    | 21.656 | 483620   | 5.521 ug/ml |
| -----                       |                   |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF042222\  
Data File : FF010371.D  
Signal(s) : FID2B.ch  
Acq On : 22 Apr 2022 12:21  
Operator : AJ\MA  
Sample : MECL2  
Misc :  
ALS Vial : 51 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Apr 22 23:03:54 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF040122.M  
Quant Title :  
QLast Update : Fri Apr 01 11:58:56 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

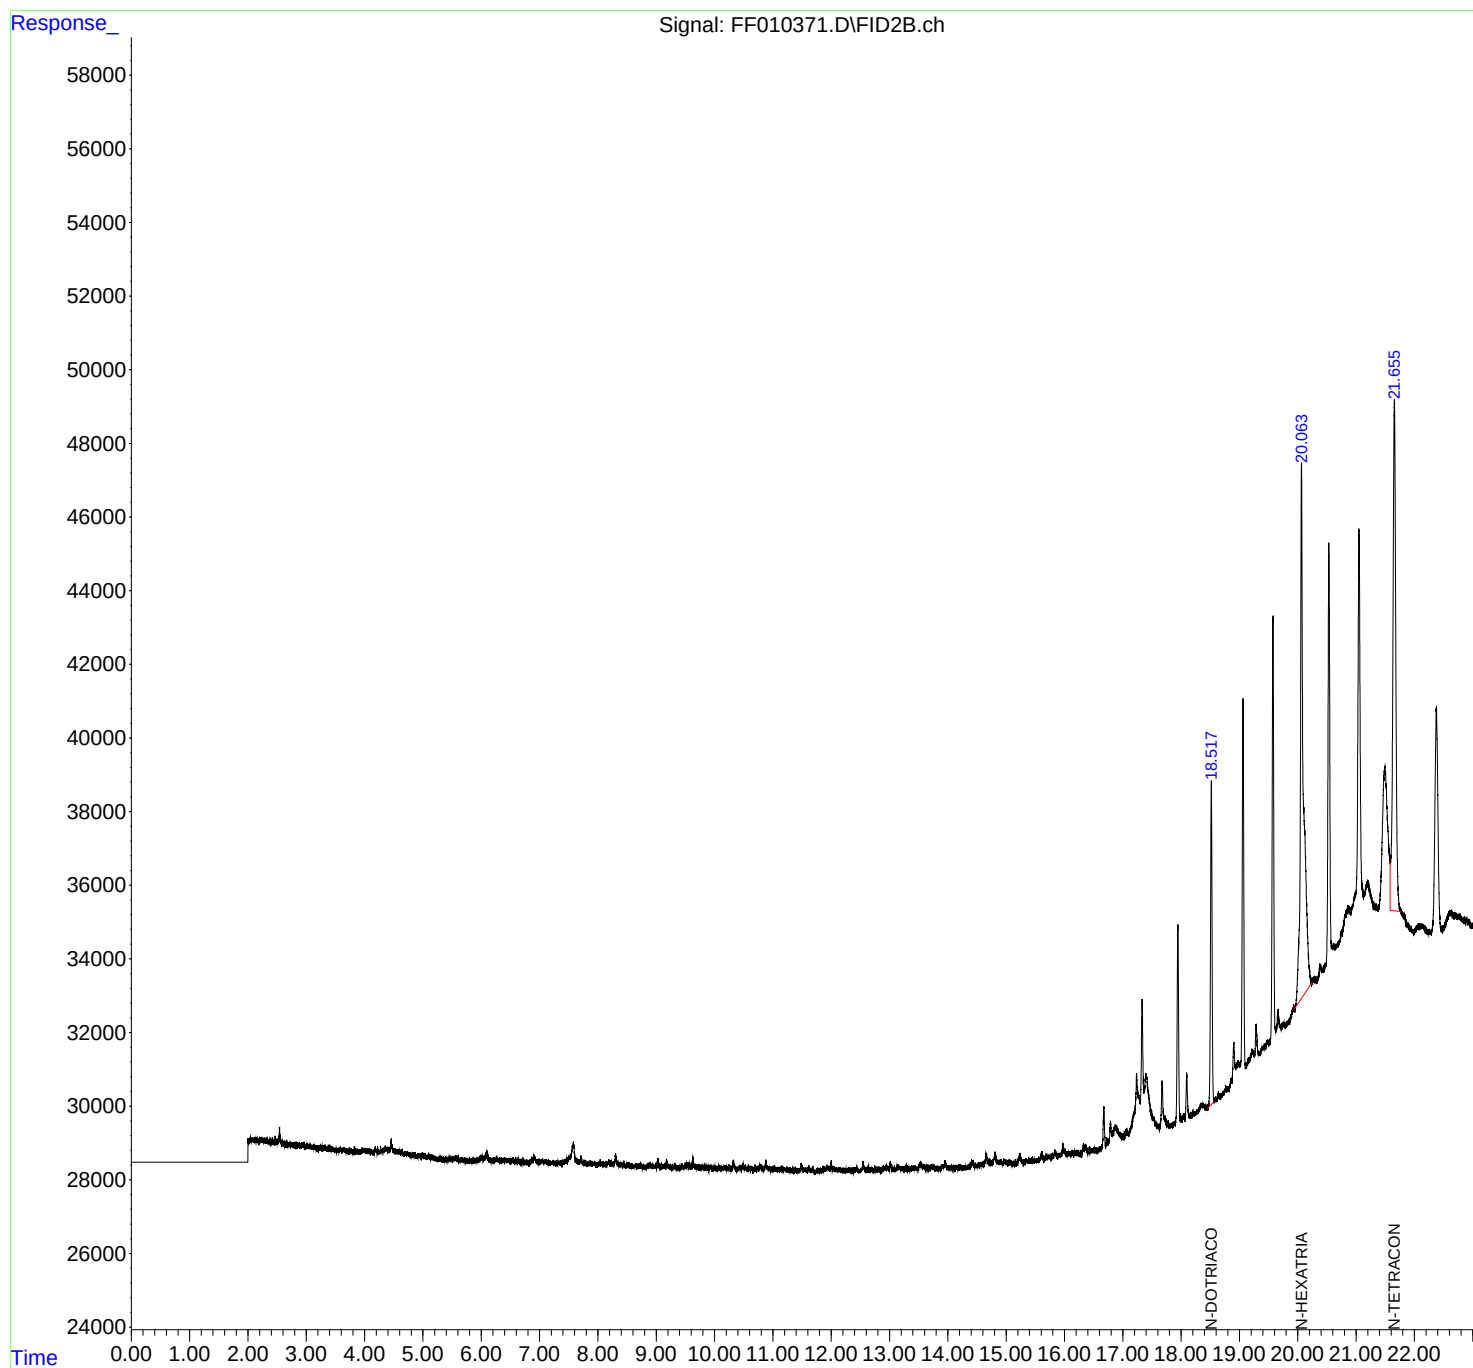


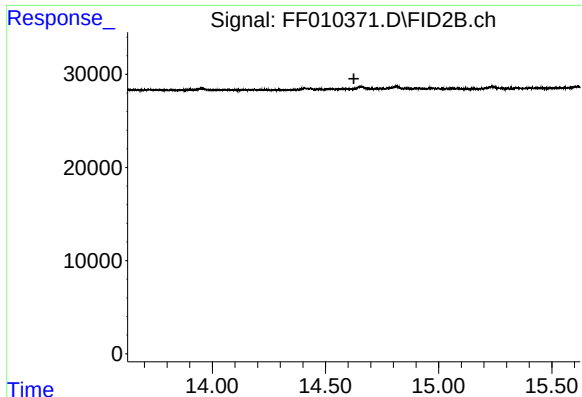

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min  
Exp R.T.: 14.625 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_F  
ClientSampleId :

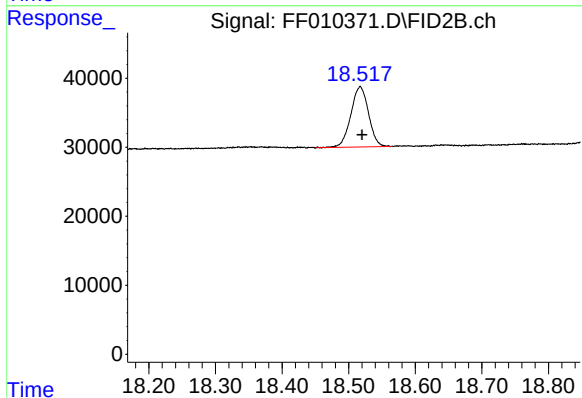


#14 N-DOTRIACONTANE

R.T.: 18.517 min  
Delta R.T.: -0.003 min  
Response: 160760  
Conc: 1.25 ug/ml

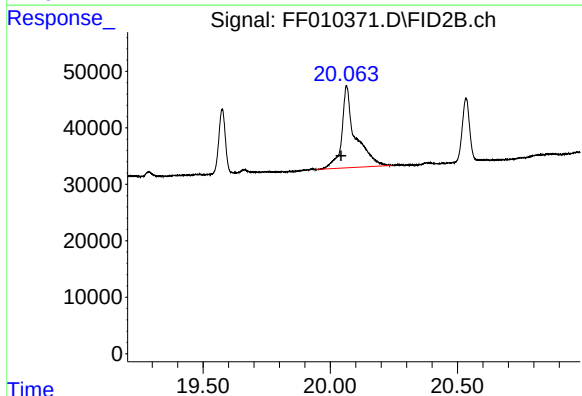

#16 N-HEXATRIACONTANE

R.T.: 20.064 min  
Delta R.T.: 0.022 min  
Response: 538446  
Conc: 5.16 ug/ml

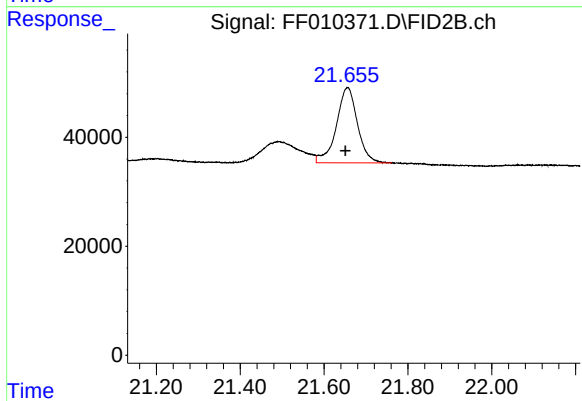

#18 N-TETRACONTANE

R.T.: 21.656 min  
Delta R.T.: 0.005 min  
Response: 483620  
Conc: 5.52 ug/ml