

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042423\
 Data File : FF012532.D
 Signal(s) : FID2B.ch
 Acq On : 24 Apr 2023 10:03
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 24 16:36:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
 Quant Title :
 QLast Update : Thu Apr 13 15:26:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.733	2044719	16.555 ug/ml
12)	N-OCTACOSANE	17.176	2067109	15.673 ug/ml
13)	N-TRIACONTANE	18.061	124956	0.958 ug/ml
14)	N-DOTRIACONTANE	18.893	183643	1.456 ug/ml
15)	N-TETRATRIACONTANE	19.674	192681	1.699 ug/ml
16)	N-HEXATRIACONTANE	20.414	240222	2.352 ug/ml
17)	N-OCTATRIACONTANE	21.146	136202	1.398 ug/ml
18)	N-TETRACONTANE	22.046	100348	1.038 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042423\
Data File : FF012532.D
Signal(s) : FID2B.ch
Acq On : 24 Apr 2023 10:03
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 24 16:36:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

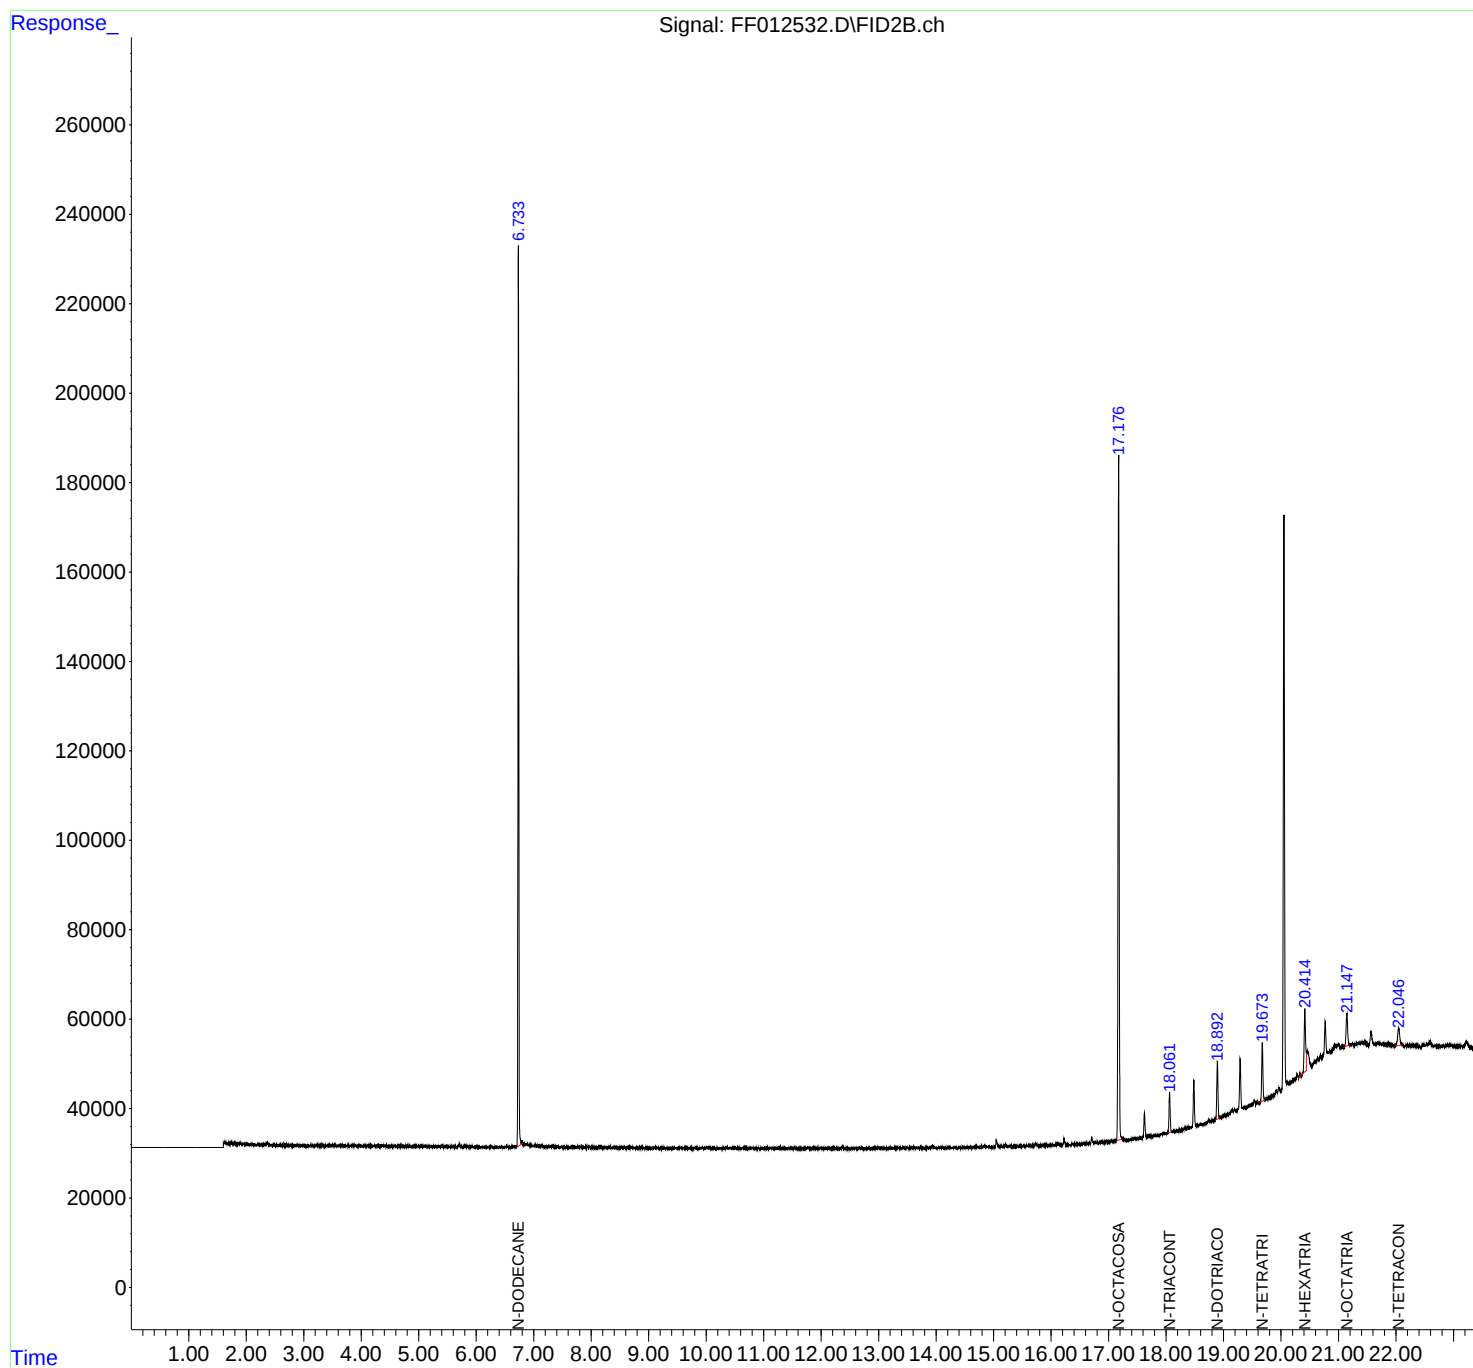


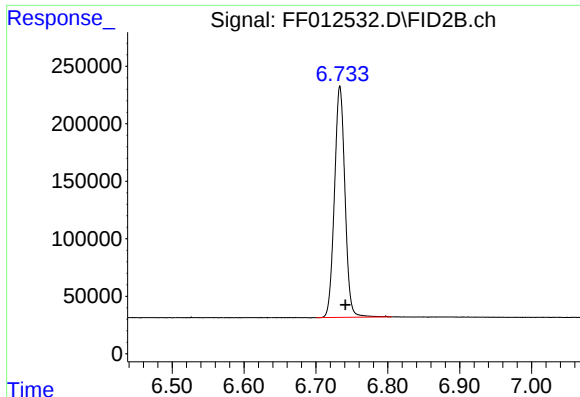

#3 N-DODECANE


R.T.: 6.733 min
Delta R.T.: -0.008 min
Response: 2044719
Conc: 16.56 ug/ml

Instrument :
FID_F
ClientSampleId :

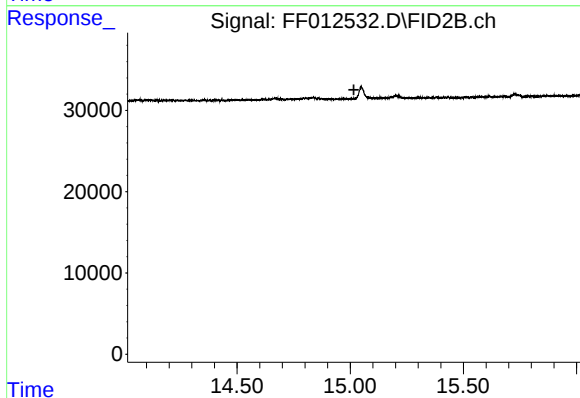


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.016 min
Response: 0
Conc: N.D.

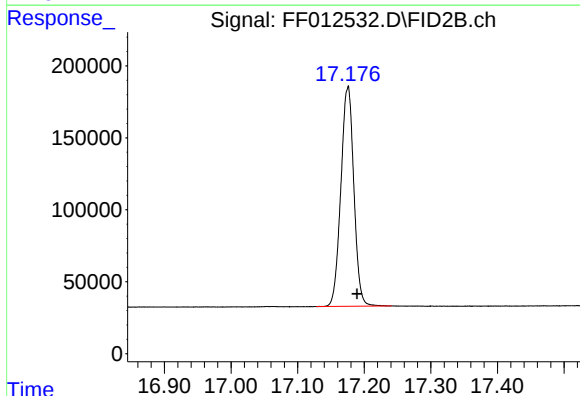


#12 N-OCTACOSANE

R.T.: 17.176 min
Delta R.T.: -0.013 min
Response: 2067109
Conc: 15.67 ug/ml

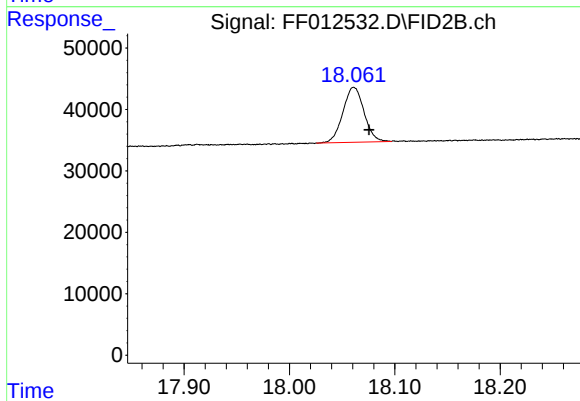

#13 N-TRIACONTANE


R.T.: 18.061 min
Delta R.T.: -0.014 min
Response: 124956
Conc: 0.96 ug/ml

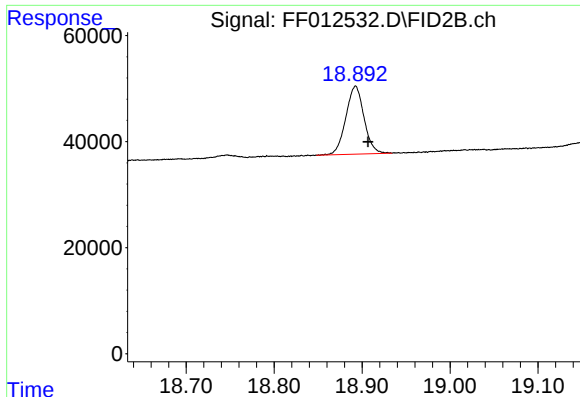

#14 N-DOTRIACONTANE


R.T.: 18.893 min
Delta R.T.: -0.014 min
Response: 183643
Conc: 1.46 ug/ml

Instrument :
FID_F
ClientSampleId :

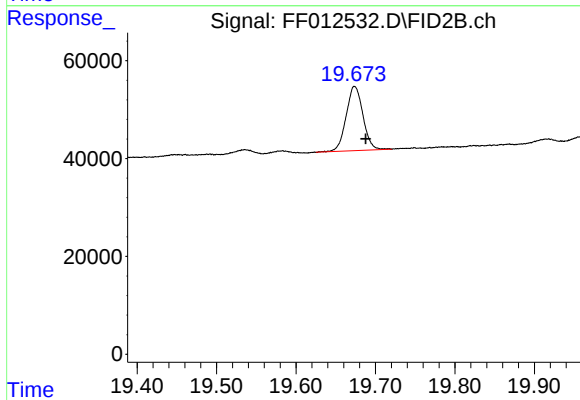


#15 N-TETRATRIACONTANE

R.T.: 19.674 min
Delta R.T.: -0.014 min
Response: 192681
Conc: 1.70 ug/ml

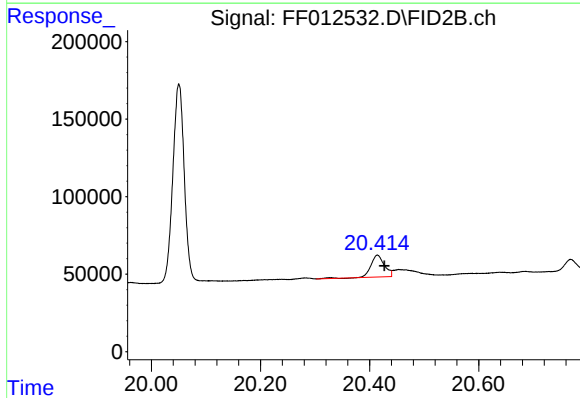


#16 N-HEXATRIACONTANE

R.T.: 20.414 min
Delta R.T.: -0.013 min
Response: 240222
Conc: 2.35 ug/ml

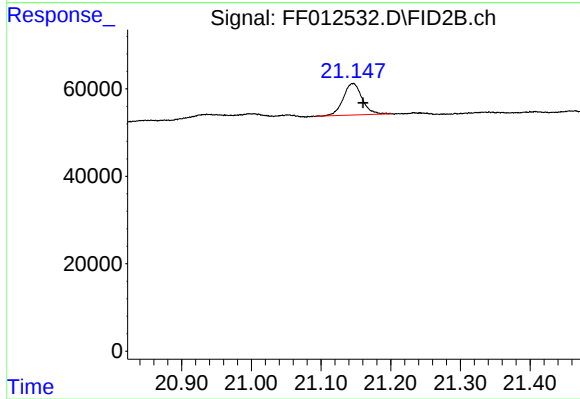

#17 N-OCTATRIACONTANE

R.T.: 21.146 min
Delta R.T.: -0.014 min
Response: 136202
Conc: 1.40 ug/ml

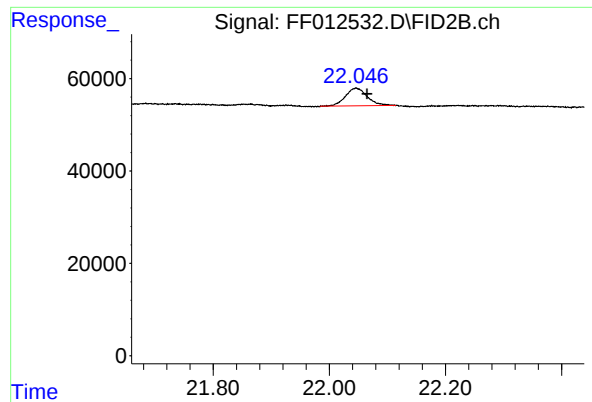

#18 N-TETRACONTANE

R.T.: 22.046 min
Delta R.T.: -0.019 min
Response: 100348
Conc: 1.04 ug/ml

Instrument :

FID_F

ClientSampleId :