

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042423\
 Data File : FF012535.D
 Signal(s) : FID2B.ch
 Acq On : 24 Apr 2023 11:31
 Operator : YP\AJ
 Sample : 02470-10RE
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 24 16:36:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
 Quant Title :
 QLast Update : Thu Apr 13 15:26:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.006	650555	5.412 ug/ml
Target Compounds			
7) N-EICOSANE	12.984f	199663	1.450 ug/ml
10) N-TETRACOSANE	15.205	124859	0.923 ug/ml
11) N-HEXACOSANE	16.230	34656	0.260 ug/ml
12) N-OCTACOSANE	17.179	42328	0.321 ug/ml
13) N-TRIACONTANE	18.066	213394	1.635 ug/ml
14) N-DOTRIACONTANE	18.887	304302	2.412 ug/ml
15) N-TETRATRIACONTANE	19.684	77484	0.683 ug/ml
16) N-HEXATRIACONTANE	20.411	147759	1.447 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042423\
Data File : FF012535.D
Signal(s) : FID2B.ch
Acq On : 24 Apr 2023 11:31
Operator : YP\AJ
Sample : 02470-10RE
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 24 16:36:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

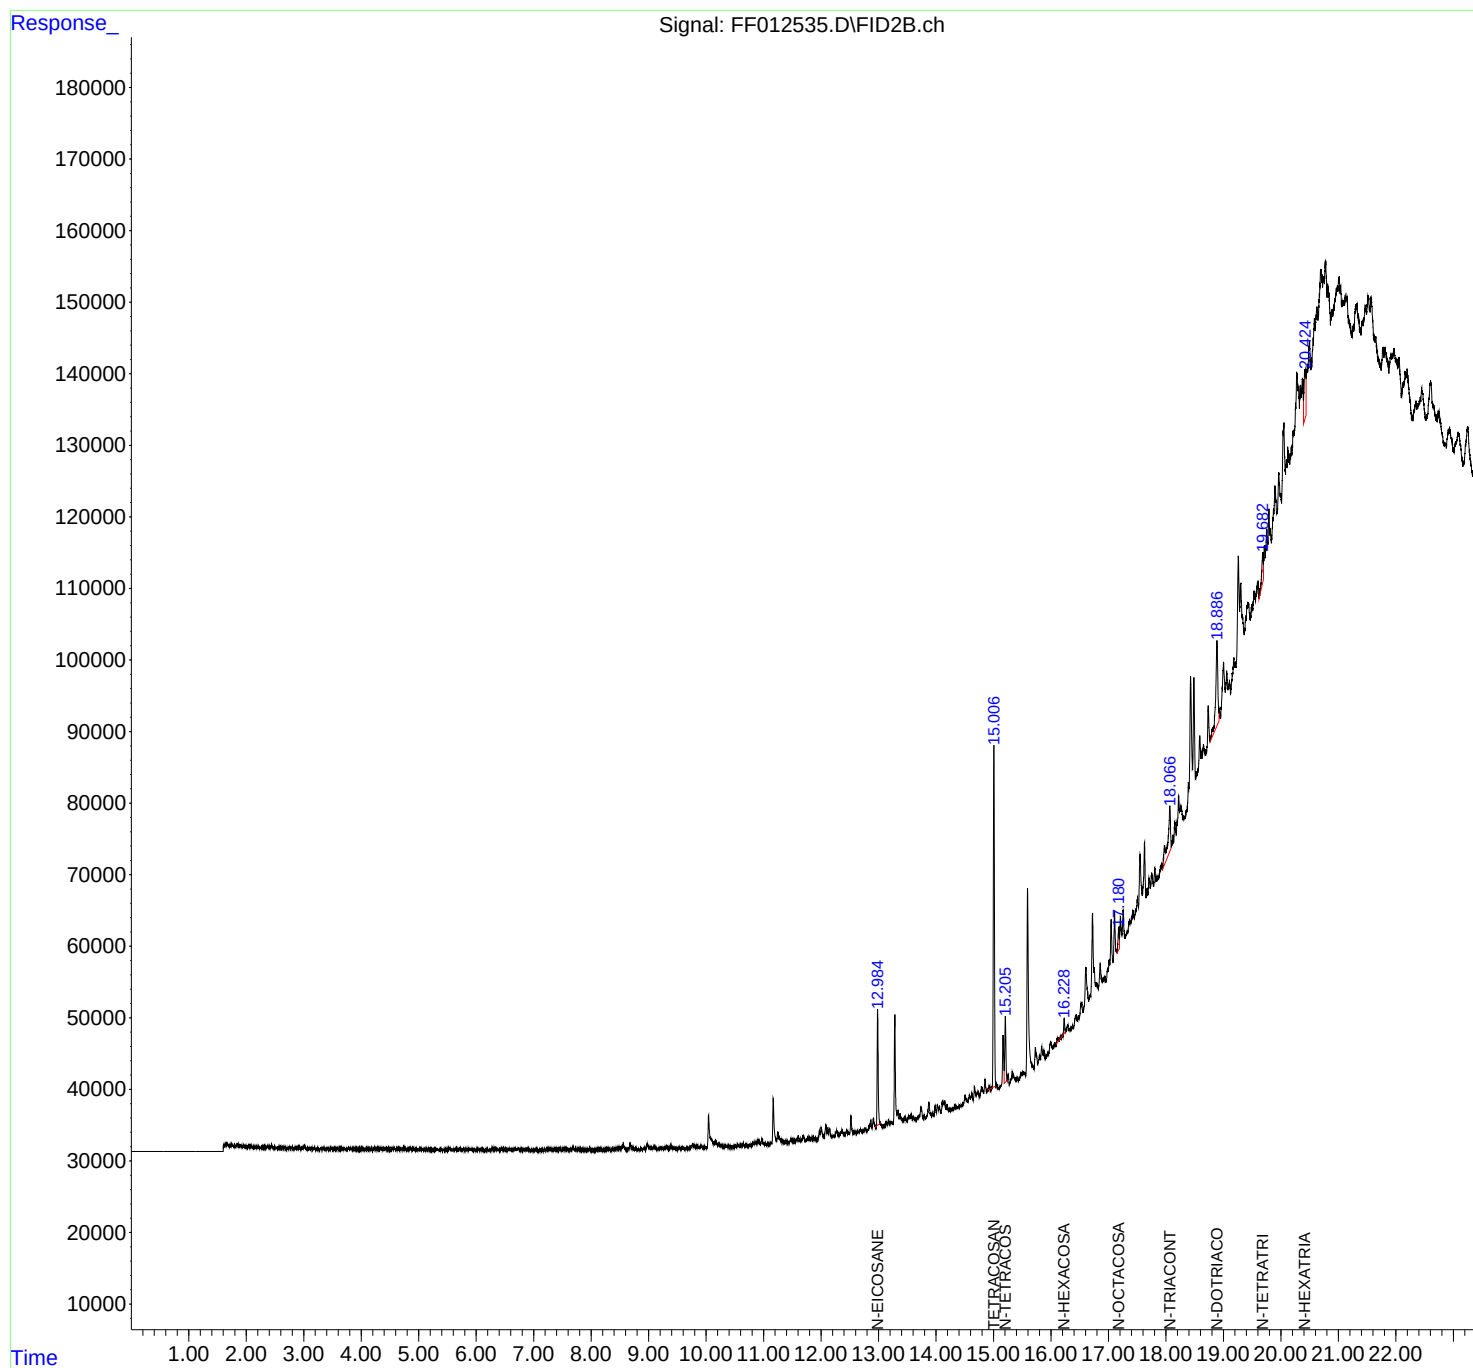


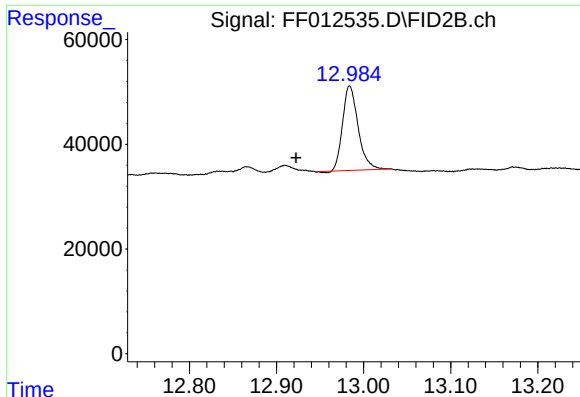

#7 N-EICOSANE


R.T.: 12.984 min
Delta R.T.: 0.061 min
Response: 199663
Conc: 1.45 ug/ml

Instrument :
FID_F
ClientSampleId :

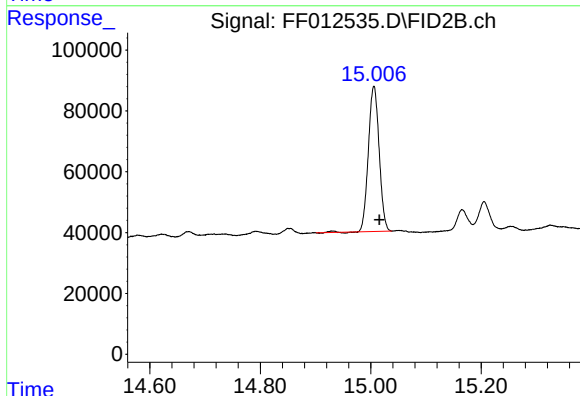


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.006 min
Delta R.T.: -0.010 min
Response: 650555
Conc: 5.41 ug/ml

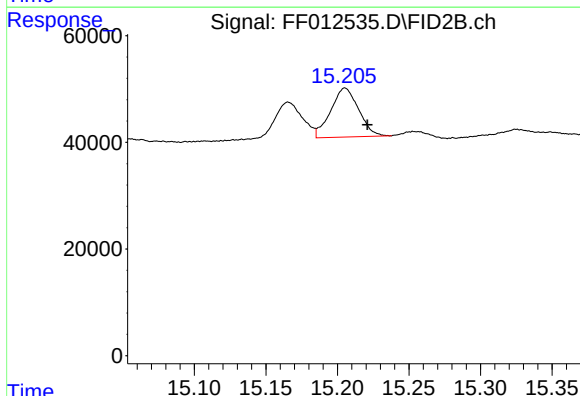


#10 N-TETRACOSANE

R.T.: 15.205 min
Delta R.T.: -0.016 min
Response: 124859
Conc: 0.92 ug/ml

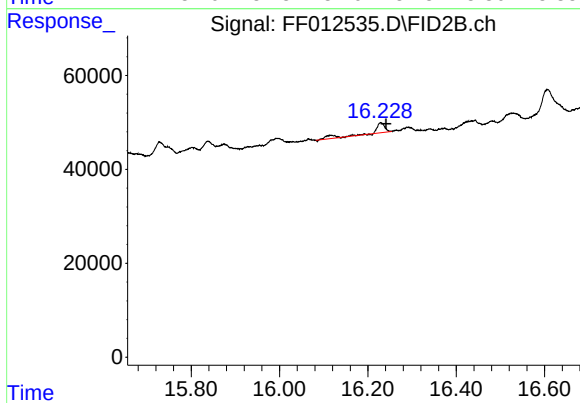

#11 N-HEXACOSANE


R.T.: 16.230 min
Delta R.T.: -0.012 min
Response: 34656
Conc: 0.26 ug/ml

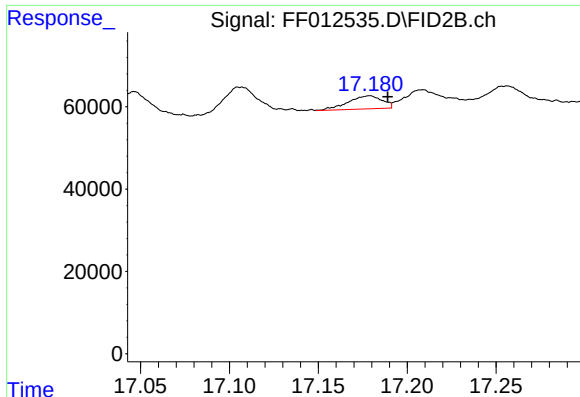

#12 N-OCTACOSANE


R.T.: 17.179 min
Delta R.T.: -0.010 min
Response: 42328
Conc: 0.32 ug/ml

Instrument :
FID_F
ClientSampleId :

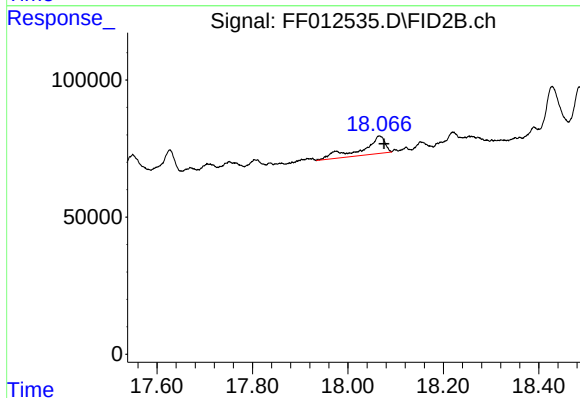


#13 N-TRIACONTANE

R.T.: 18.066 min
Delta R.T.: -0.010 min
Response: 213394
Conc: 1.64 ug/ml

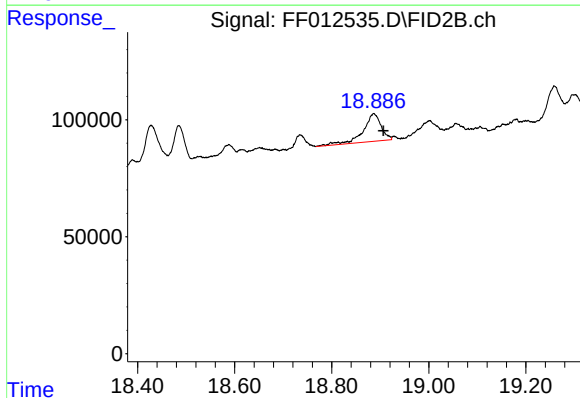


#14 N-DOTRIACONTANE

R.T.: 18.887 min
Delta R.T.: -0.020 min
Response: 304302
Conc: 2.41 ug/ml

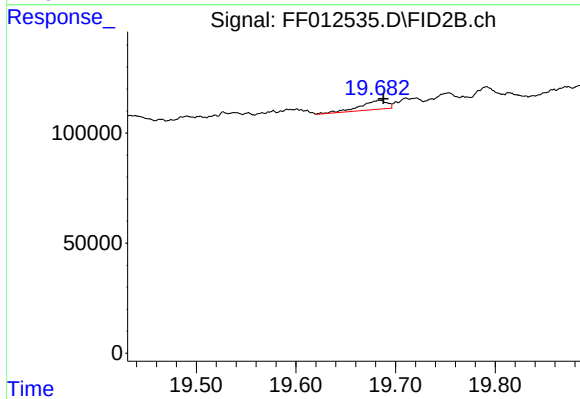

#15 N-TETRATRIACONTANE

R.T.: 19.684 min
Delta R.T.: -0.004 min
Response: 77484
Conc: 0.68 ug/ml

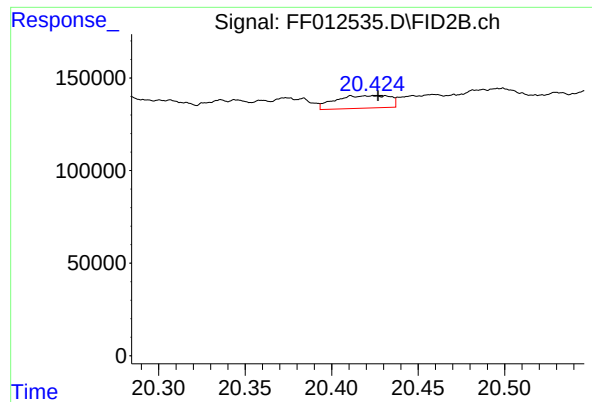

#16 N-HEXATRIACONTANE

R.T.: 20.411 min
Delta R.T.: -0.015 min
Response: 147759
Conc: 1.45 ug/ml

Instrument :

FID_F

ClientSampleId :