

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042519\
 Data File : FF004352.D
 Signal(s) : FID2B.ch
 Acq On : 25 Apr 2019 14:27
 Operator : AJ\SJ
 Sample : K2203-17 2X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 26 01:24:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.525	1050767	8.083 ug/ml
Target Compounds			
4) N-TETRADECANE	8.150	150196	1.056 ug/ml
7) N-EICOSANE	12.489	1778669	11.836 ug/ml
8) N-DOCOSANE	13.659	117159	0.783 ug/ml
10) N-TETRACOSANE	14.717	1095079	7.434 ug/ml
12) N-OCTACOSANE	16.735	281220	1.956 ug/ml
13) N-TRIACONTANE	17.592	320199	2.242 ug/ml
14) N-DOTRIACONTANE	18.423	491950	3.485 ug/ml
15) N-TETRATRIACONTANE	19.234	155578	1.167 ug/ml
16) N-HEXATRIACONTANE	19.964	612825	4.830 ug/ml
17) N-OCTATRIACONTANE	20.639f	59351	0.521 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042519\
Data File : FF004352.D
Signal(s) : FID2B.ch
Acq On : 25 Apr 2019 14:27
Operator : AJ\SJ
Sample : K2203-17 2X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 26 01:24:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

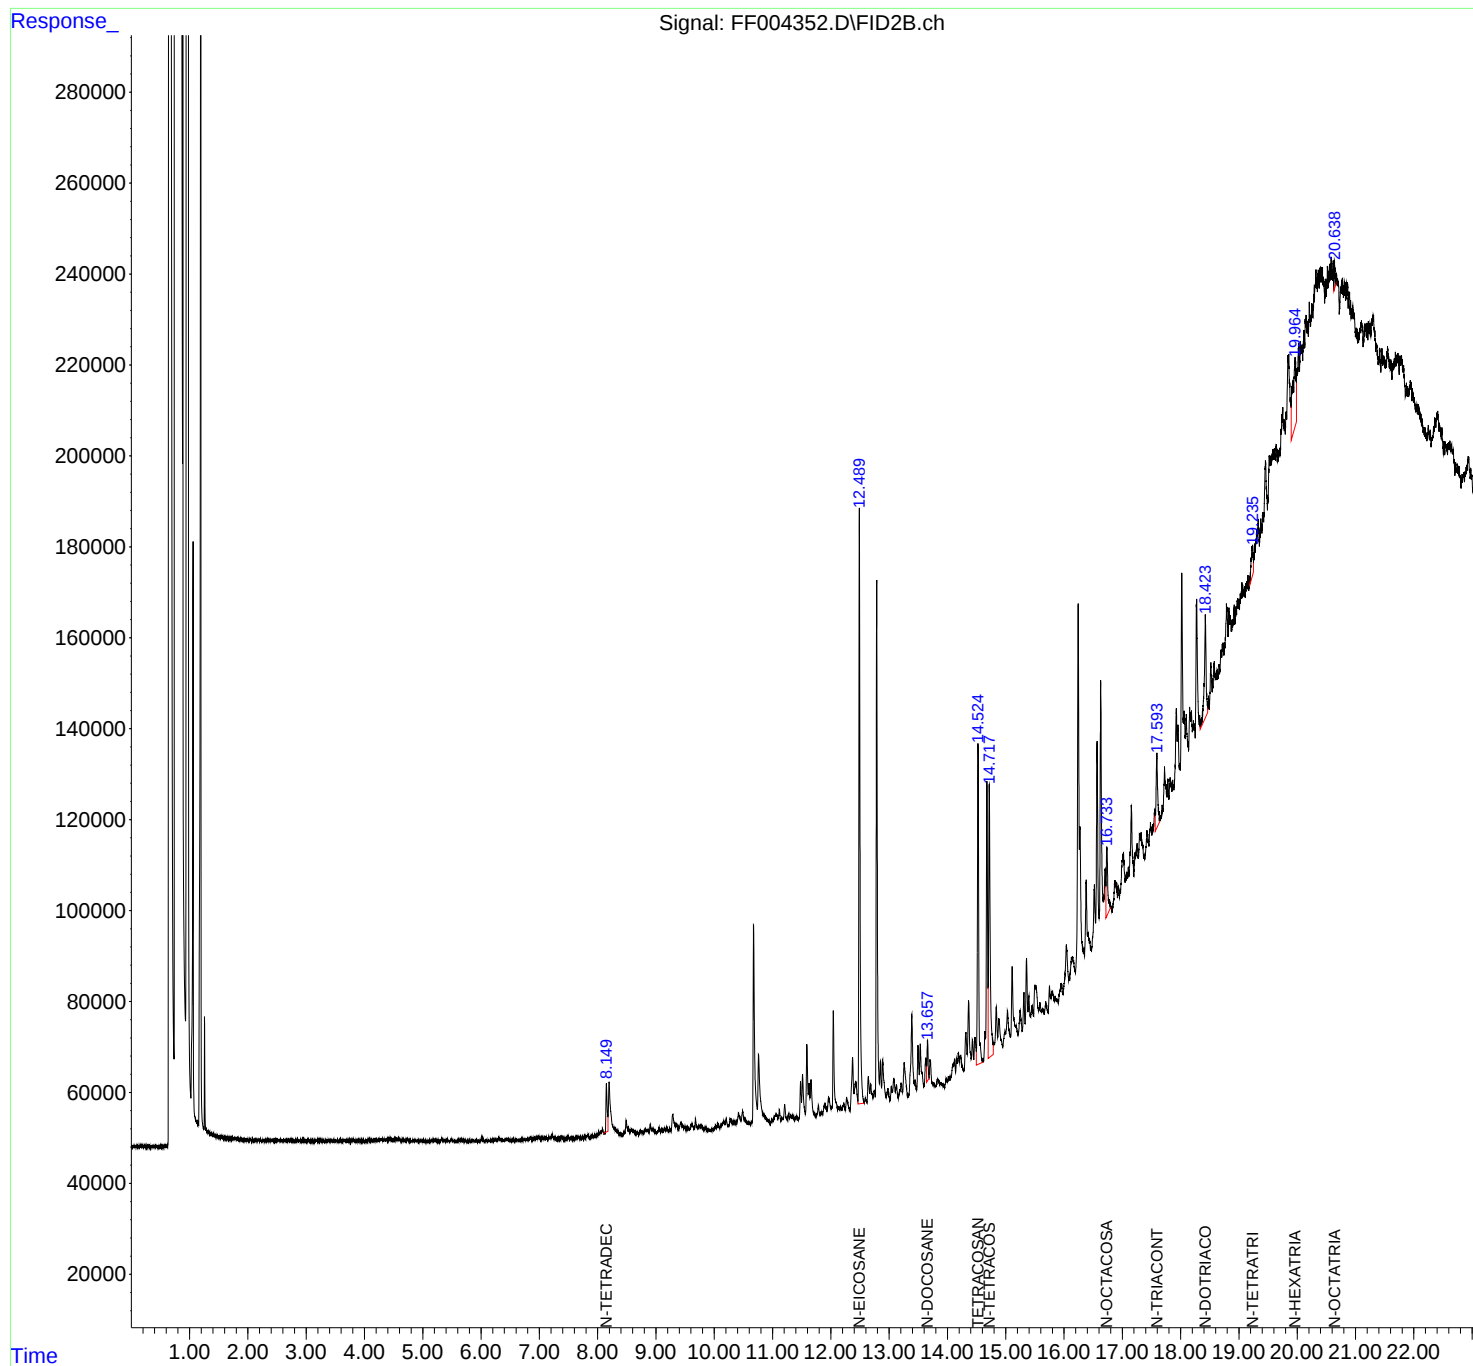

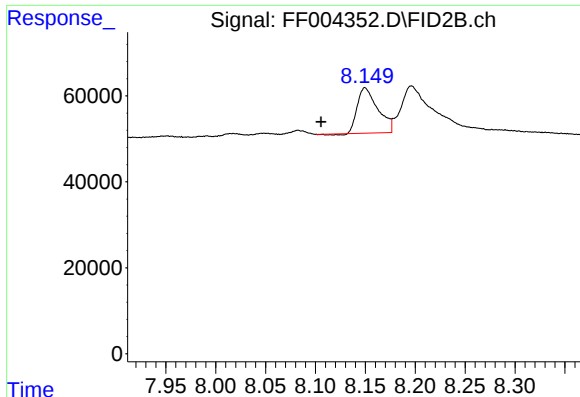


#4 N-TETRADECANE

R.T.: 8.150 min
Delta R.T.: 0.044 min
Response: 150196
Conc: 1.06 ug/ml

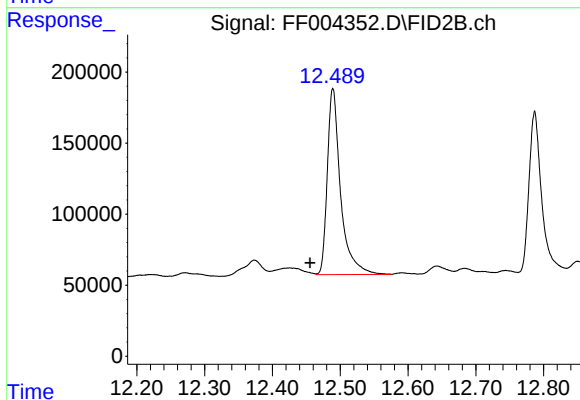


#7 N-EICOSANE

R.T.: 12.489 min
Delta R.T.: 0.033 min
Response: 1778669
Conc: 11.84 ug/ml

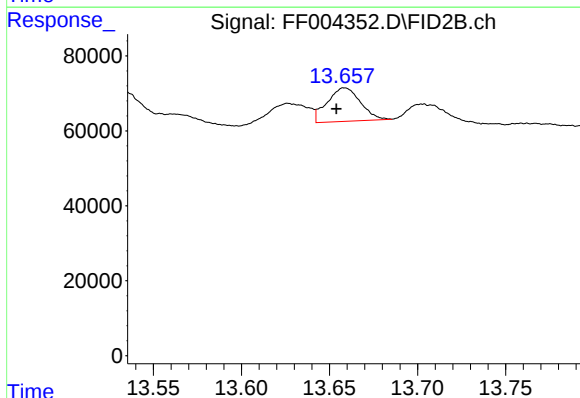


#8 N-DOCOSANE

R.T.: 13.659 min
Delta R.T.: 0.005 min
Response: 117159
Conc: 0.78 ug/ml

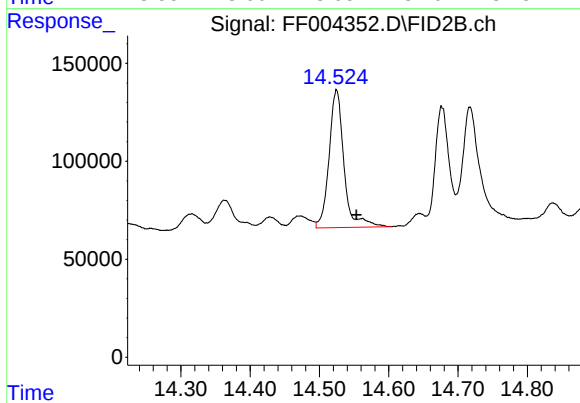


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.525 min
Delta R.T.: -0.029 min
Response: 1050767
Conc: 8.08 ug/ml

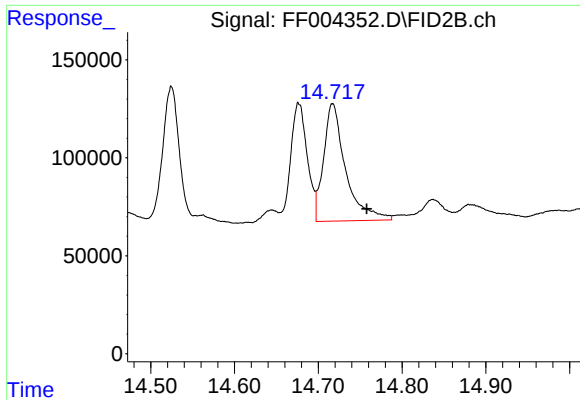


#10 N-TETRACOSANE

R.T.: 14.717 min
Delta R.T.: -0.041 min
Response: 1095079
Conc: 7.43 ug/ml

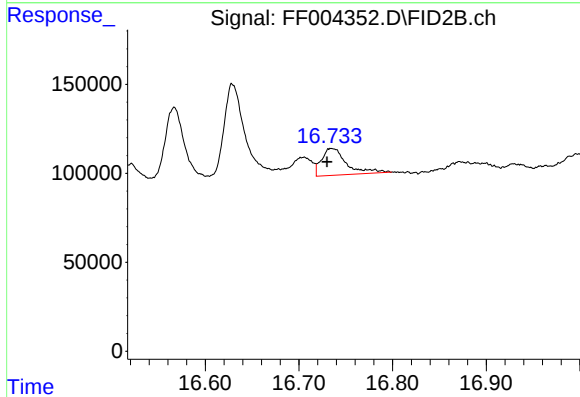


#12 N-OCTACOSANE

R.T.: 16.735 min
Delta R.T.: 0.005 min
Response: 281220
Conc: 1.96 ug/ml

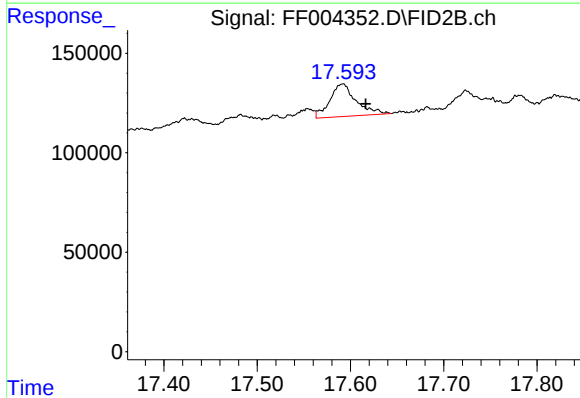


#13 N-TRIACONTANE

R.T.: 17.592 min
Delta R.T.: -0.025 min
Response: 320199
Conc: 2.24 ug/ml

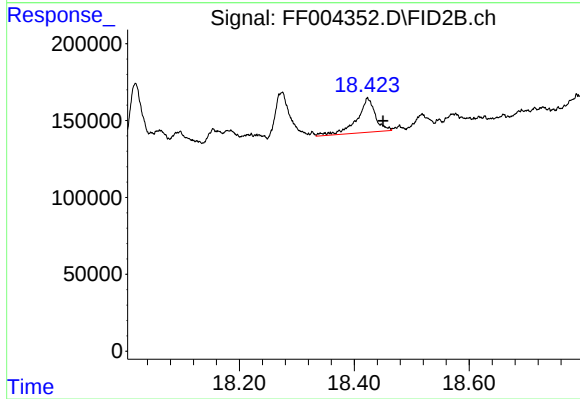

#14 N-DOTRIACONTANE

R.T.: 18.423 min
Delta R.T.: -0.027 min
Response: 491950
Conc: 3.48 ug/ml

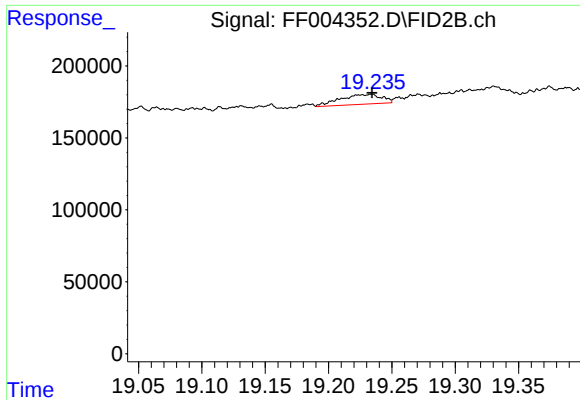


#15 N-TETRATRIACONTANE

R.T.: 19.234 min

Delta R.T.: 0.000 min

Response: 155578

Conc: 1.17 ug/ml

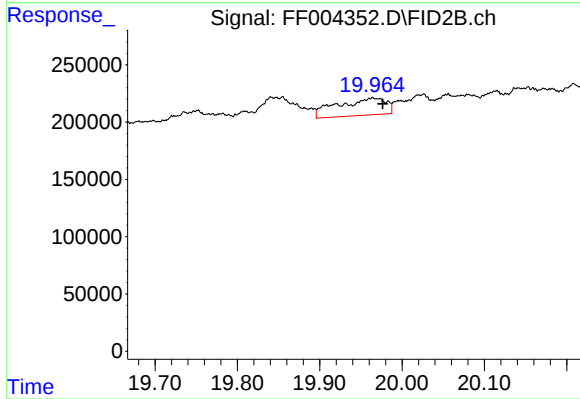


#16 N-HEXATRIACONTANE

R.T.: 19.964 min

Delta R.T.: -0.012 min

Response: 612825

Conc: 4.83 ug/ml

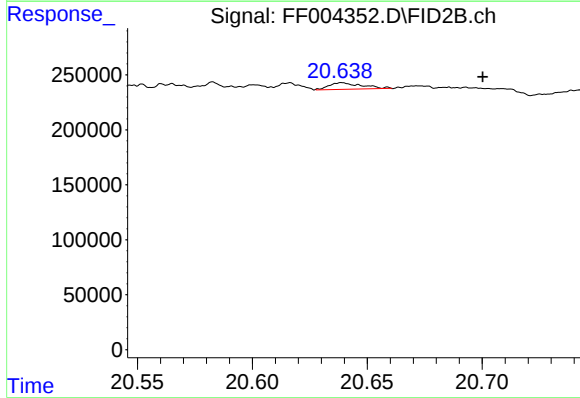

#17 N-OCTATRIACONTANE

R.T.: 20.639 min

Delta R.T.: -0.061 min

Response: 59351

Conc: 0.52 ug/ml