

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042622\
Data File : FF010407.D
Signal(s) : FID2B.ch
Acq On : 26 Apr 2022 18:22
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 27 01:24:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.613	2455420	20.543 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.669	112610	0.853 ug/ml
14) N-DOTRIACONTANE	18.502	241617	1.872 ug/ml
15) N-TETRATRIACONTANE	19.284	94177	0.809 ug/ml
16) N-HEXATRIACONTANE	20.022	42441	0.407 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042622\
Data File : FF010407.D
Signal(s) : FID2B.ch
Acq On : 26 Apr 2022 18:22
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 27 01:24:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

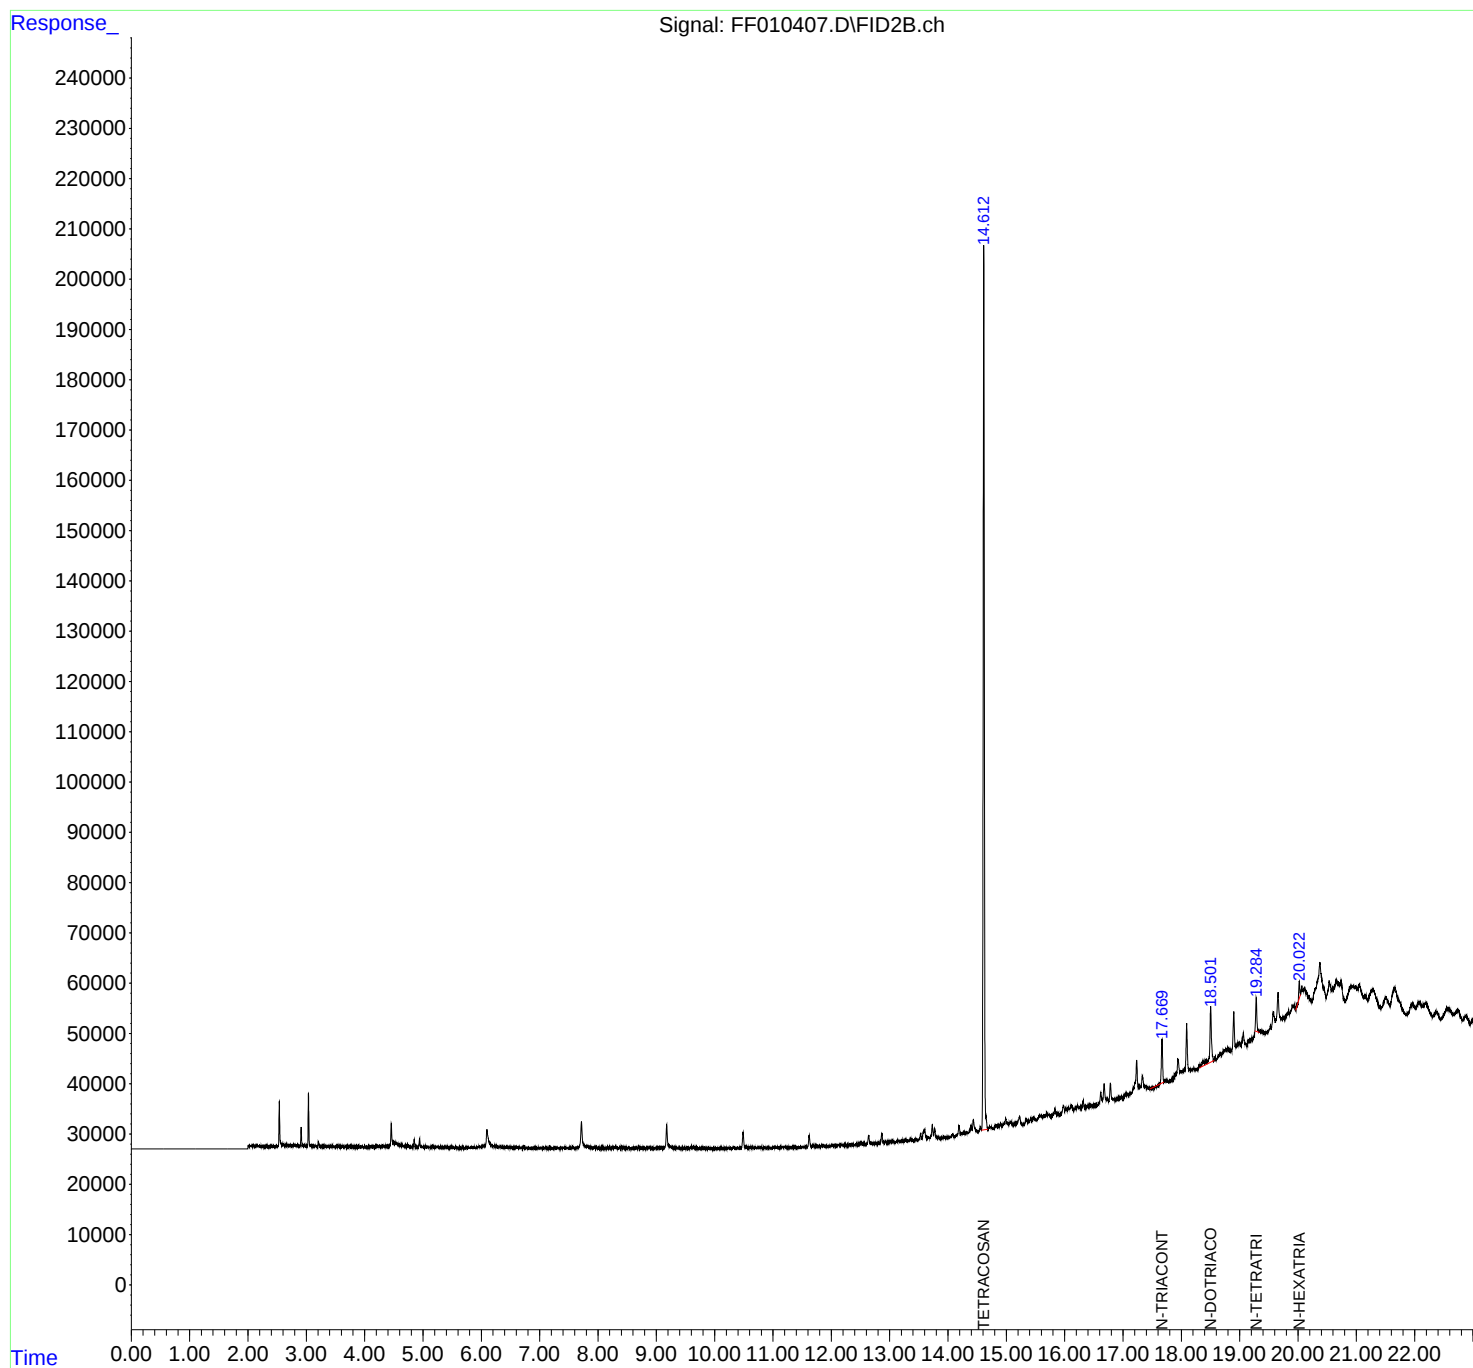


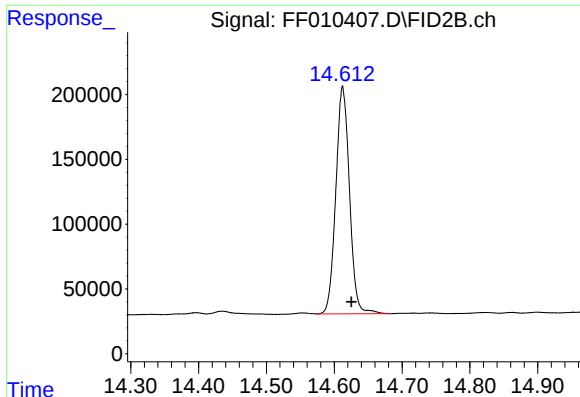

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.613 min
Delta R.T.: -0.013 min
Response: 2455420
Conc: 20.54 ug/ml

Instrument :
FID_F
ClientSampleId :

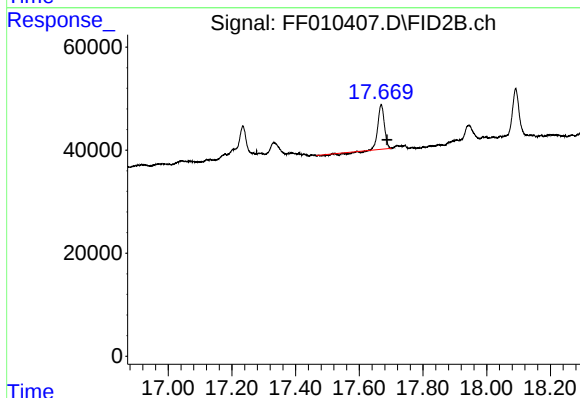


#13 N-TRIACONTANE

R.T.: 17.669 min
Delta R.T.: -0.018 min
Response: 112610
Conc: 0.85 ug/ml

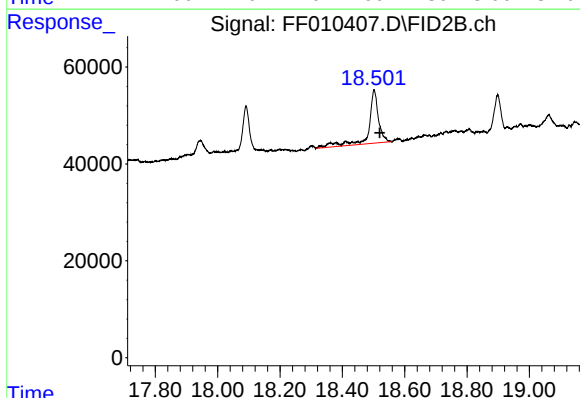


#14 N-DOTRIACONTANE

R.T.: 18.502 min
Delta R.T.: -0.018 min
Response: 241617
Conc: 1.87 ug/ml

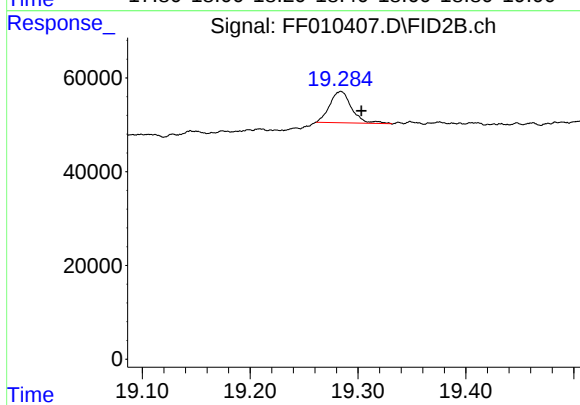

#15 N-TETRATRIACONTANE

R.T.: 19.284 min
Delta R.T.: -0.020 min
Response: 94177
Conc: 0.81 ug/ml

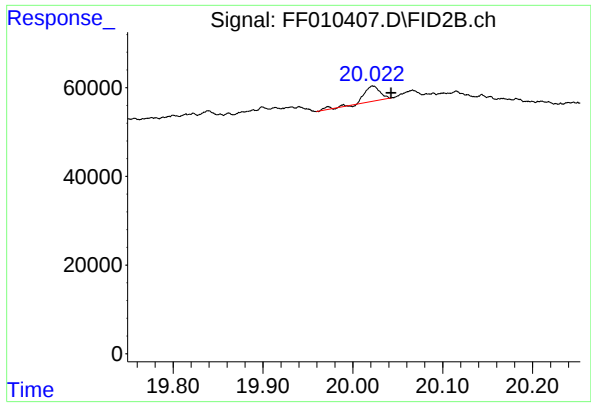

#16 N-HEXATRIACONTANE

R.T.: 20.022 min
Delta R.T.: -0.020 min
Response: 42441
Conc: 0.41 ug/ml

Instrument :
FID_F
ClientSampleId :