

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042622\
Data File : FF010399.D
Signal(s) : FID2B.ch
Acq On : 26 Apr 2022 11:46
Operator : AJ\MA
Sample : N2549-04 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SIMW-04-20220422-A

Integration File: Sample.e
Quant Time: Apr 27 01:22:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.609	479516	4.012 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042622\
Data File : FF010399.D
Signal(s) : FID2B.ch
Acq On : 26 Apr 2022 11:46
Operator : AJ\MA
Sample : N2549-04 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SIMW-04-20220422-A

Integration File: Sample.e
Quant Time: Apr 27 01:22:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

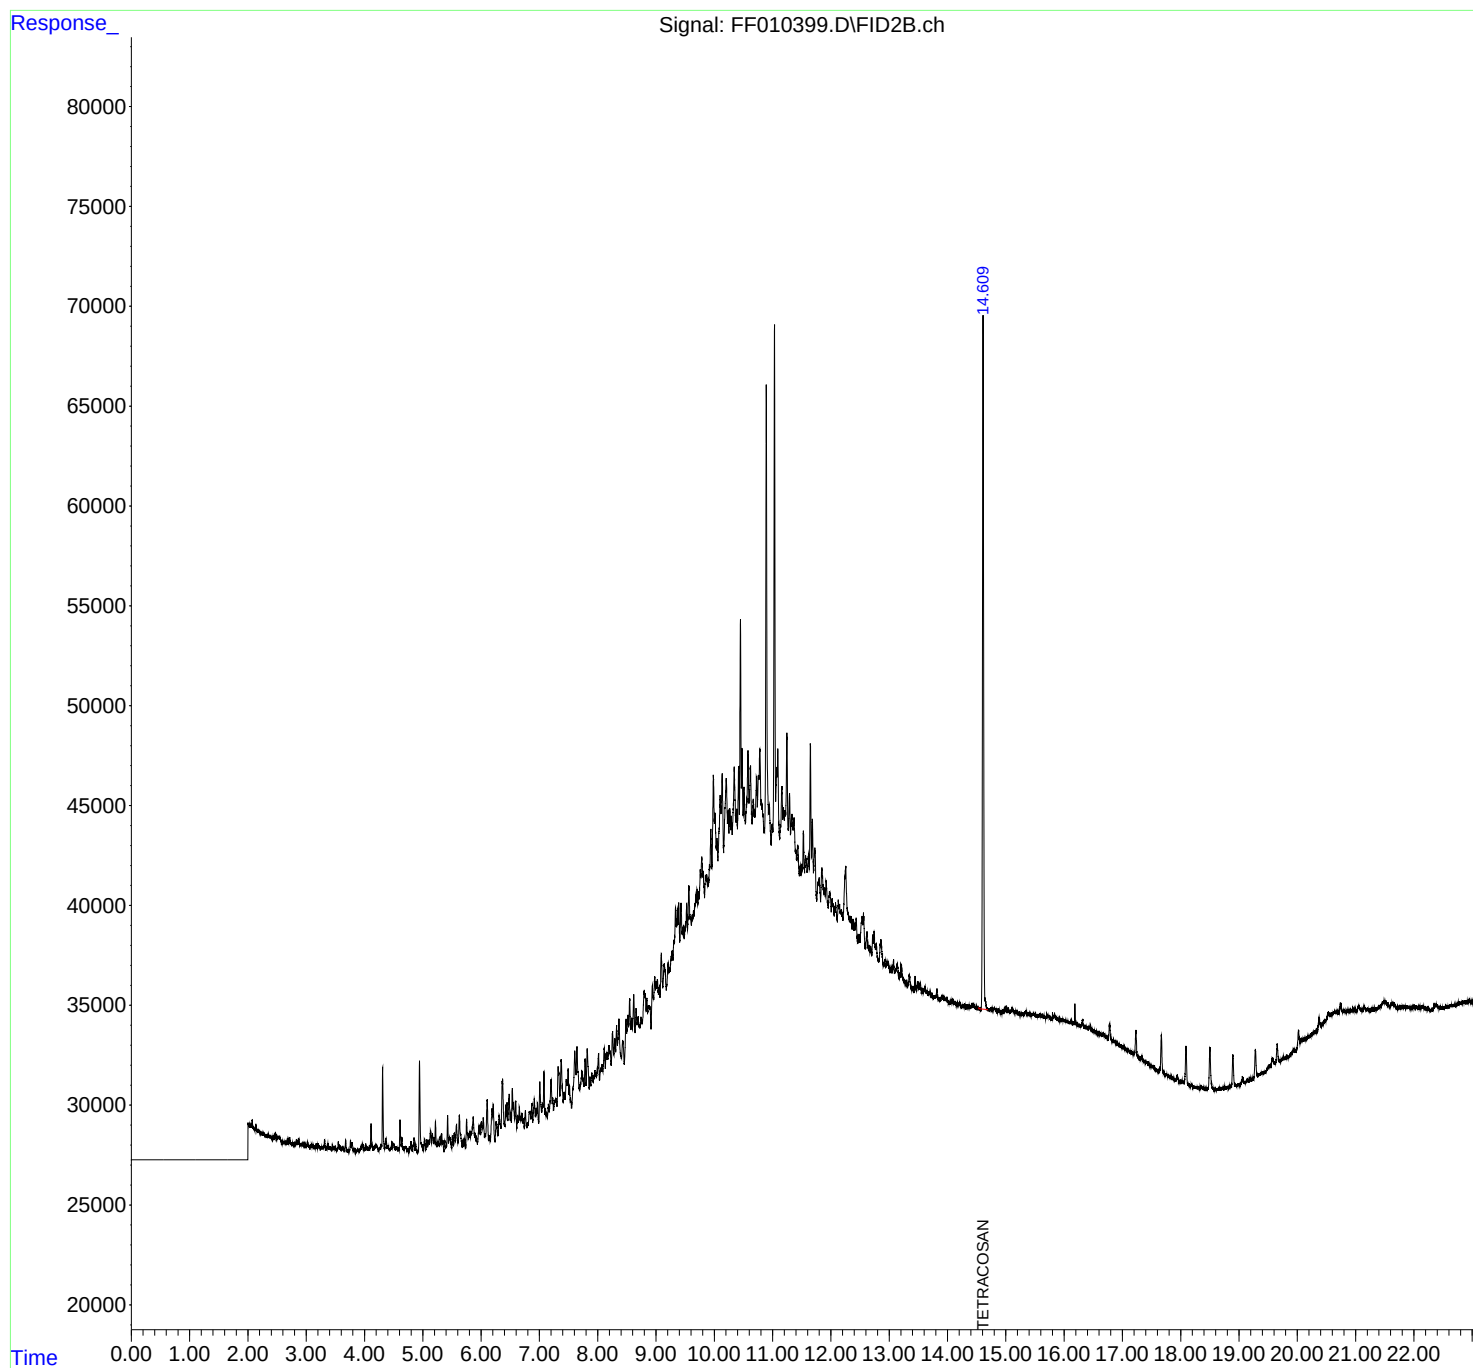

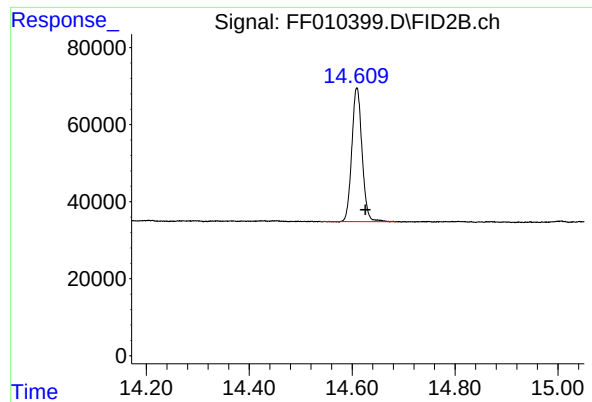

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.609 min
Delta R.T.: -0.016 min
Response: 479516
Conc: 4.01 ug/ml

Instrument :

FID_F

ClientSampleId :

SIMW-04-20220422-A