

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042624\
 Data File : FF014106.D
 Signal(s) : FID2B.ch
 Acq On : 26 Apr 2024 08:18
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 27 02:36:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041124.M
 Quant Title :
 QLast Update : Thu Apr 11 13:04:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.861	306229	2.516 ug/ml
15) N-TETRATRIACONTANE	19.560f	54654	0.495 ug/ml
16) N-HEXATRIACONTANE	20.412	421010	4.218 ug/ml
18) N-TETRACONTANE	22.026	433481	5.255 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042624\
Data File : FF014106.D
Signal(s) : FID2B.ch
Acq On : 26 Apr 2024 08:18
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 27 02:36:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041124.M
Quant Title :
QLast Update : Thu Apr 11 13:04:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

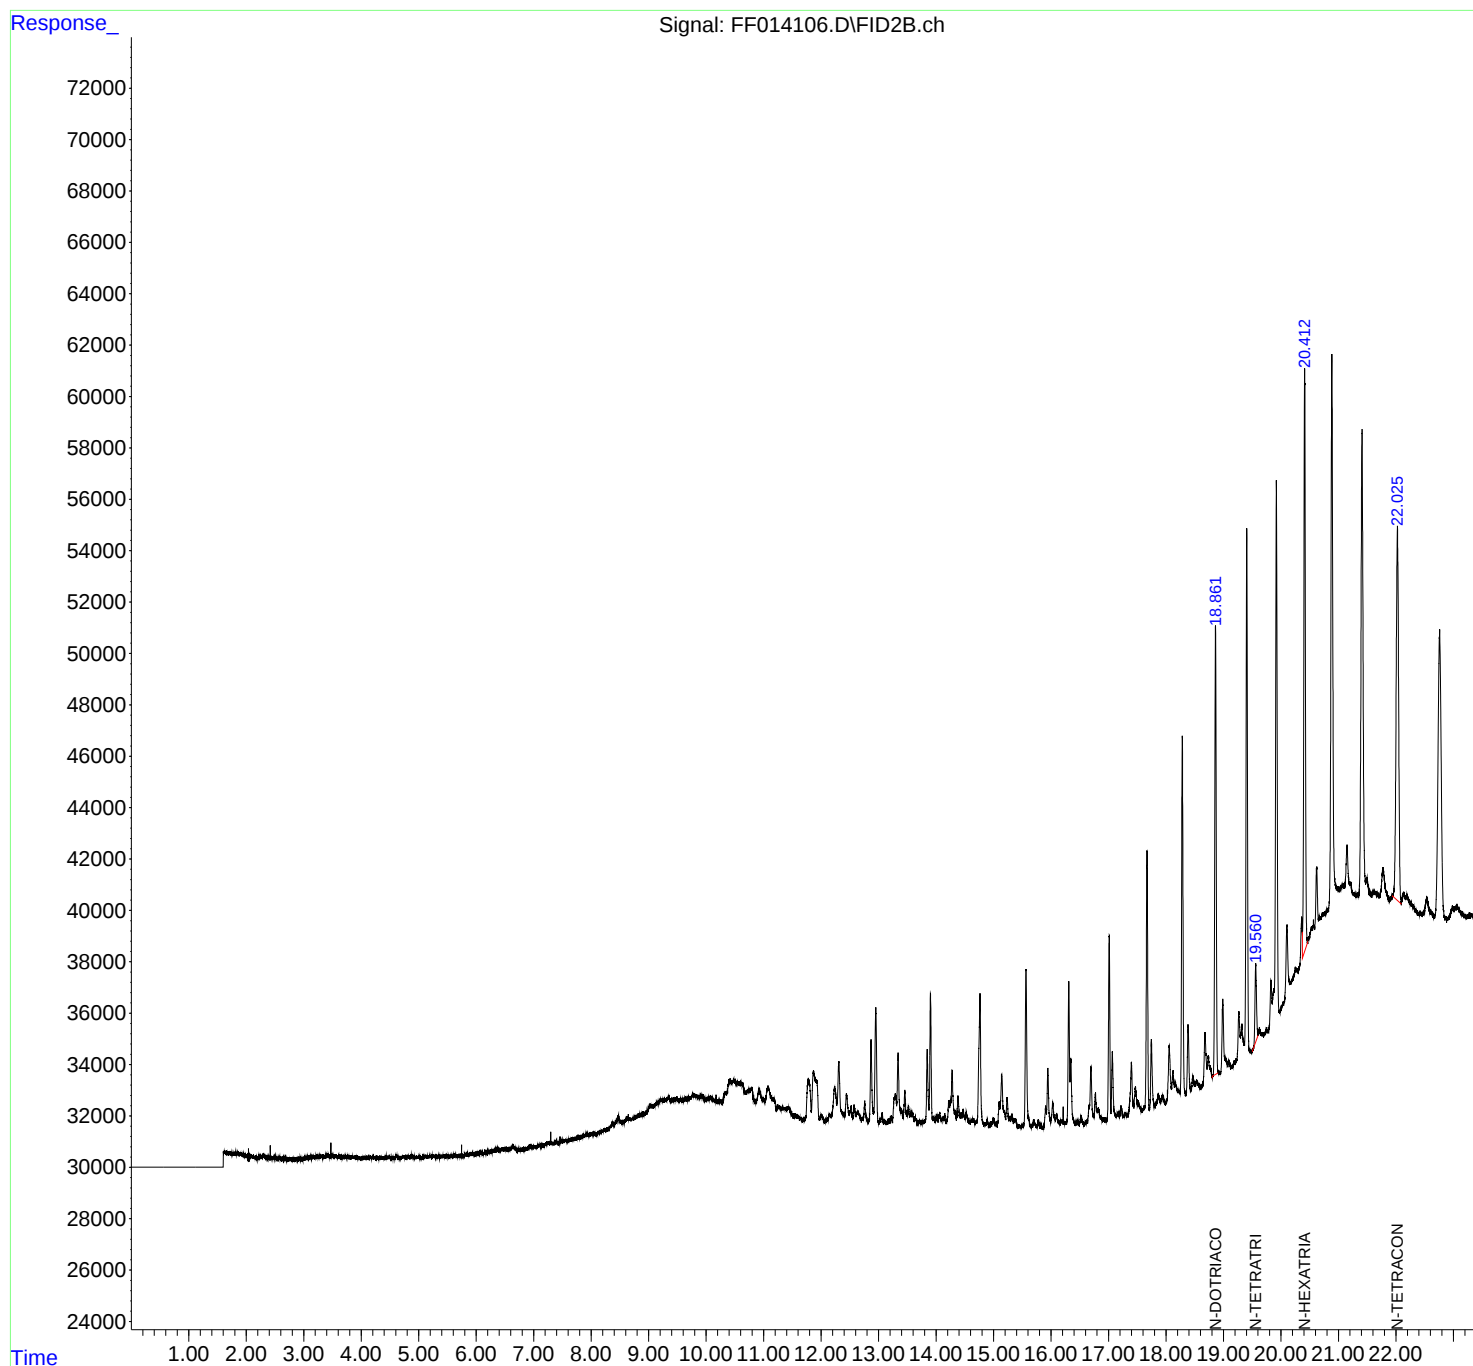


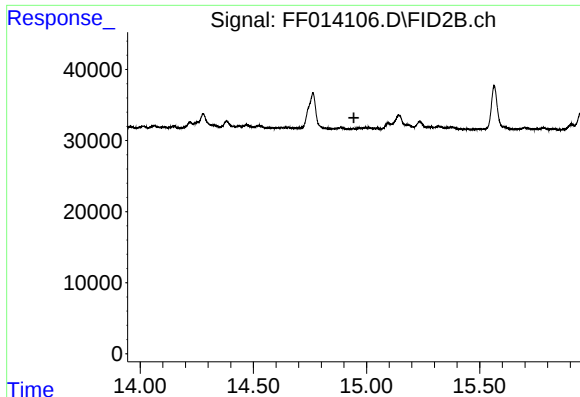

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.944 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

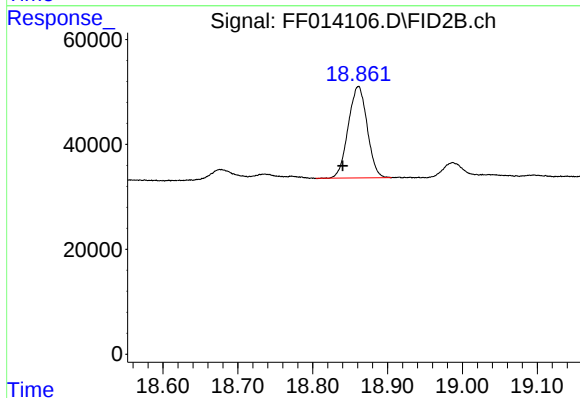


#14 N-DOTRIACONTANE

R.T.: 18.861 min
Delta R.T.: 0.021 min
Response: 306229
Conc: 2.52 ug/ml

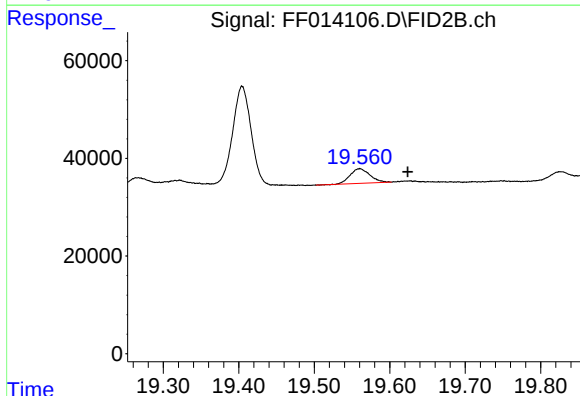


#15 N-TETRATRIACONTANE

R.T.: 19.560 min
Delta R.T.: -0.063 min
Response: 54654
Conc: 0.49 ug/ml

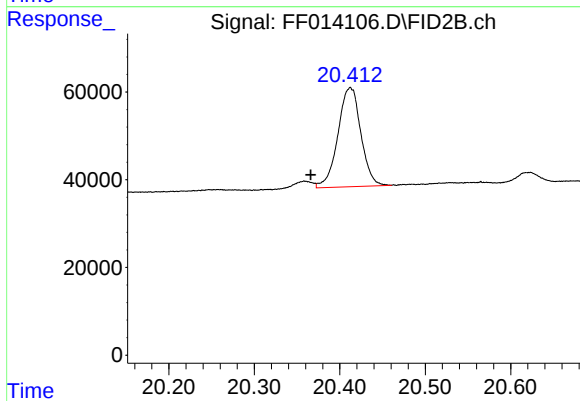

#16 N-HEXATRIACONTANE

R.T.: 20.412 min
Delta R.T.: 0.046 min
Response: 421010
Conc: 4.22 ug/ml

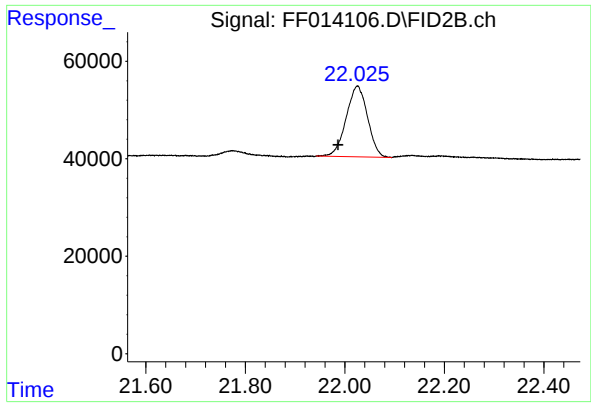

#18 N-TETRACONTANE

R.T.: 22.026 min
Delta R.T.: 0.039 min
Response: 433481
Conc: 5.25 ug/ml

Instrument :
FID_F
ClientSampleId :