

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042624\
Data File : FF014107.D
Signal(s) : FID2B.ch
Acq On : 26 Apr 2024 09:45
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 27 02:36:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041124.M
Quant Title :
QLast Update : Thu Apr 11 13:04:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.944	1764187	16.168 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.863	58433	0.480 ug/ml
16) N-HEXATRIACONTANE	20.412	107955	1.082 ug/ml
18) N-TETRACONTANE	22.019	117224	1.421 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042624\
Data File : FF014107.D
Signal(s) : FID2B.ch
Acq On : 26 Apr 2024 09:45
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 27 02:36:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041124.M
Quant Title :
QLast Update : Thu Apr 11 13:04:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

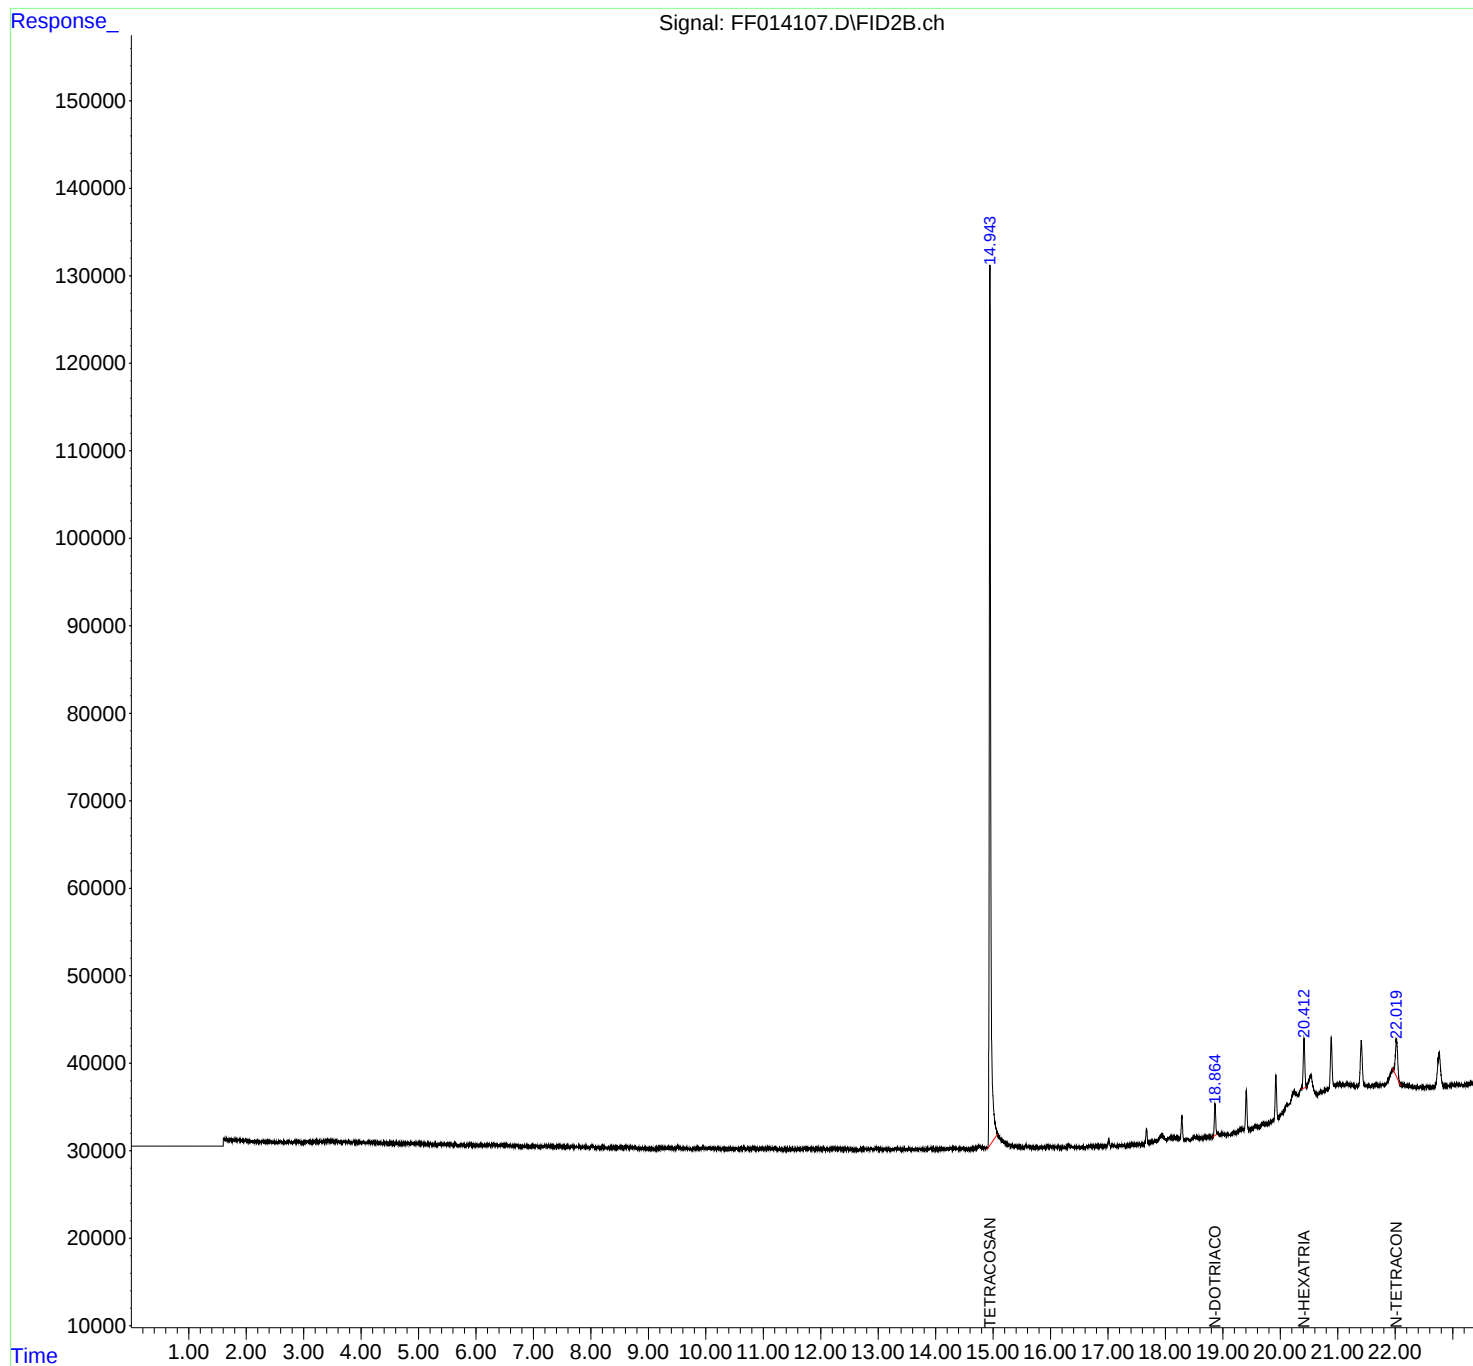


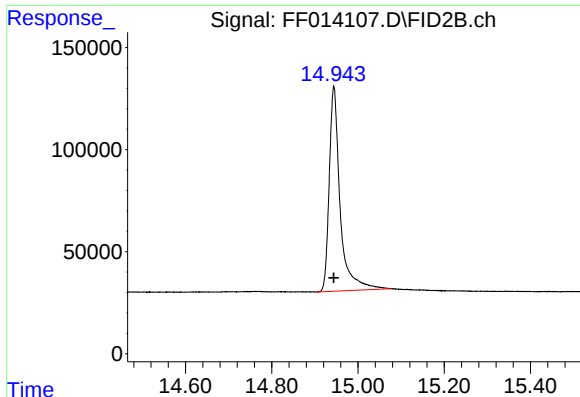

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.944 min
Delta R.T.: 0.000 min
Response: 1764187
Conc: 16.17 ug/ml

Instrument :
FID_F
ClientSampleId :

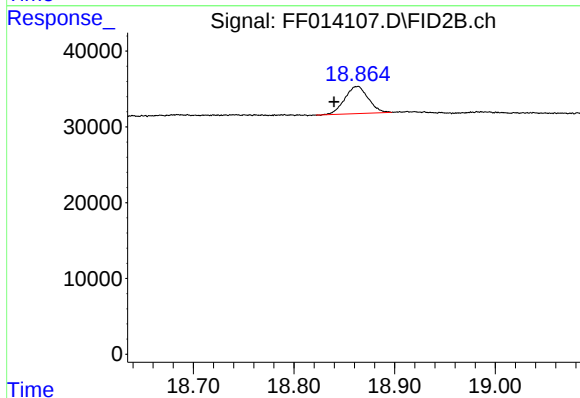


#14 N-DOTRIACONTANE

R.T.: 18.863 min
Delta R.T.: 0.023 min
Response: 58433
Conc: 0.48 ug/ml

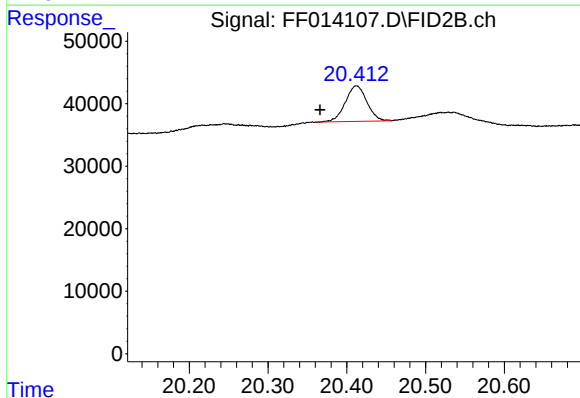

#16 N-HEXATRIACONTANE

R.T.: 20.412 min
Delta R.T.: 0.046 min
Response: 107955
Conc: 1.08 ug/ml

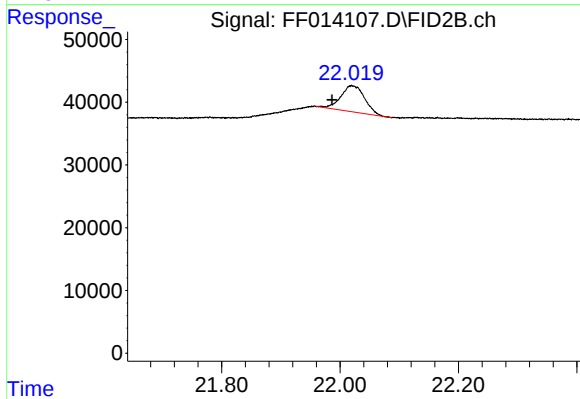

#18 N-TETRACONTANE

R.T.: 22.019 min
Delta R.T.: 0.033 min
Response: 117224
Conc: 1.42 ug/ml