

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042722\
Data File : FF010409.D
Signal(s) : FID2B.ch
Acq On : 27 Apr 2022 10:33
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 28 02:11:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
8)	N-DOCOSANE	13.702	59540	0.445 ug/ml
14)	N-DOTRIACONTANE	18.517	573571	4.444 ug/ml
16)	N-HEXATRIACONTANE	20.063	478120	4.584 ug/ml
18)	N-TETRACONTANE	21.654	412070	4.704 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042722\
Data File : FF010409.D
Signal(s) : FID2B.ch
Acq On : 27 Apr 2022 10:33
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 28 02:11:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

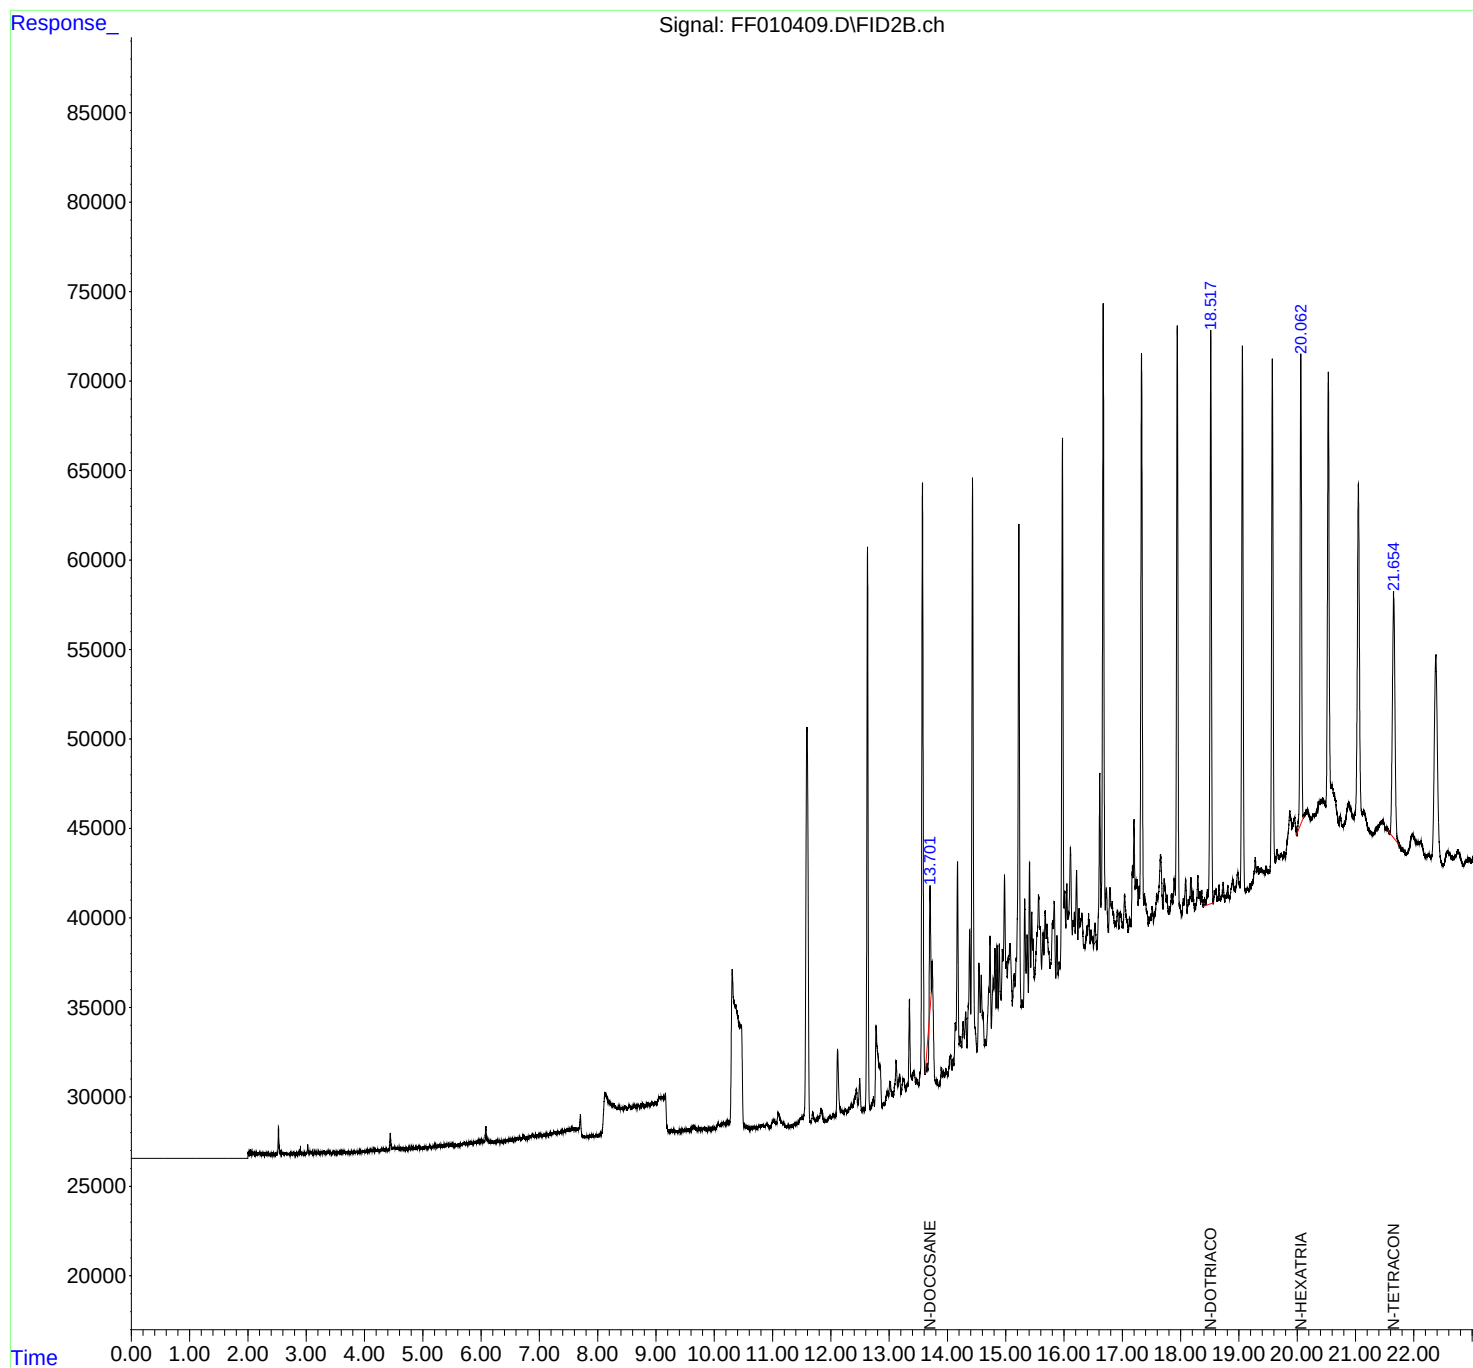


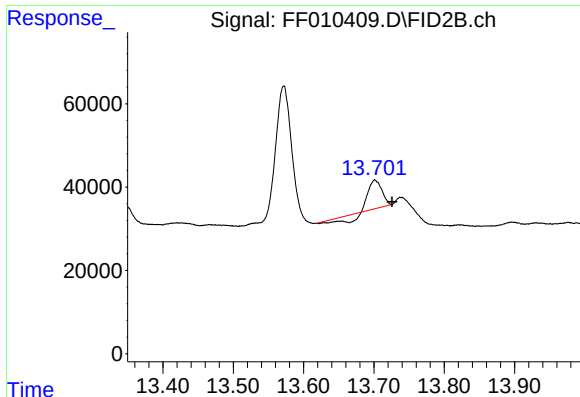

#8 N-DOCOSANE


R.T.: 13.702 min
Delta R.T.: -0.024 min
Response: 59540
Conc: 0.44 ug/ml

Instrument :
FID_F
ClientSampleId :

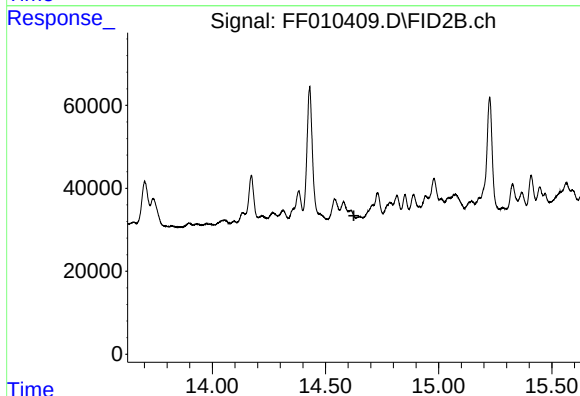


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.625 min
Response: 0
Conc: N.D.

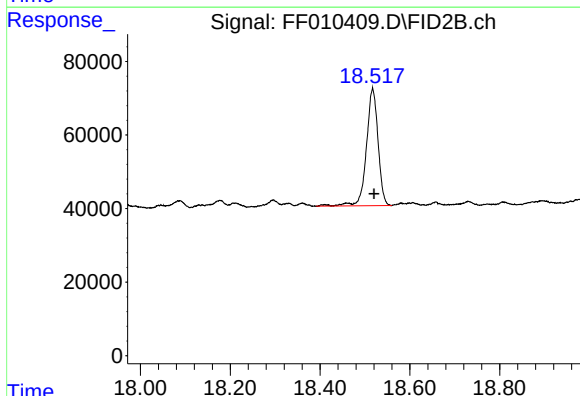


#14 N-DOTRIACONTANE

R.T.: 18.517 min
Delta R.T.: -0.003 min
Response: 573571
Conc: 4.44 ug/ml

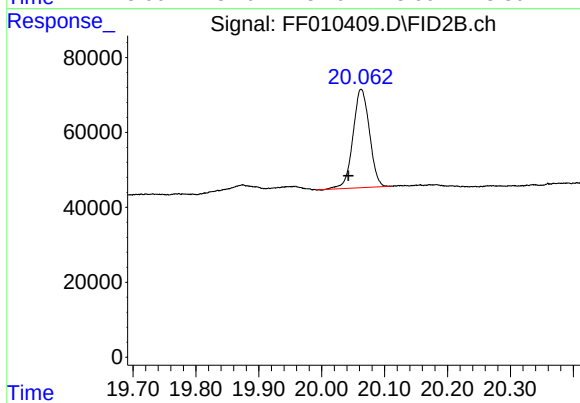

#16 N-HEXATRIACONTANE

R.T.: 20.063 min
Delta R.T.: 0.020 min
Response: 478120
Conc: 4.58 ug/ml

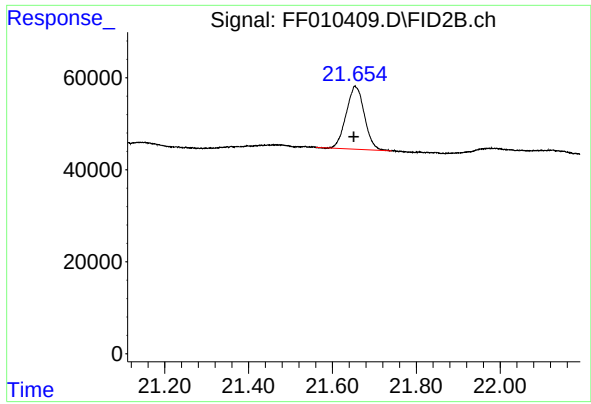

#18 N-TETRACONTANE

R.T.: 21.654 min
Delta R.T.: 0.003 min
Response: 412070
Conc: 4.70 ug/ml

Instrument :
FID_F
ClientSampleId :