

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042722\
Data File : FF010410.D
Signal(s) : FID2B.ch
Acq On : 27 Apr 2022 12:03
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 28 02:12:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.612	2285813	19.124 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.669	130174	0.986 ug/ml
14) N-DOTRIACONTANE	18.501	183522	1.422 ug/ml
15) N-TETRATRIACONTANE	19.284	100175	0.861 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF042722\
Data File : FF010410.D
Signal(s) : FID2B.ch
Acq On : 27 Apr 2022 12:03
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 28 02:12:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

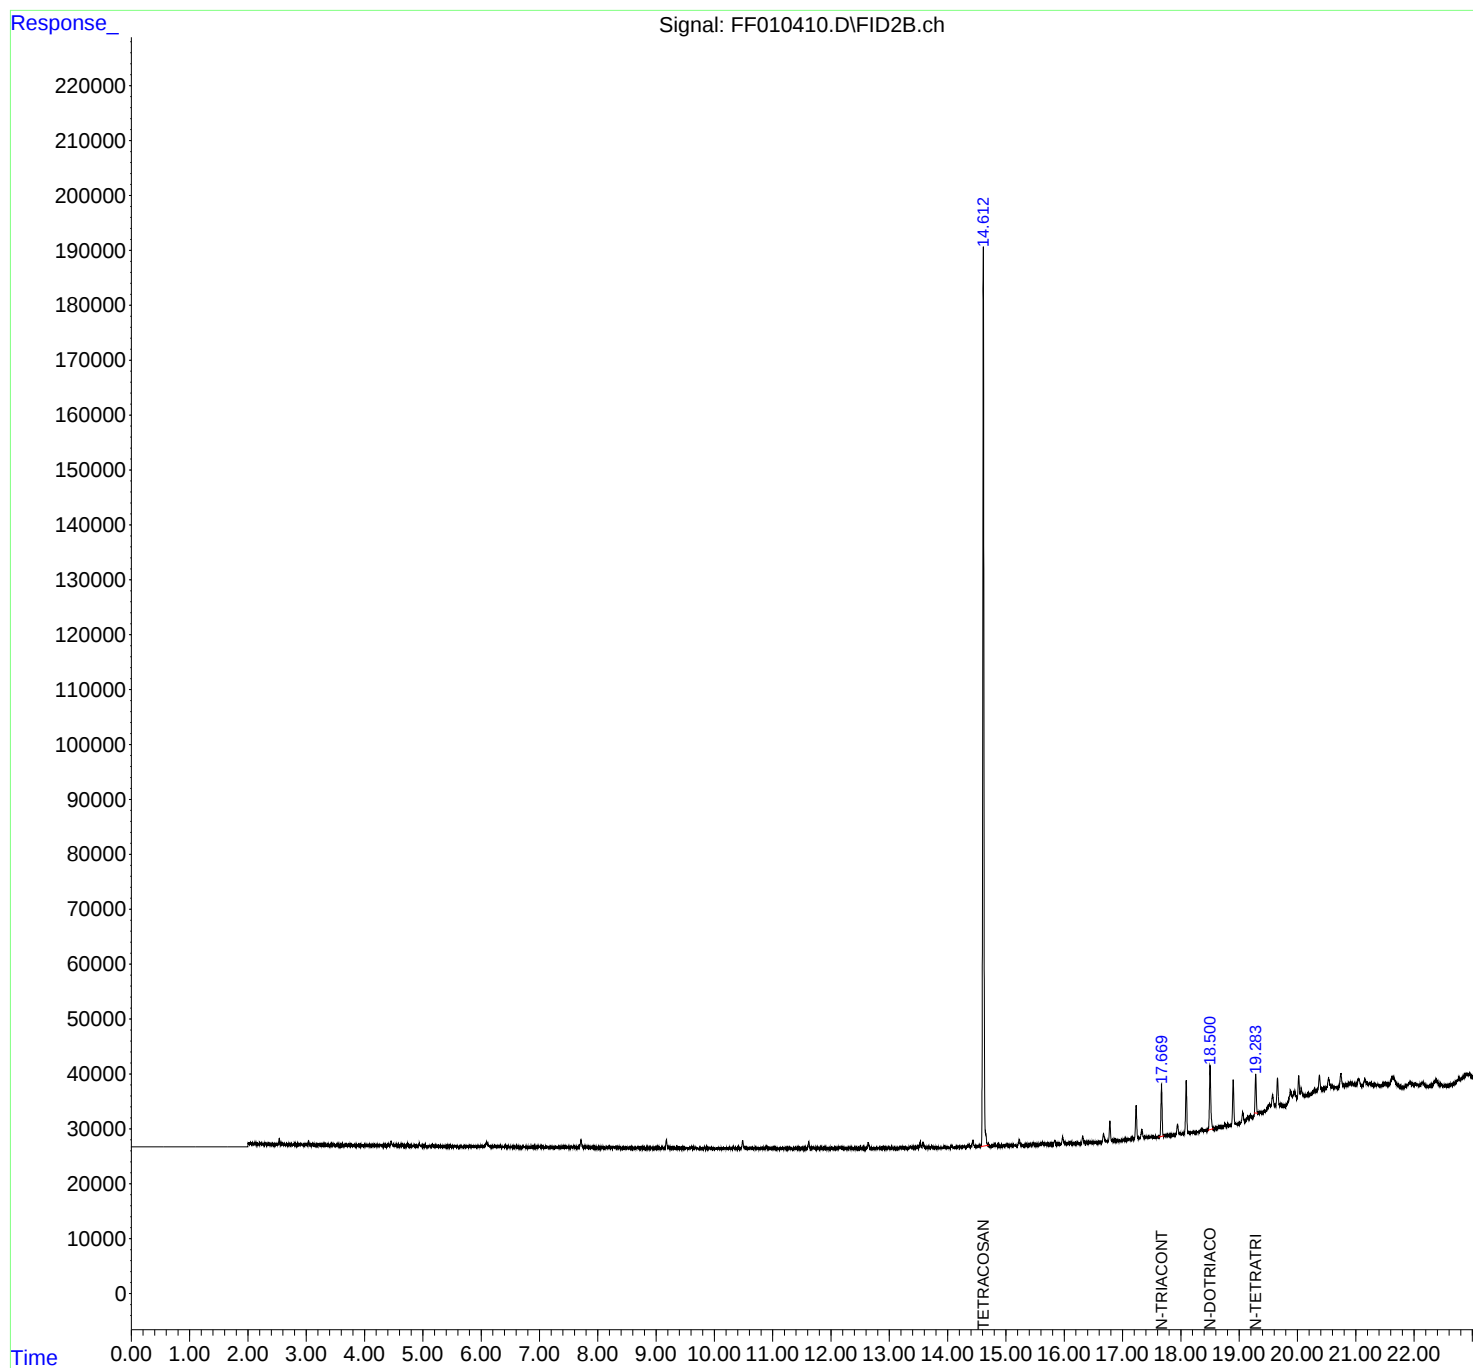


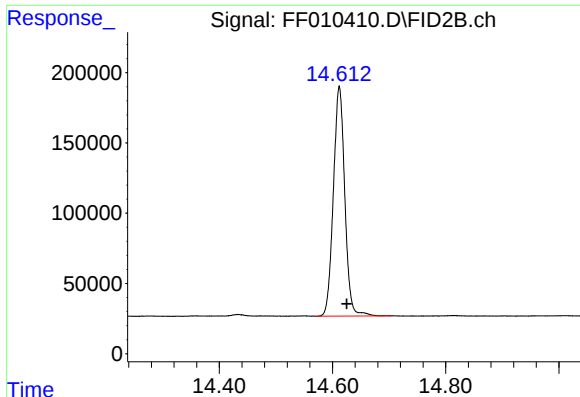

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.612 min
Delta R.T.: -0.013 min
Response: 2285813
Conc: 19.12 ug/ml

Instrument :
FID_F
ClientSampleId :

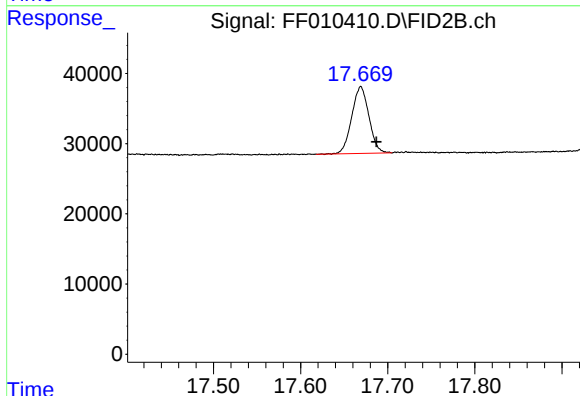


#13 N-TRIACONTANE

R.T.: 17.669 min
Delta R.T.: -0.018 min
Response: 130174
Conc: 0.99 ug/ml

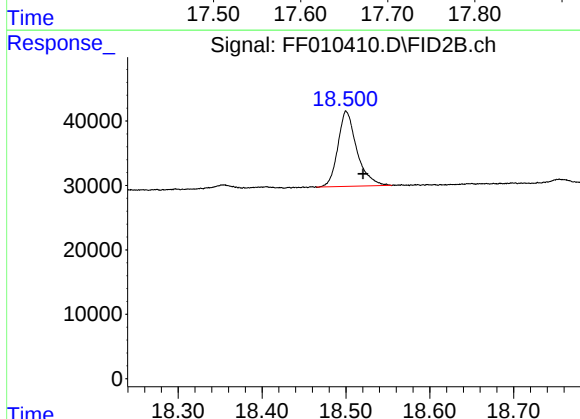

#14 N-DOTRIACONTANE

R.T.: 18.501 min
Delta R.T.: -0.019 min
Response: 183522
Conc: 1.42 ug/ml

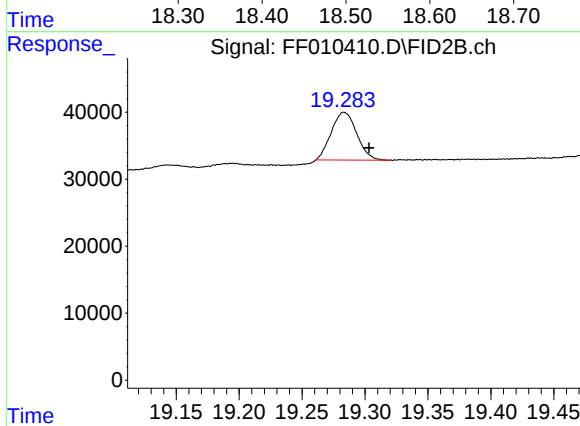

#15 N-TETRATRIACONTANE

R.T.: 19.284 min
Delta R.T.: -0.020 min
Response: 100175
Conc: 0.86 ug/ml