

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF042722\  
 Data File : FF010423.D  
 Signal(s) : FID2B.ch  
 Acq On : 27 Apr 2022 20:25  
 Operator : AJ\MA  
 Sample : N2577-01  
 Misc :  
 ALS Vial : 63 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Apr 28 02:14:28 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF040122.M  
 Quant Title :  
 QLast Update : Fri Apr 01 11:58:56 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.609 | 1902648  | 15.918 ug/ml |
| Target Compounds              |        |          |              |
| 2) N-DECANE                   | 4.344  | 477992   | 3.595 ug/ml  |
| 3) N-DODECANE                 | 6.390  | 1726681  | 12.968 ug/ml |
| 4) N-TETRADECANE              | 8.150  | 2122776  | 16.010 ug/ml |
| 5) N-HEXADECANE               | 9.720f | 632380   | 4.763 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF042722\  
Data File : FF010423.D  
Signal(s) : FID2B.ch  
Acq On : 27 Apr 2022 20:25  
Operator : AJ\MA  
Sample : N2577-01  
Misc :  
ALS Vial : 63 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Apr 28 02:14:28 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF040122.M  
Quant Title :  
QLast Update : Fri Apr 01 11:58:56 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

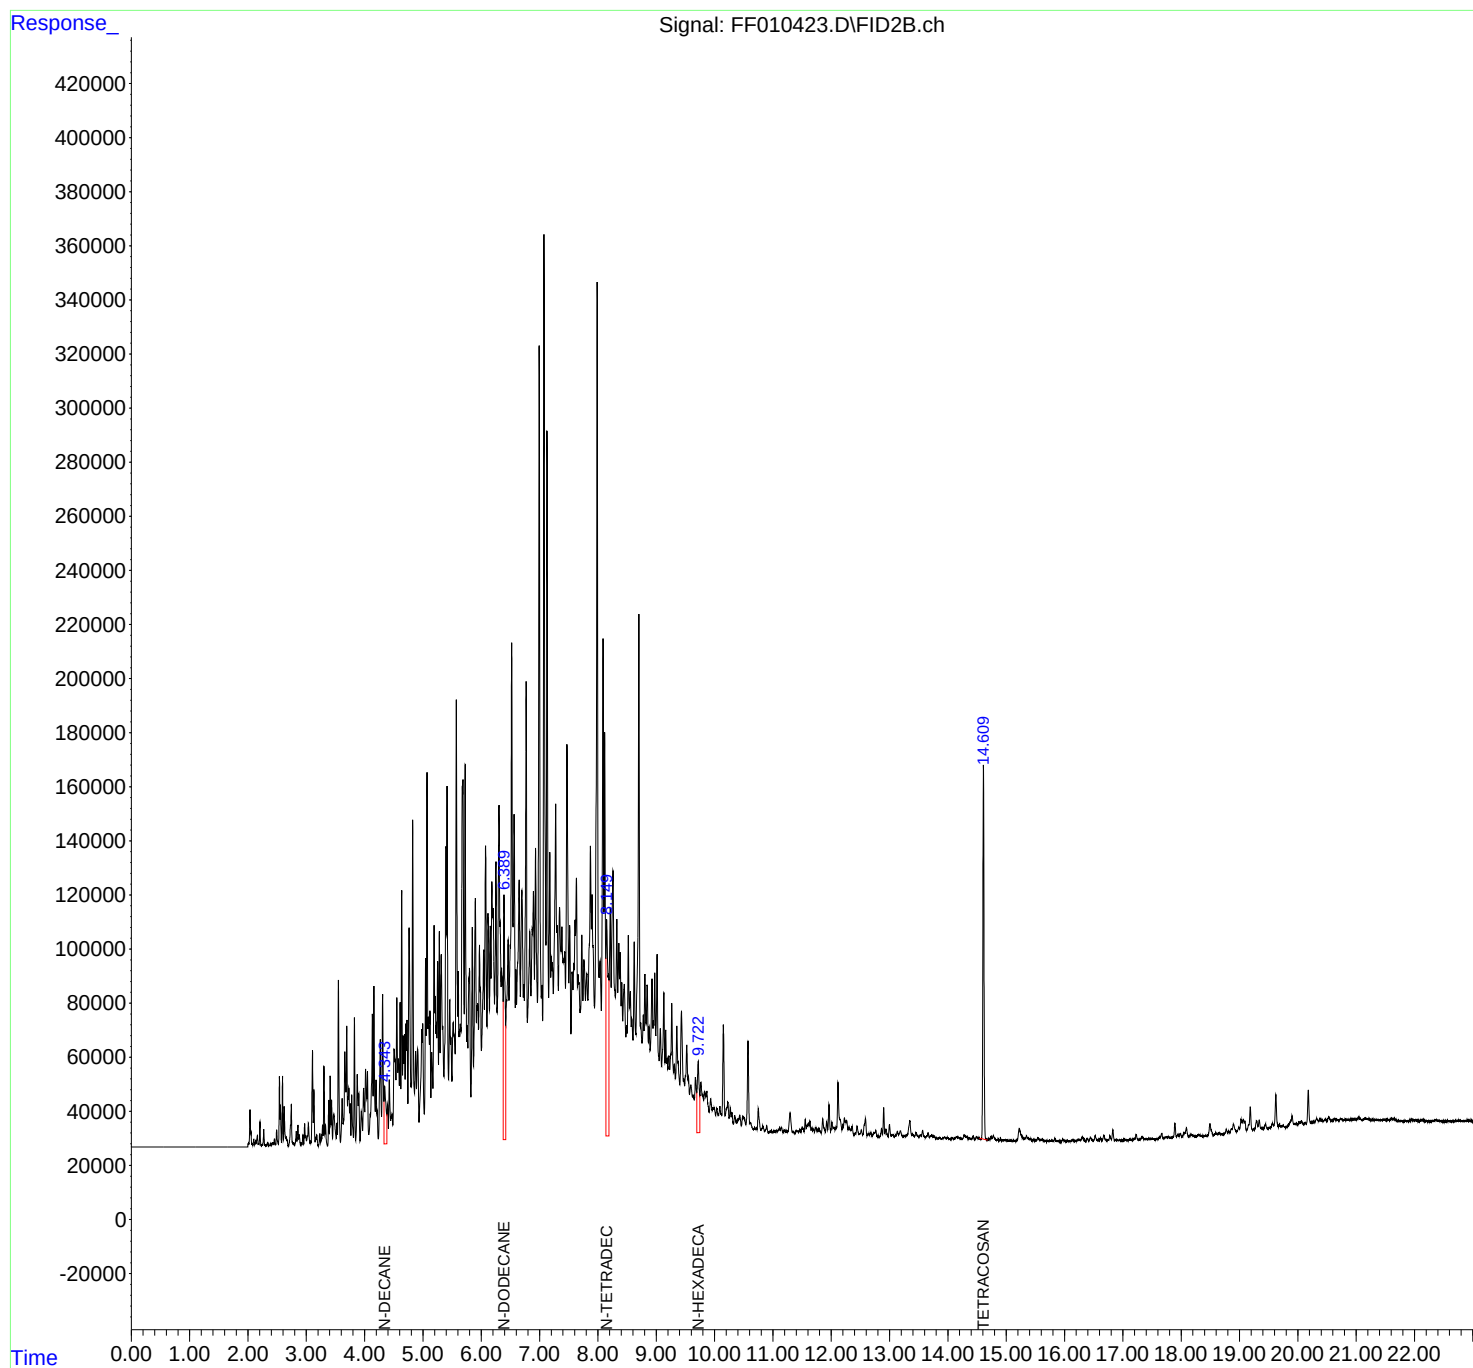


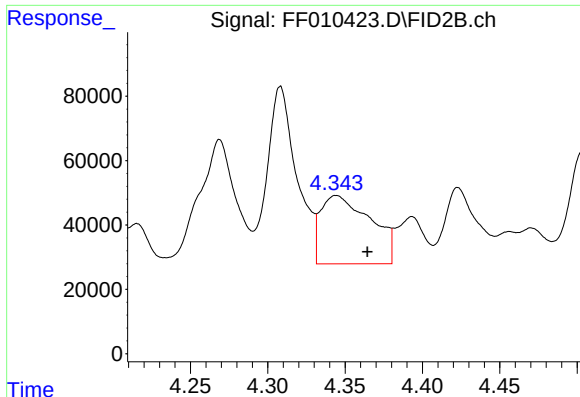

#2 N-DECANE


R.T.: 4.344 min  
Delta R.T.: -0.020 min  
Response: 477992  
Conc: 3.60 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

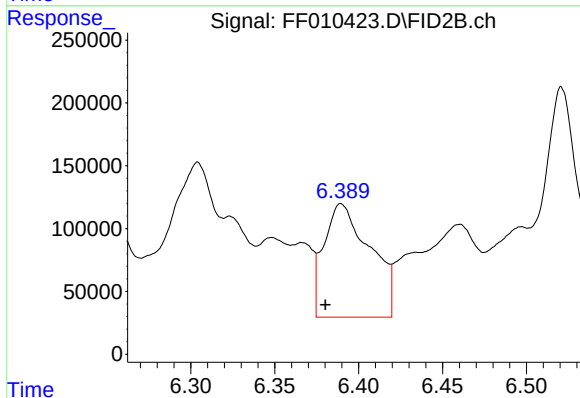


#3 N-DODECANE

R.T.: 6.390 min  
Delta R.T.: 0.010 min  
Response: 1726681  
Conc: 12.97 ug/ml

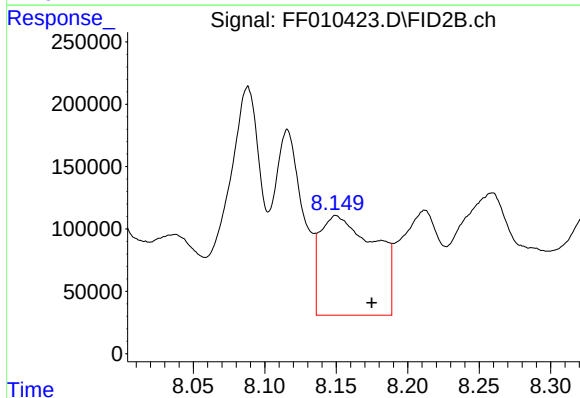


#4 N-TETRADECANE

R.T.: 8.150 min  
Delta R.T.: -0.024 min  
Response: 2122776  
Conc: 16.01 ug/ml

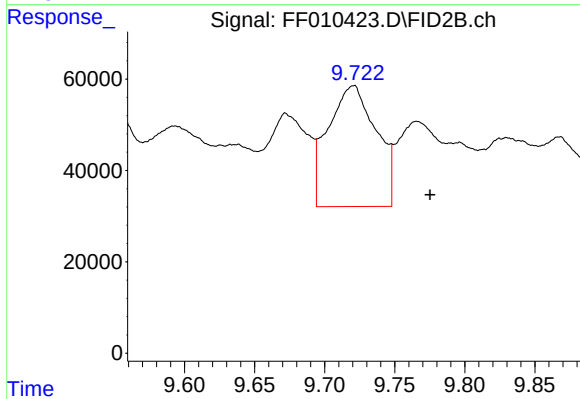

#5 N-HEXADECANE

R.T.: 9.720 min  
Delta R.T.: -0.055 min  
Response: 632380  
Conc: 4.76 ug/ml

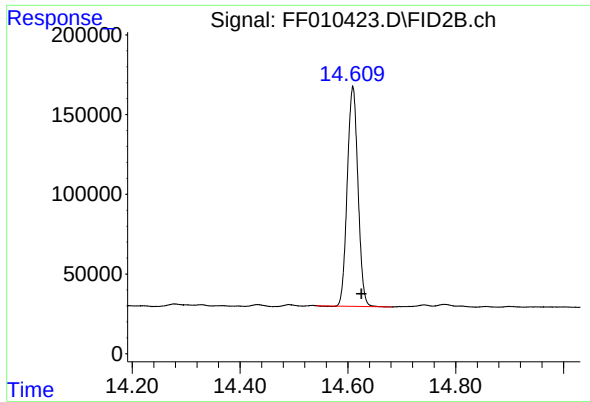

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.609 min  
Delta R.T.: -0.016 min  
Response: 1902648  
Conc: 15.92 ug/ml

Instrument :  
FID\_F  
ClientSampleId :