

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF042722\  
Data File : FF010427.D  
Signal(s) : FID2B.ch  
Acq On : 27 Apr 2022 22:25  
Operator : AJ\MA  
Sample : N2577-05  
Misc :  
ALS Vial : 67 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
BLIND-DUPLICATE-4-25-22

Integration File: Sample.e  
Quant Time: Apr 28 02:15:07 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF040122.M  
Quant Title :  
QLast Update : Fri Apr 01 11:58:56 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.609 | 2117980  | 17.719 ug/ml |
| Target Compounds              |        |          |              |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF042722\  
Data File : FF010427.D  
Signal(s) : FID2B.ch  
Acq On : 27 Apr 2022 22:25  
Operator : AJ\MA  
Sample : N2577-05  
Misc :  
ALS Vial : 67 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
BLIND-DUPLICATE-4-25-22

Integration File: Sample.e  
Quant Time: Apr 28 02:15:07 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF040122.M  
Quant Title :  
QLast Update : Fri Apr 01 11:58:56 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

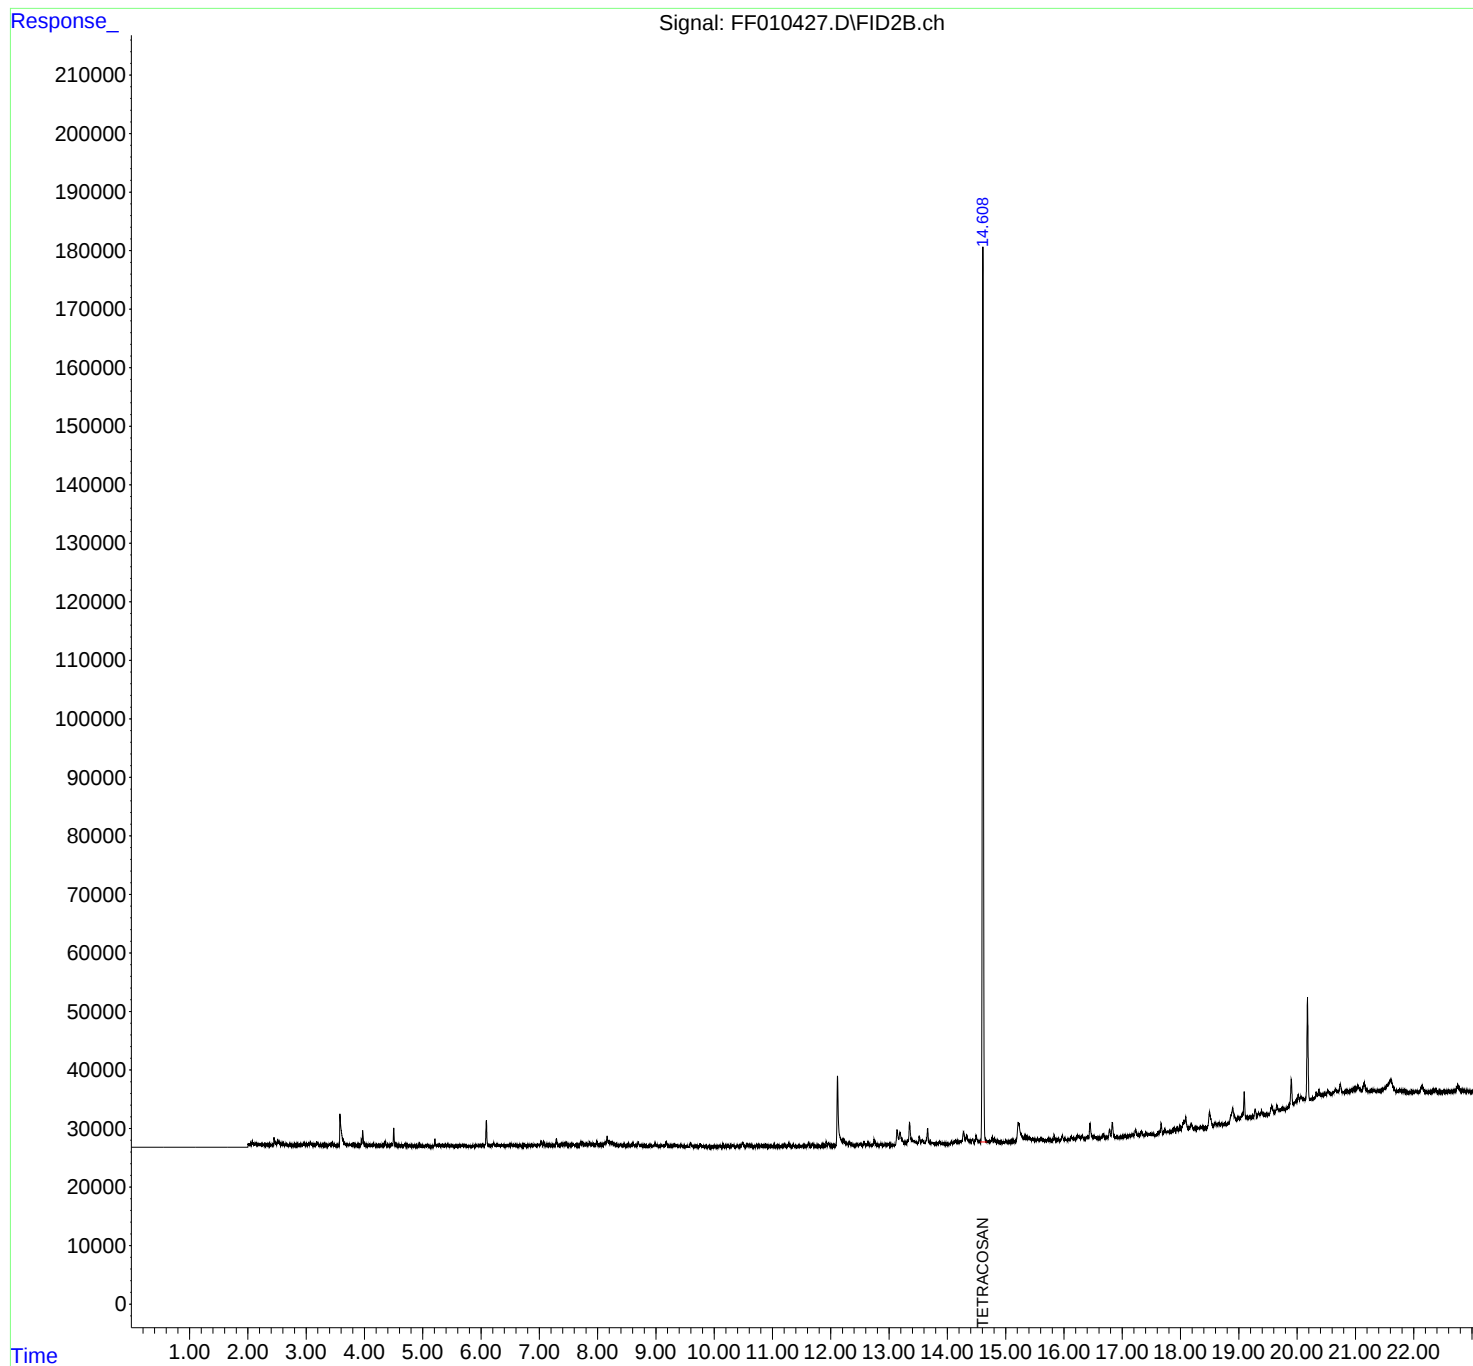

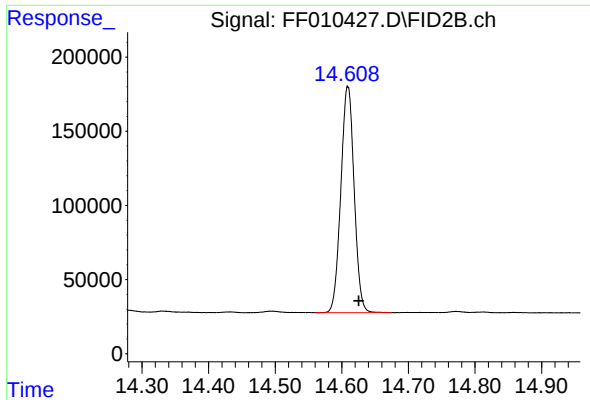

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.609 min  
Delta R.T.: -0.016 min  
Response: 2117980  
Conc: 17.72 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
BLIND-DUPLICATE-4-25-22