

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF042722\  
Data File : FF010430.D  
Signal(s) : FID2B.ch  
Acq On : 27 Apr 2022 23:55  
Operator : AJ\MA  
Sample : N2577-08  
Misc :  
ALS Vial : 70 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
GT-11-(15-20)

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/28/2022  
Supervised By :mohammad ahmed 04/29/2022

Integration File: Sample.e  
Quant Time: Apr 28 02:15:41 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF040122.M  
Quant Title :  
QLast Update : Fri Apr 01 11:58:56 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.607 | 1474835  | 12.339 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF042722\  
Data File : FF010430.D  
Signal(s) : FID2B.ch  
Acq On : 27 Apr 2022 23:55  
Operator : AJ\MA  
Sample : N2577-08  
Misc :  
ALS Vial : 70 Sample Multiplier: 1


Instrument :  
FID\_F  
ClientSampleId :  
GT-11-(15-20)


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/28/2022  
Supervised By :mohammad ahmed 04/29/2022

Integration File: Sample.e  
Quant Time: Apr 28 02:15:41 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF040122.M  
Quant Title :  
QLast Update : Fri Apr 01 11:58:56 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

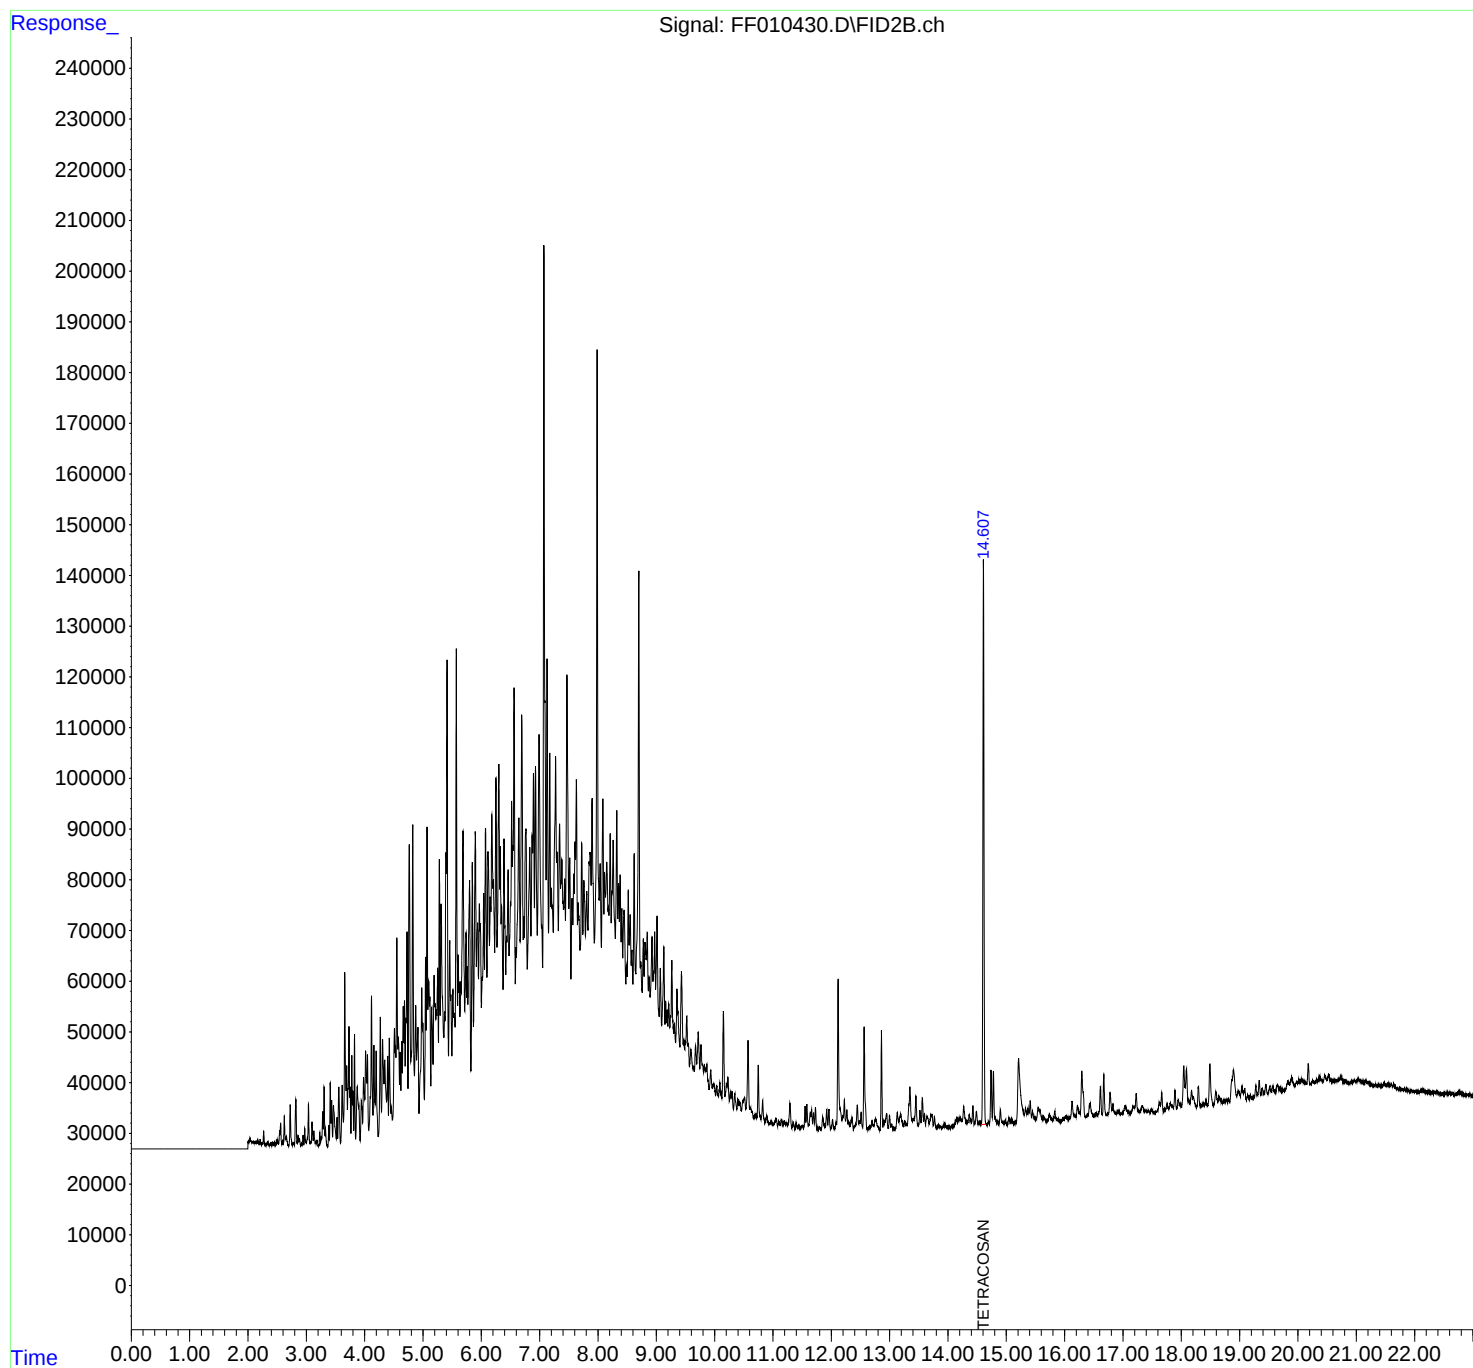

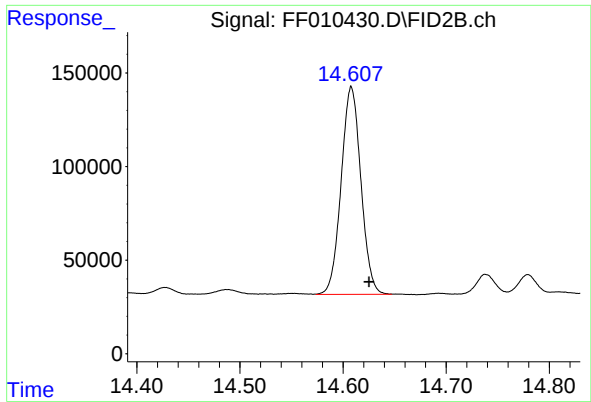

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.607 min  
Delta R.T.: -0.018 min  
Response: 1474835  
Conc: 12.34 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
GT-11-(15-20)

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/28/2022  
Supervised By :mohammad ahmed 04/29/2022