

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF043022\
Data File : FF010459.D
Signal(s) : FID2B.ch
Acq On : 29 Apr 2022 12:15
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 29 22:36:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
Quant Title :
QLast Update : Fri Apr 29 04:08:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.368	2286862	16.872 ug/ml
12) N-OCTACOSANE	16.780	2471151	18.793 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF043022\
Data File : FF010459.D
Signal(s) : FID2B.ch
Acq On : 29 Apr 2022 12:15
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 29 22:36:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
Quant Title :
QLast Update : Fri Apr 29 04:08:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

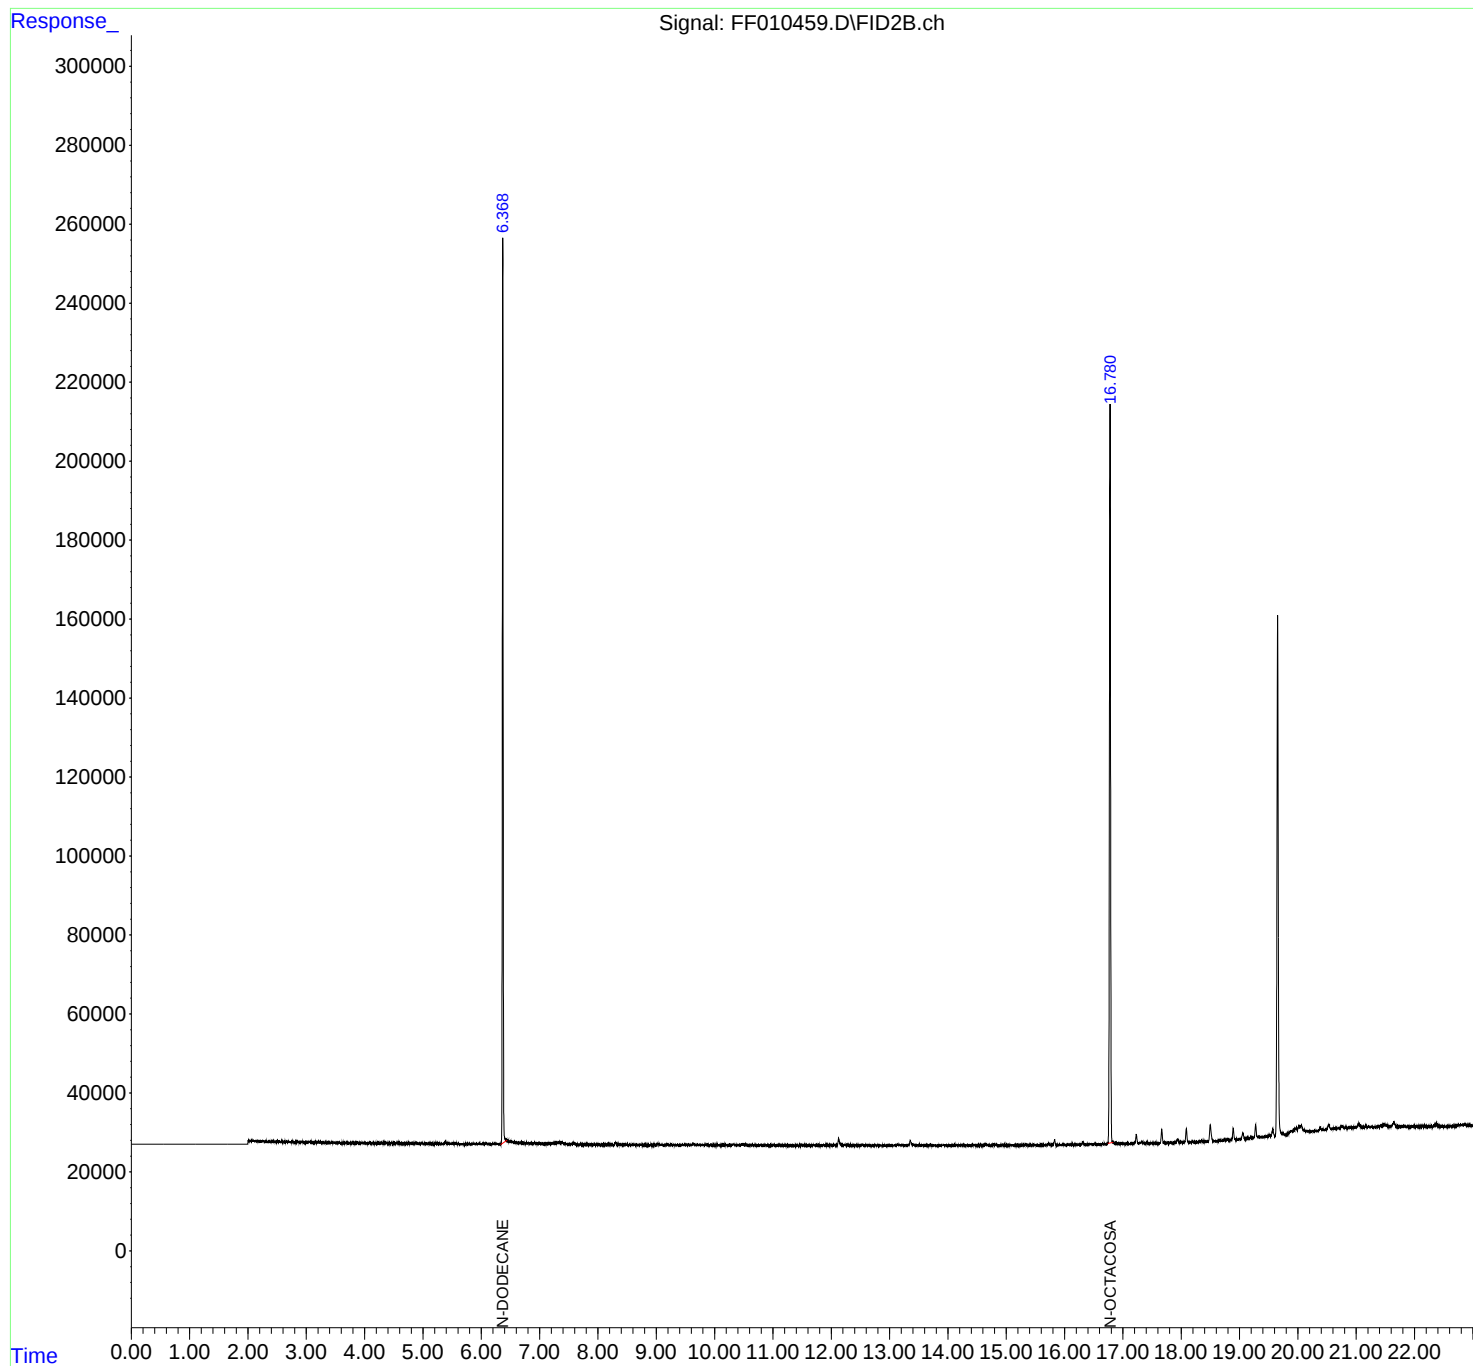


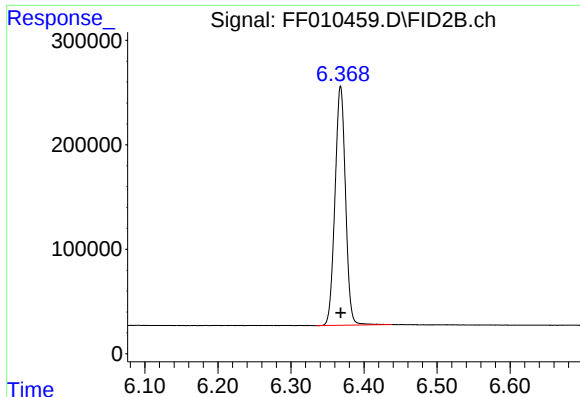

#3 N-DODECANE


R.T.: 6.368 min
Delta R.T.: 0.000 min
Response: 2286862
Conc: 16.87 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

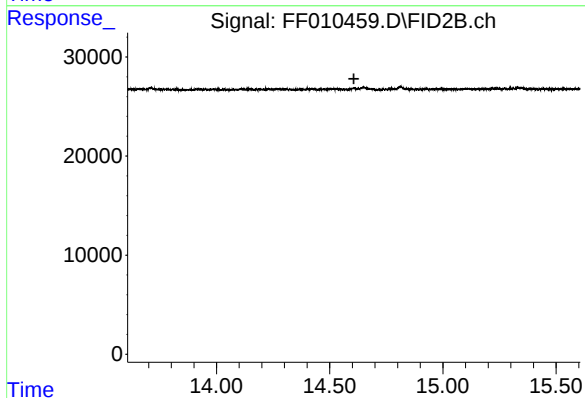

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.607 min
Response: 0
Conc: N.D.

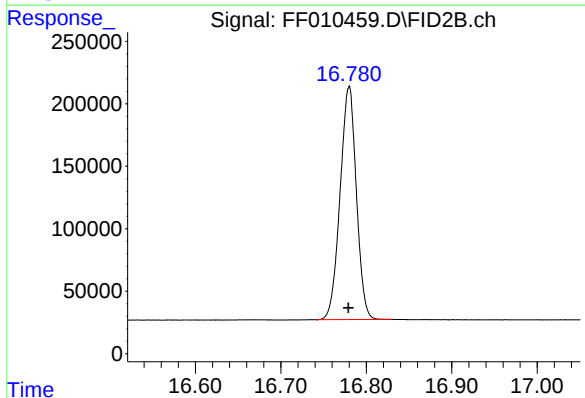

#12 N-OCTACOSANE

R.T.: 16.780 min
Delta R.T.: 0.000 min
Response: 2471151
Conc: 18.79 ug/ml