

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF043022\  
 Data File : FF010465.D  
 Signal(s) : FID2B.ch  
 Acq On : 29 Apr 2022 19:22  
 Operator : AJ\MA  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :  
 I.BLK

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 05/02/2022  
 Supervised By :mohammad ahmed 05/02/2022

Integration File: autoint1.e  
 Quant Time: Apr 29 22:37:17 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF042922.M  
 Quant Title :  
 QLast Update : Fri Apr 29 04:08:29 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.617 | 1877625  | 15.310 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF043022\  
Data File : FF010465.D  
Signal(s) : FID2B.ch  
Acq On : 29 Apr 2022 19:22  
Operator : AJ\MA  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1


Instrument :  
FID\_F  
ClientSampleId :  
I.BLK


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 05/02/2022  
Supervised By :mohammad ahmed 05/02/2022

Integration File: autoint1.e  
Quant Time: Apr 29 22:37:17 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF042922.M  
Quant Title :  
QLast Update : Fri Apr 29 04:08:29 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

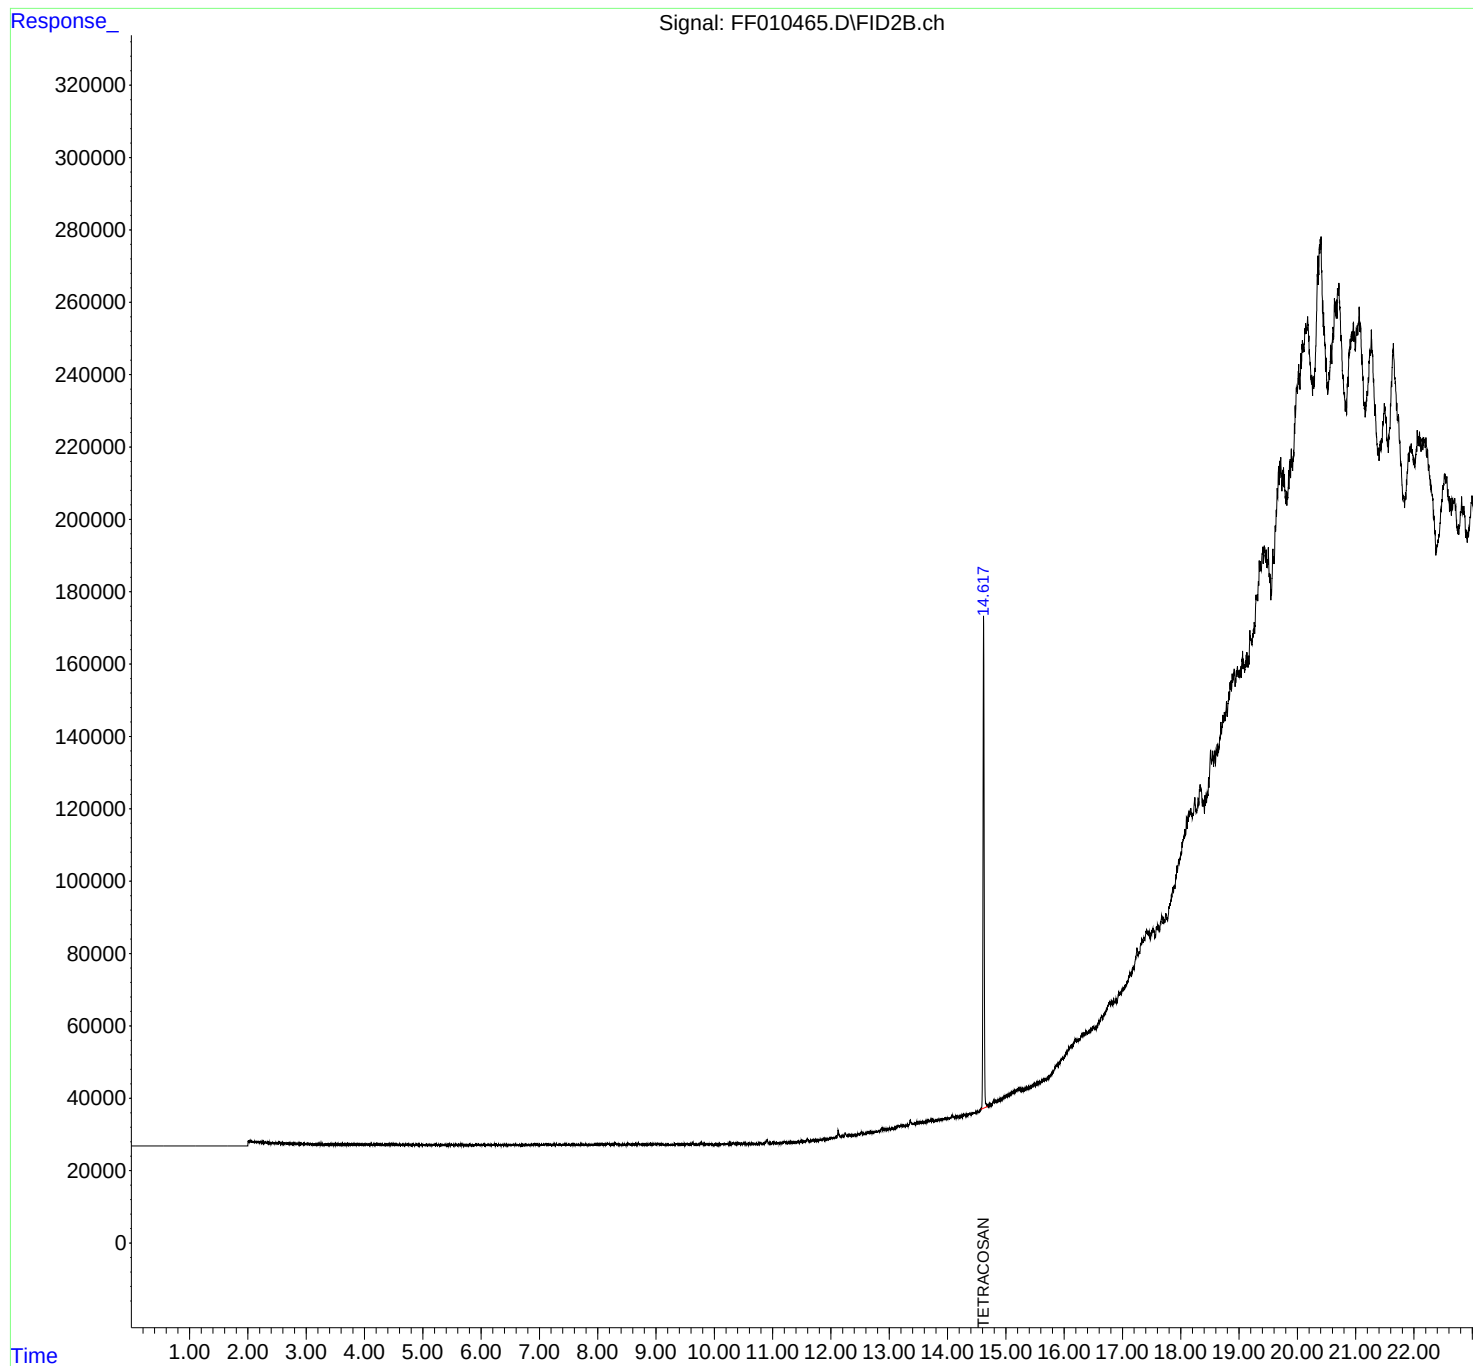

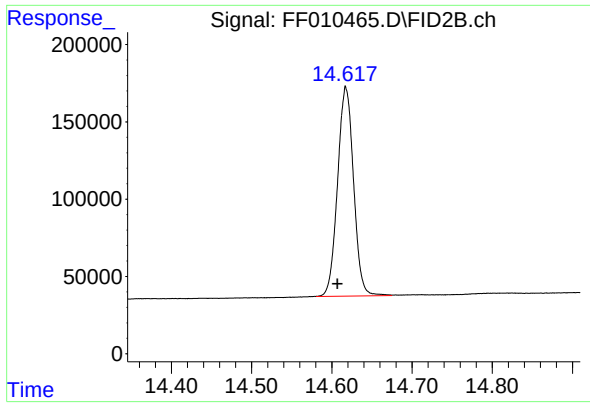

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.617 min  
Delta R.T.: 0.010 min  
Response: 1877625  
Conc: 15.31 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 05/02/2022  
Supervised By :mohammad ahmed 05/02/2022