

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050123\
Data File : FF012543.D
Signal(s) : FID2B.ch
Acq On : 01 May 2023 09:39
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 02 01:12:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
15) N-TETRATRIACONTANE	19.685	32223	0.284 ug/ml
16) N-HEXATRIACONTANE	20.438	50612	0.496 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050123\
Data File : FF012543.D
Signal(s) : FID2B.ch
Acq On : 01 May 2023 09:39
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 02 01:12:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

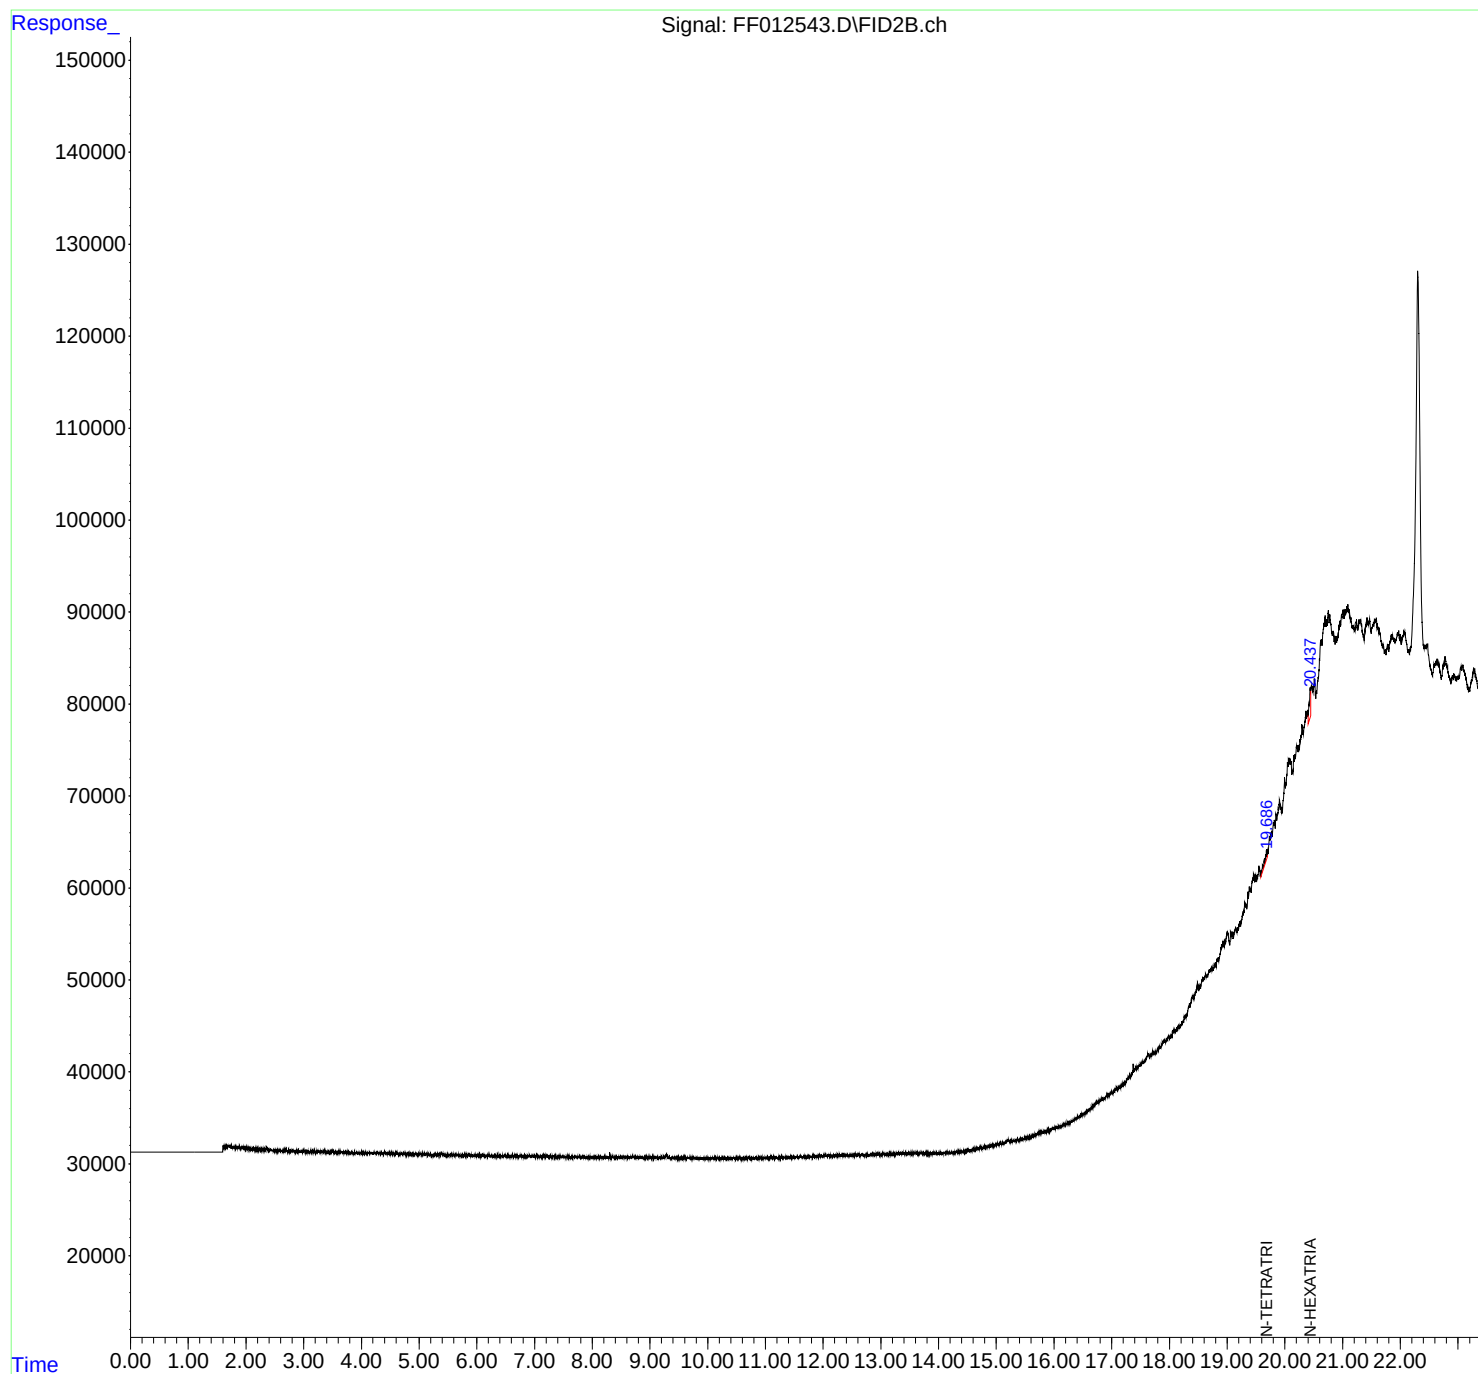


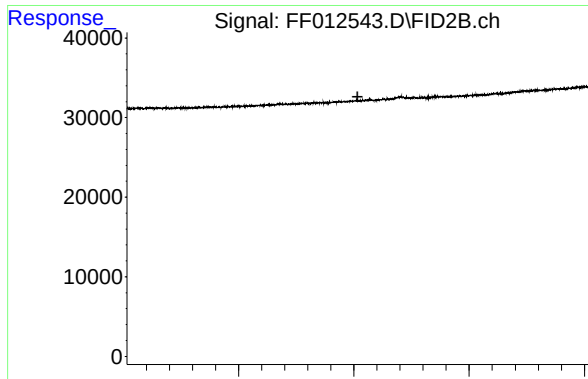

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.016 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

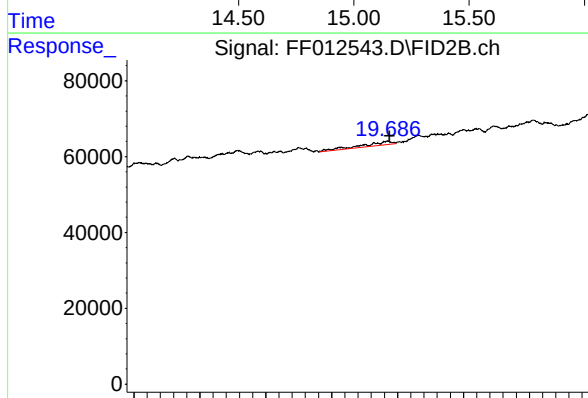

#15 N-TETRATRIACONTANE

R.T.: 19.685 min
Delta R.T.: -0.002 min
Response: 32223
Conc: 0.28 ug/ml

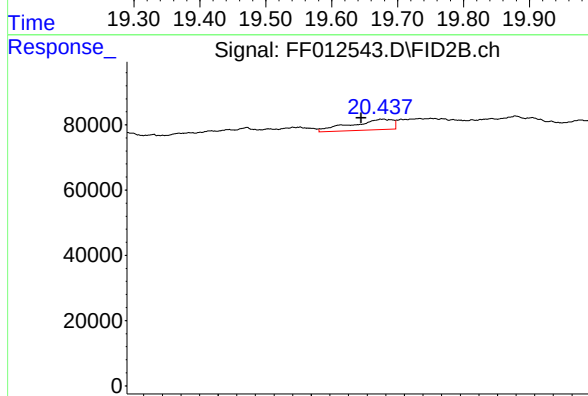

#16 N-HEXATRIACONTANE

R.T.: 20.438 min
Delta R.T.: 0.012 min
Response: 50612
Conc: 0.50 ug/ml