

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050123\
 Data File : FF012552.D
 Signal(s) : FID2B.ch
 Acq On : 01 May 2023 14:06
 Operator : YP\AJ
 Sample : 02416-11 5X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 02 01:13:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
 Quant Title :
 QLast Update : Thu Apr 13 15:26:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.009	316953	2.637 ug/ml
Target Compounds			
3) N-DODECANE	6.686f	56419	0.457 ug/ml
7) N-EICOSANE	12.909	68853	0.500 ug/ml
8) N-DOCOSANE	14.110	76207	0.566 ug/ml
10) N-TETRACOSANE	15.209	561123	4.148 ug/ml
11) N-HEXACOSANE	16.231	45936	0.345 ug/ml
12) N-OCTACOSANE	17.183	71468	0.542 ug/ml
13) N-TRIACONTANE	18.070	184513	1.414 ug/ml
14) N-DOTRIACONTANE	18.884	342491	2.715 ug/ml
15) N-TETRATRIACONTANE	19.684	108966	0.961 ug/ml
16) N-HEXATRIACONTANE	20.424	347747	3.405 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050123\
Data File : FF012552.D
Signal(s) : FID2B.ch
Acq On : 01 May 2023 14:06
Operator : YP\AJ
Sample : 02416-11 5X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 02 01:13:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

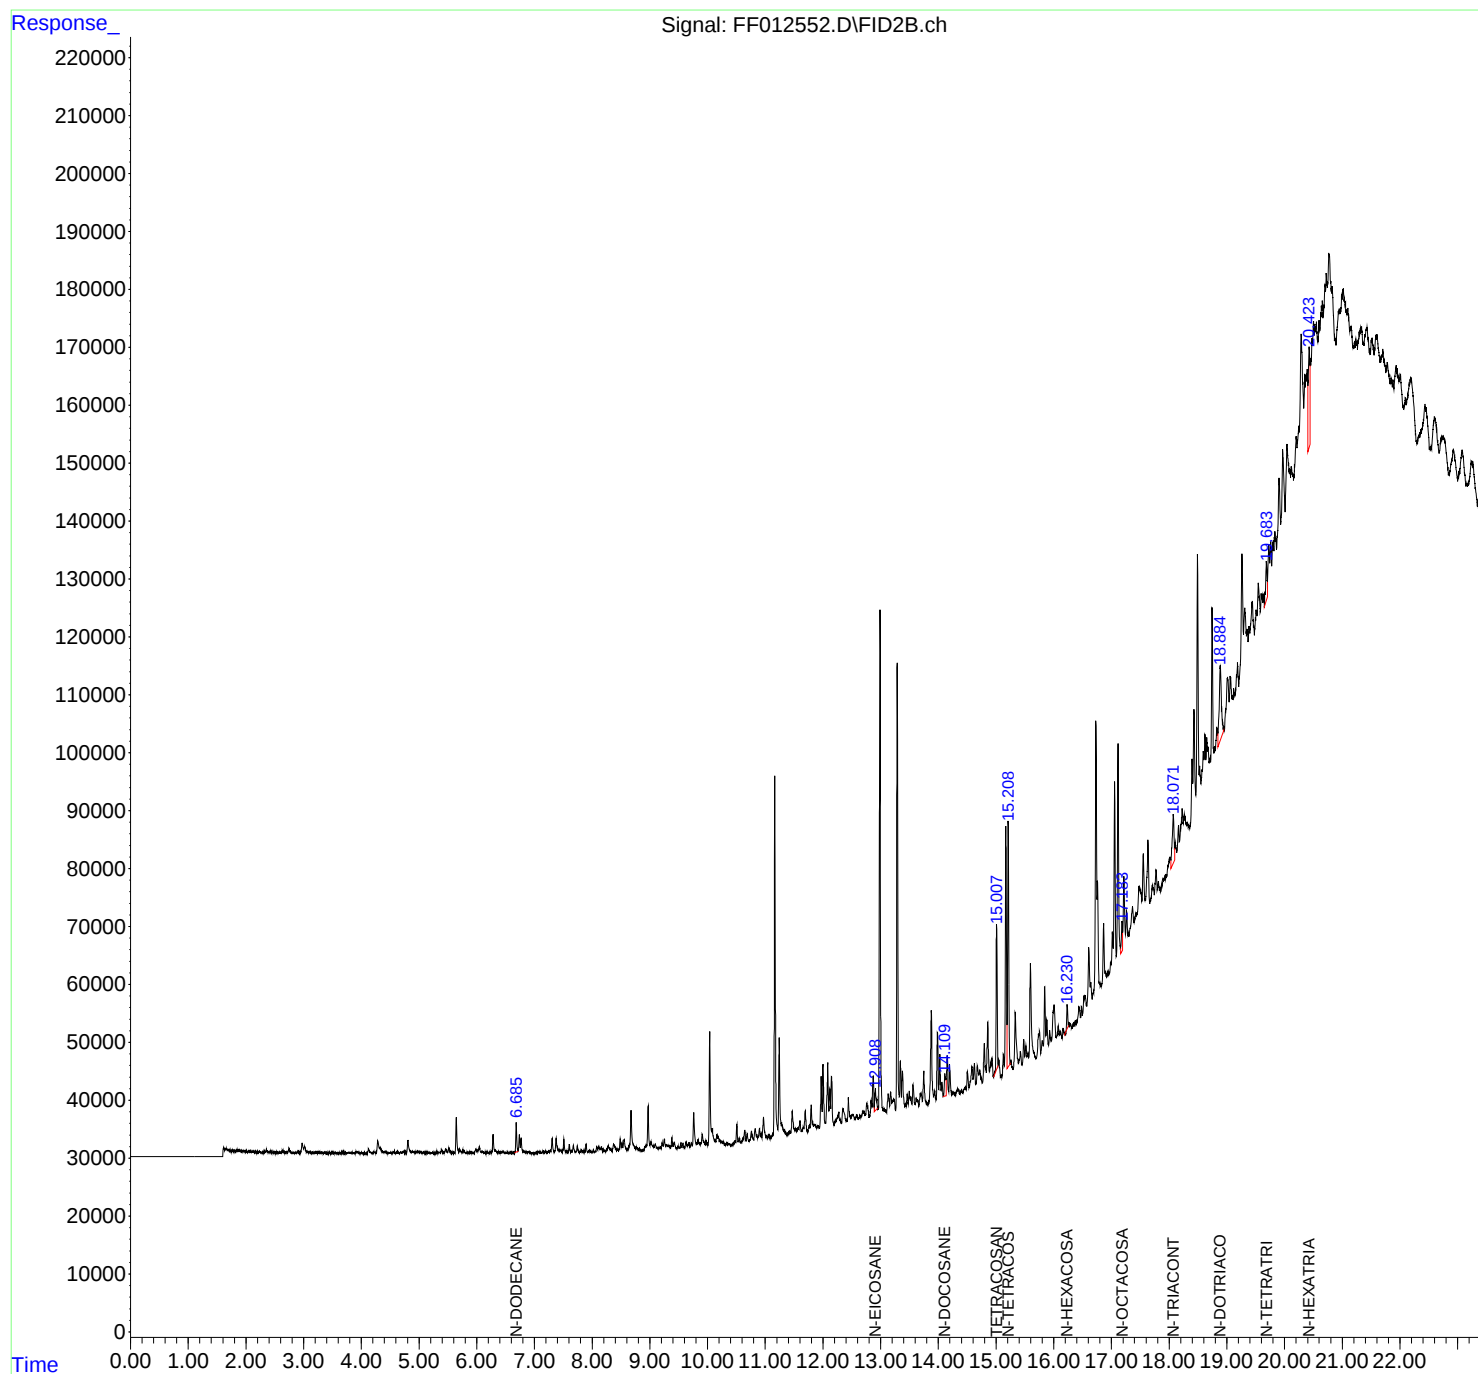


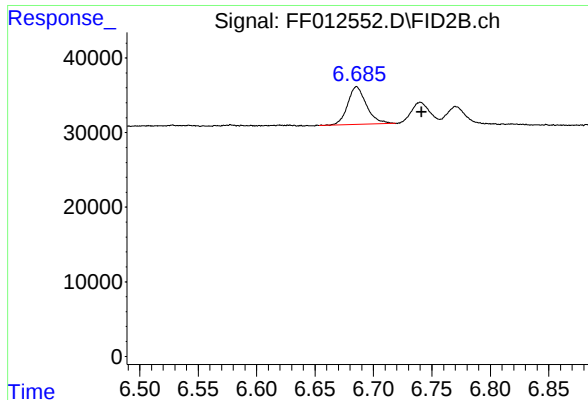

#3 N-DODECANE


R.T.: 6.686 min
Delta R.T.: -0.056 min
Response: 56419
Conc: 0.46 ug/ml

Instrument :
FID_F
ClientSampleId :

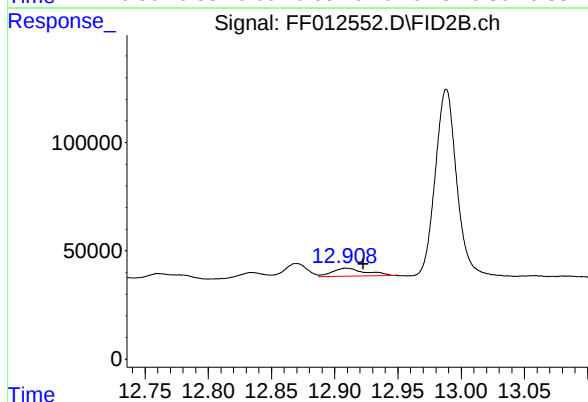


#7 N-EICOSANE

R.T.: 12.909 min
Delta R.T.: -0.014 min
Response: 68853
Conc: 0.50 ug/ml

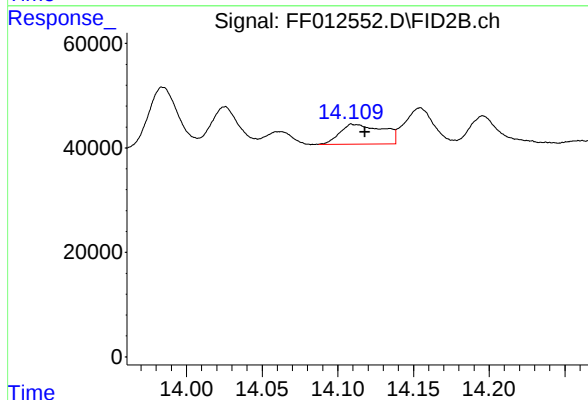


#8 N-DOCOSANE

R.T.: 14.110 min
Delta R.T.: -0.008 min
Response: 76207
Conc: 0.57 ug/ml

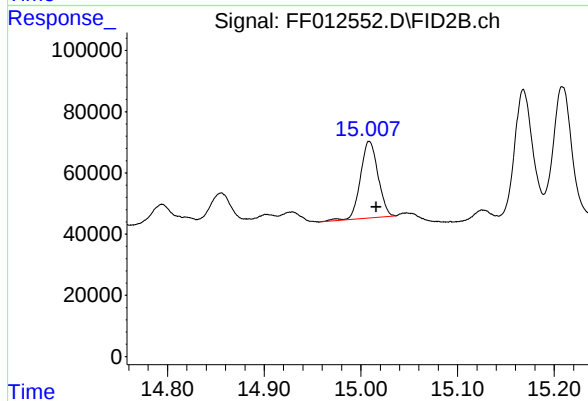

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.009 min
Delta R.T.: -0.007 min
Response: 316953
Conc: 2.64 ug/ml

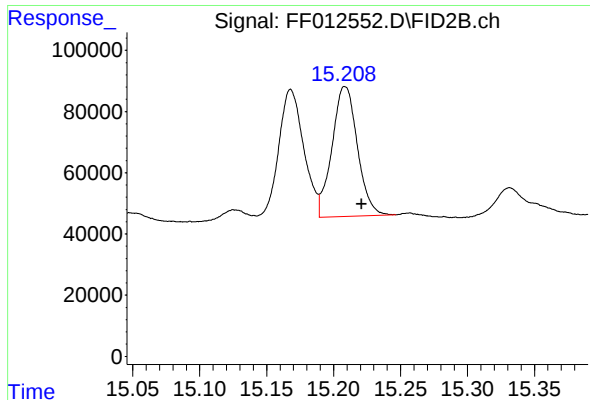

#10 N-TETRACOSANE


R.T.: 15.209 min
Delta R.T.: -0.012 min
Response: 561123
Conc: 4.15 ug/ml

Instrument :
FID_F
ClientSampleId :

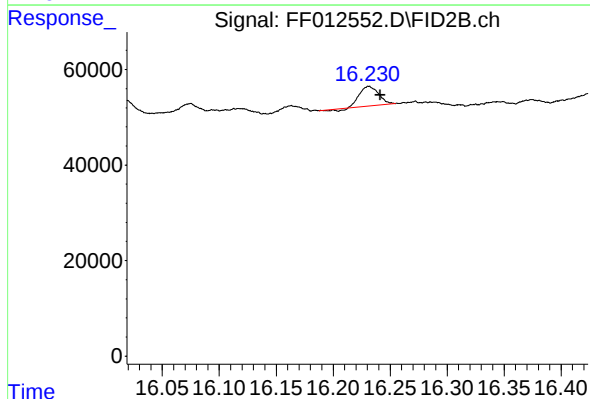


#11 N-HEXACOSANE

R.T.: 16.231 min
Delta R.T.: -0.010 min
Response: 45936
Conc: 0.34 ug/ml

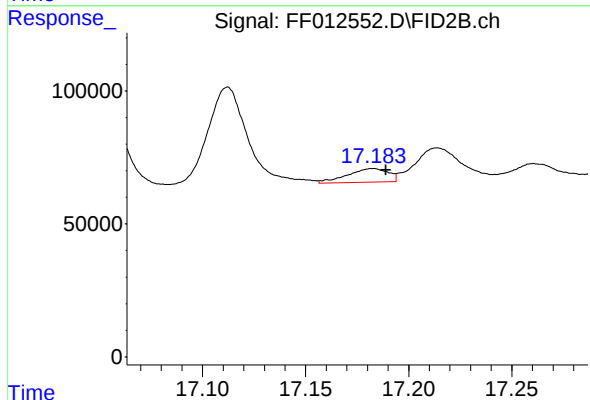


#12 N-OCTACOSANE

R.T.: 17.183 min
Delta R.T.: -0.006 min
Response: 71468
Conc: 0.54 ug/ml

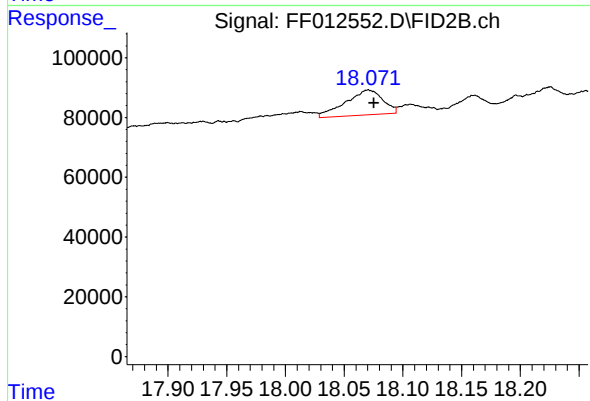

#13 N-TRIACONTANE

R.T.: 18.070 min
Delta R.T.: -0.005 min
Response: 184513
Conc: 1.41 ug/ml

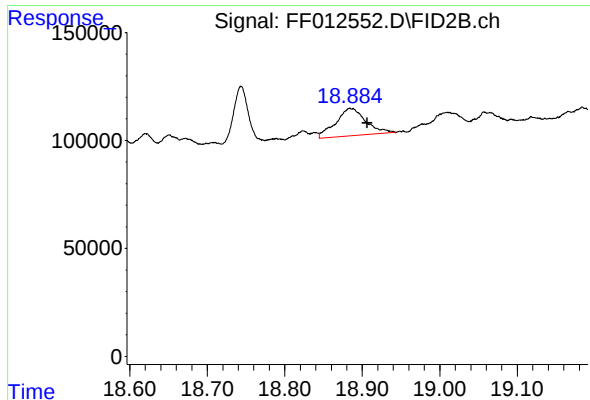


#14 N-DOTRIACONTANE

R.T.: 18.884 min
Delta R.T.: -0.023 min
Response: 342491
Conc: 2.71 ug/ml

Instrument :


FID_F

ClientSampleId :

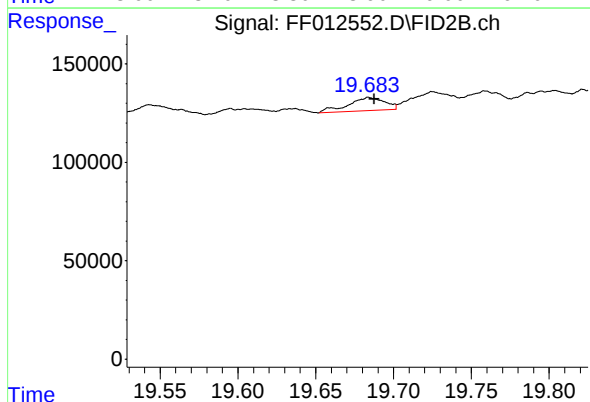

#15 N-TETRATRIACONTANE

R.T.: 19.684 min
Delta R.T.: -0.003 min
Response: 108966
Conc: 0.96 ug/ml

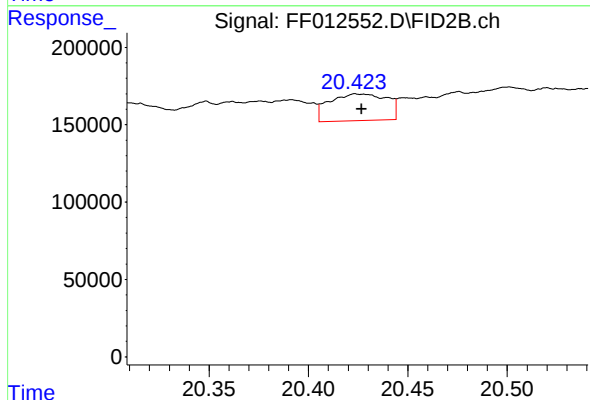

#16 N-HEXATRIACONTANE

R.T.: 20.424 min
Delta R.T.: -0.003 min
Response: 347747
Conc: 3.41 ug/ml