

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050123\
Data File : FF012549.D
Signal(s) : FID2B.ch
Acq On : 01 May 2023 12:38
Operator : YP\AJ
Sample : 02416-11
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
NATIONAL-GRID-COMP

Integration File: autoint1.e
Quant Time: May 02 01:13:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.007	1941359	16.151 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050123\
Data File : FF012549.D
Signal(s) : FID2B.ch
Acq On : 01 May 2023 12:38
Operator : YP\AJ
Sample : 02416-11
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
NATIONAL-GRID-COMP

Integration File: autoint1.e
Quant Time: May 02 01:13:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

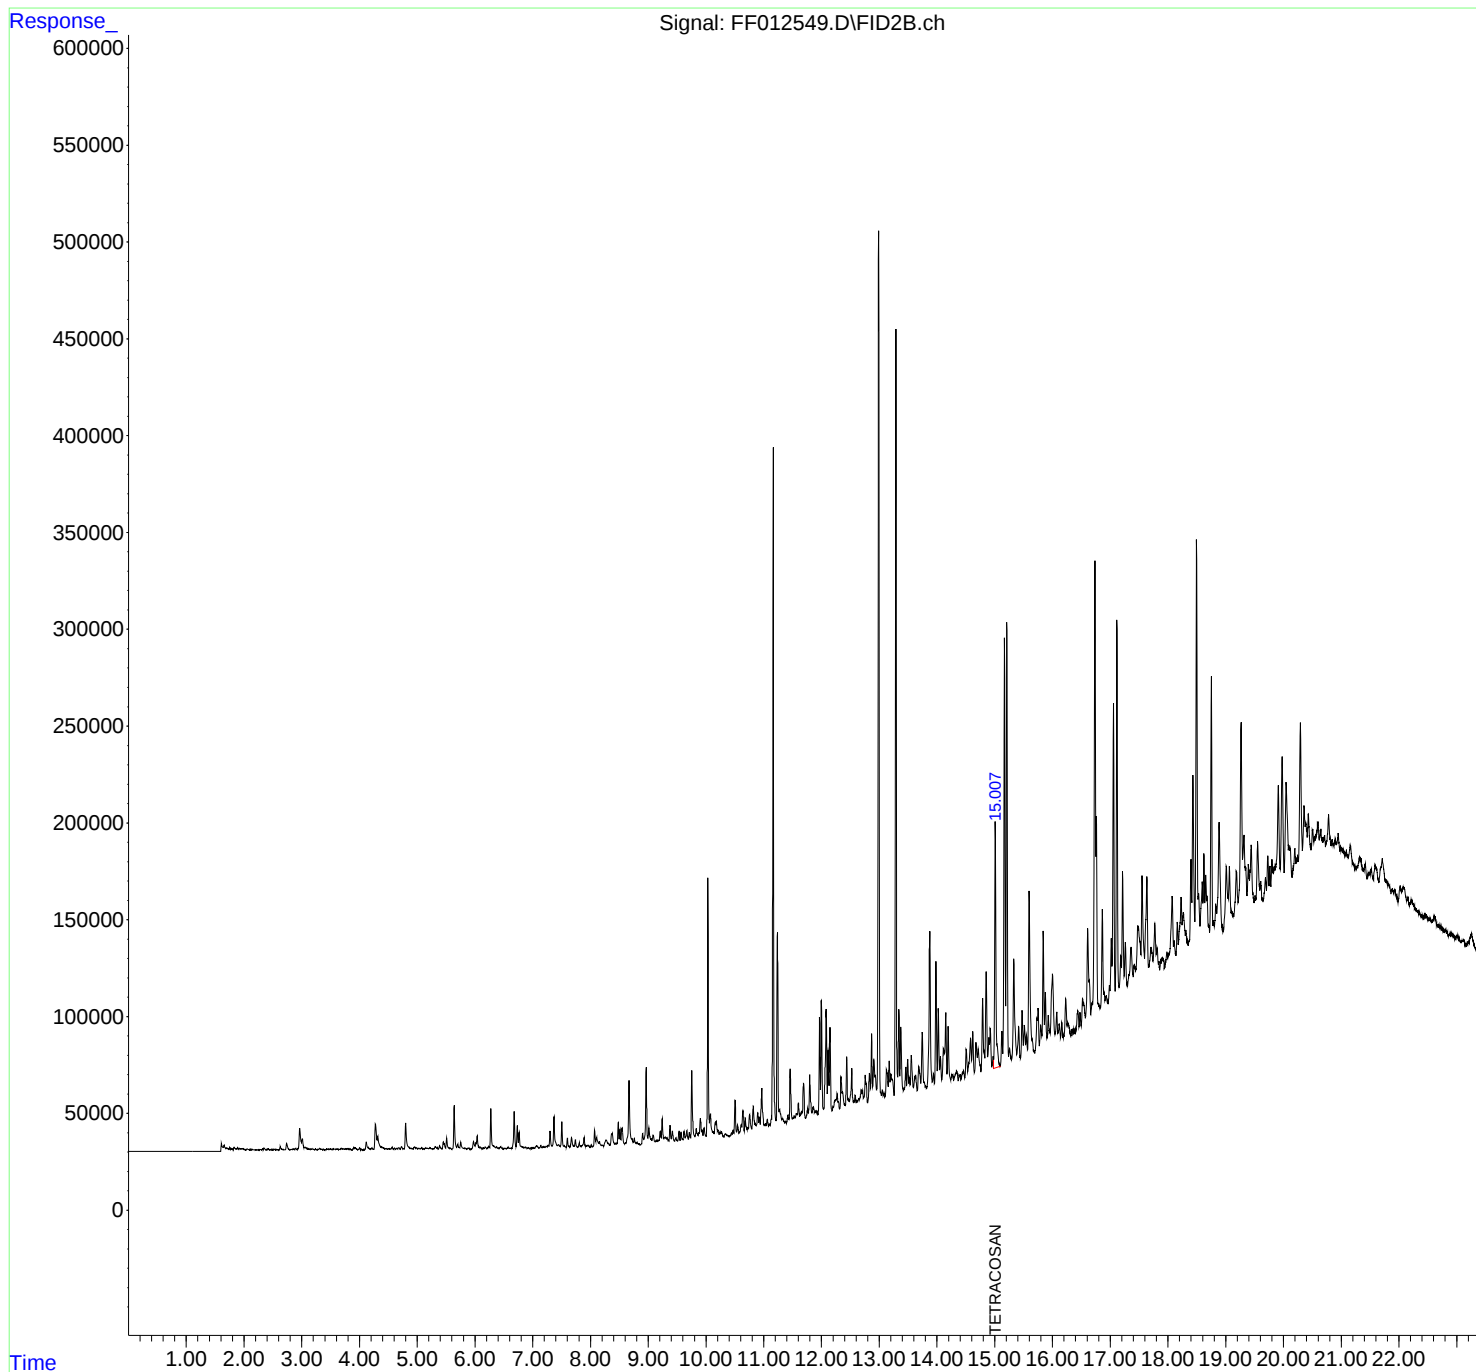

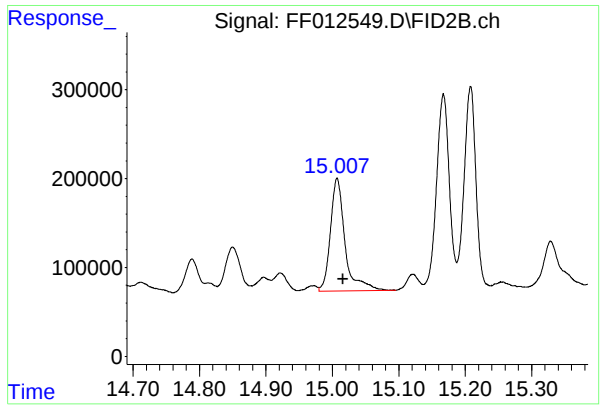

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.007 min
Delta R.T.: -0.009 min
Response: 1941359
Conc: 16.15 ug/ml

Instrument :
FID_F
ClientSampleId :
NATIONAL-GRID-COMP