

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050222\
 Data File : FF010467.D
 Signal(s) : FID2B.ch
 Acq On : 02 May 2022 11:25
 Operator : AJ\MA
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 03 01:30:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
 Quant Title :
 QLast Update : Fri Apr 29 04:08:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.590	297836	2.429 ug/ml
Target Compounds			
7) N-EICOSANE	12.488	232658	1.661 ug/ml
8) N-DOCOSANE	13.702	411656	2.964 ug/ml
10) N-TETRACOSANE	14.810	214999	1.556 ug/ml
11) N-HEXACOSANE	15.836	347400	2.567 ug/ml
12) N-OCTACOSANE	16.783	127743	0.971 ug/ml
13) N-TRIACONTANE	17.668	254266	2.000 ug/ml
14) N-DOTRIACONTANE	18.506	599397	4.997 ug/ml
15) N-TETRATRIACONTANE	19.283	445866	4.201 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050222\
Data File : FF010467.D
Signal(s) : FID2B.ch
Acq On : 02 May 2022 11:25
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 03 01:30:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
Quant Title :
QLast Update : Fri Apr 29 04:08:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

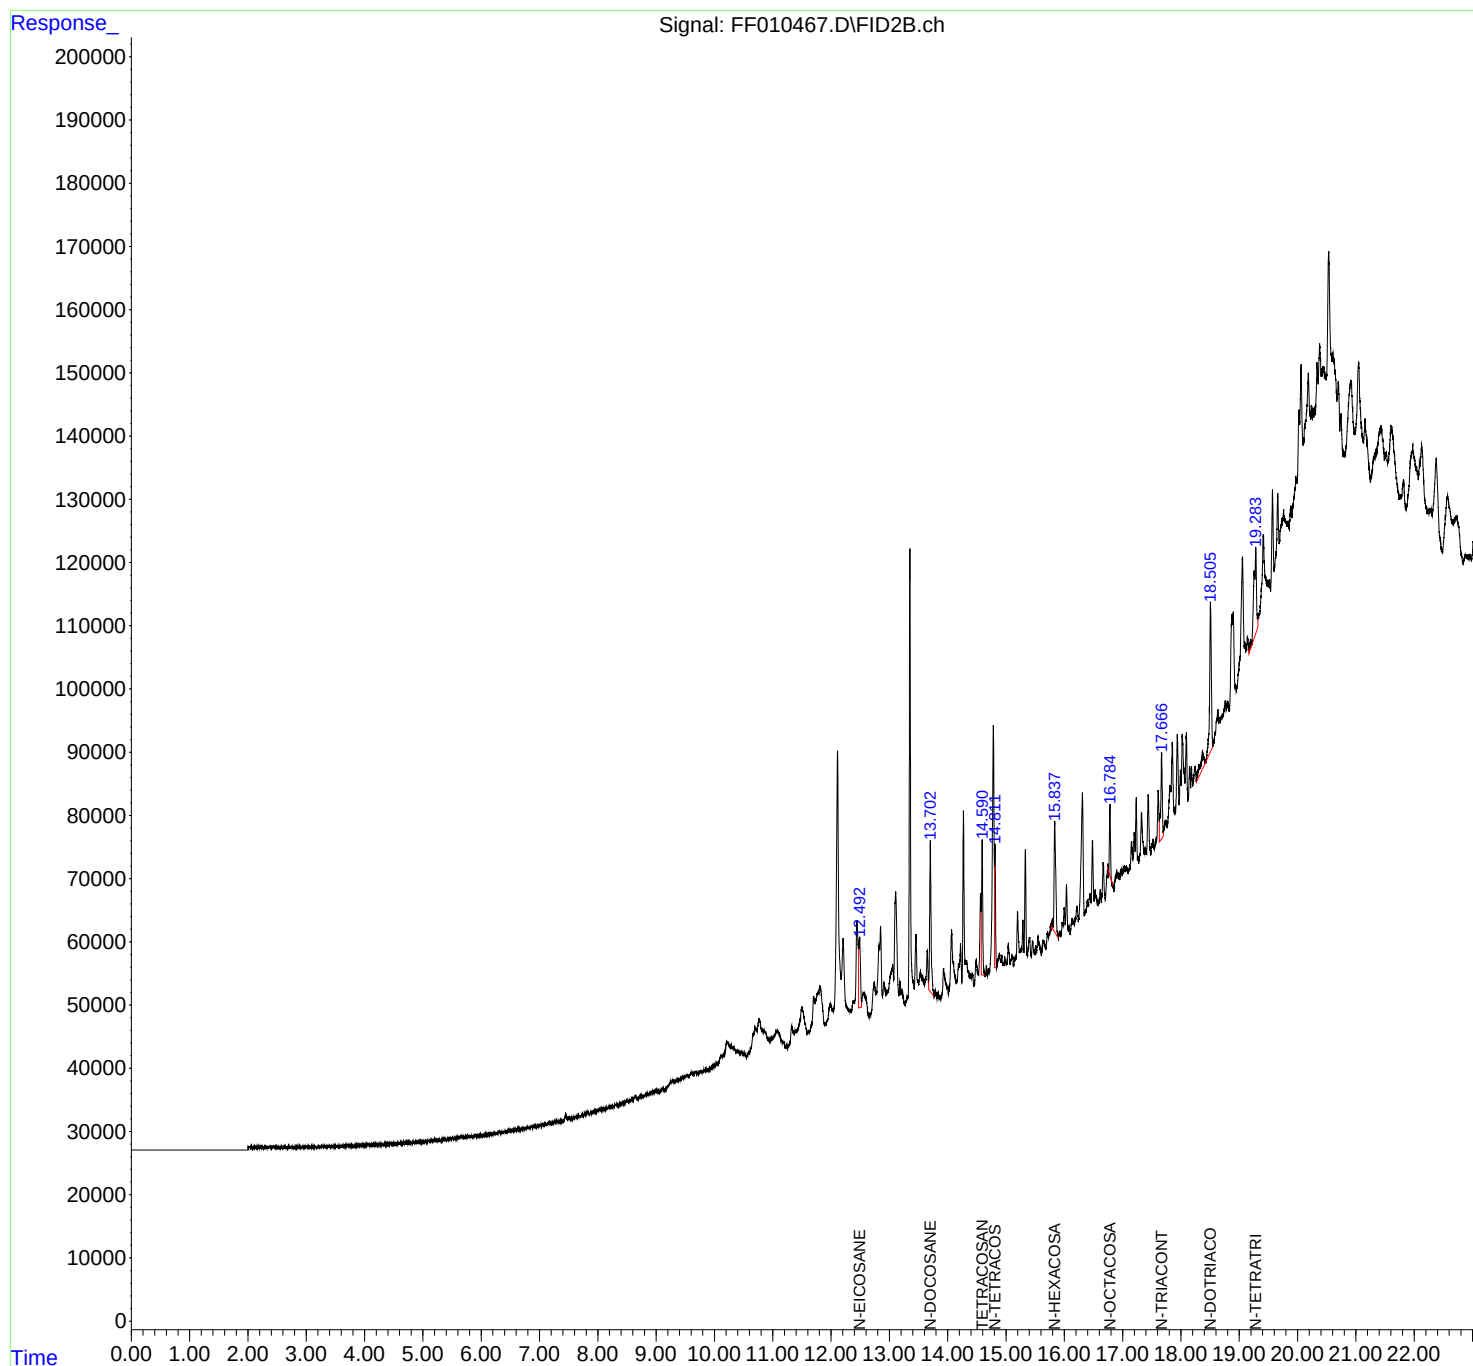


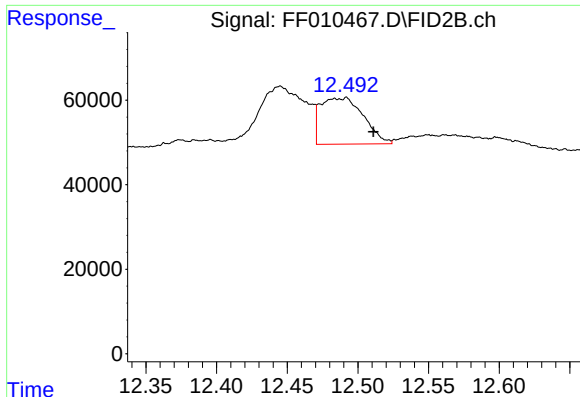

#7 N-EICOSANE


R.T.: 12.488 min
Delta R.T.: -0.023 min
Response: 232658
Conc: 1.66 ug/ml

Instrument :
FID_F
ClientSampleId :

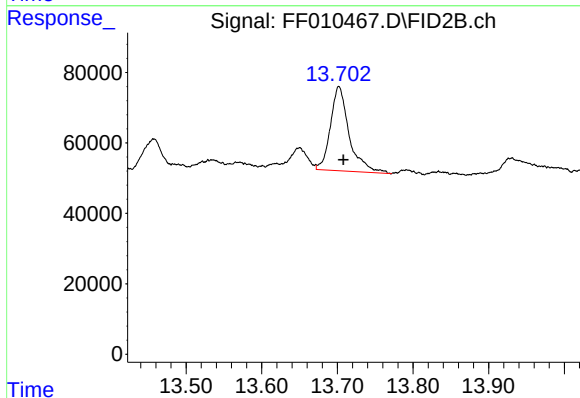


#8 N-DOCOSANE

R.T.: 13.702 min
Delta R.T.: -0.006 min
Response: 411656
Conc: 2.96 ug/ml

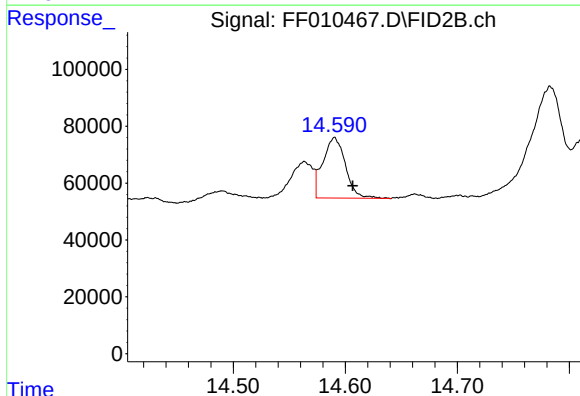


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.590 min
Delta R.T.: -0.016 min
Response: 297836
Conc: 2.43 ug/ml

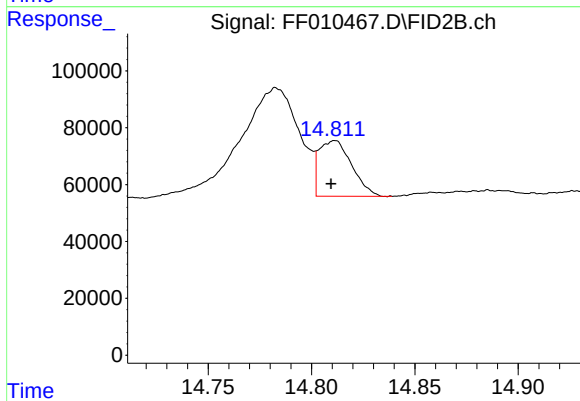

#10 N-TETRACOSANE


R.T.: 14.810 min
Delta R.T.: 0.000 min
Response: 214999
Conc: 1.56 ug/ml

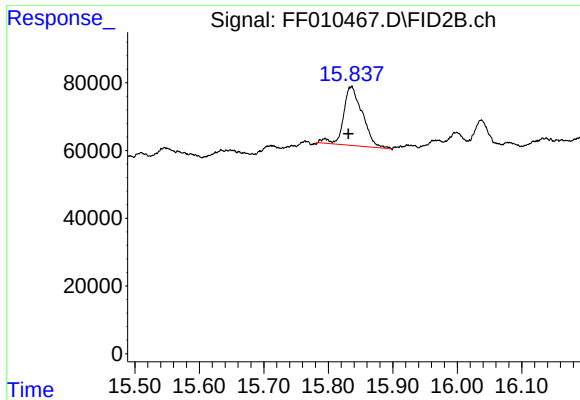

#11 N-HEXACOSANE


R.T.: 15.836 min
Delta R.T.: 0.005 min
Response: 347400
Conc: 2.57 ug/ml

Instrument :
FID_F
ClientSampleId :

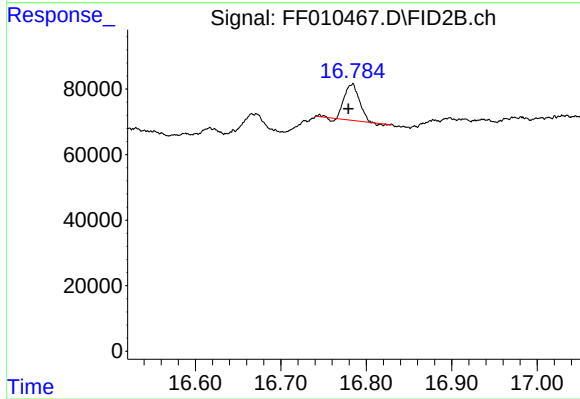


#12 N-OCTACOSANE

R.T.: 16.783 min
Delta R.T.: 0.004 min
Response: 127743
Conc: 0.97 ug/ml

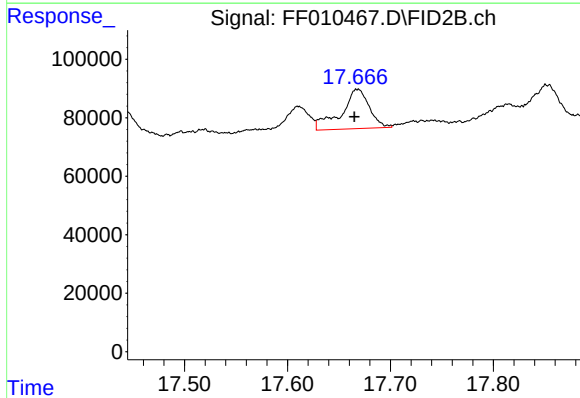


#13 N-TRIACONTANE

R.T.: 17.668 min
Delta R.T.: 0.003 min
Response: 254266
Conc: 2.00 ug/ml

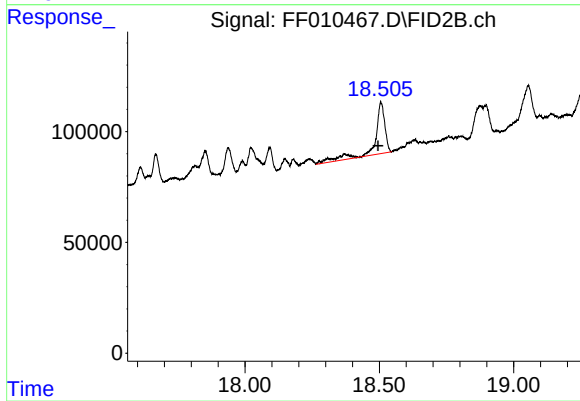

#14 N-DOTRIACONTANE

R.T.: 18.506 min
Delta R.T.: 0.010 min
Response: 599397
Conc: 5.00 ug/ml

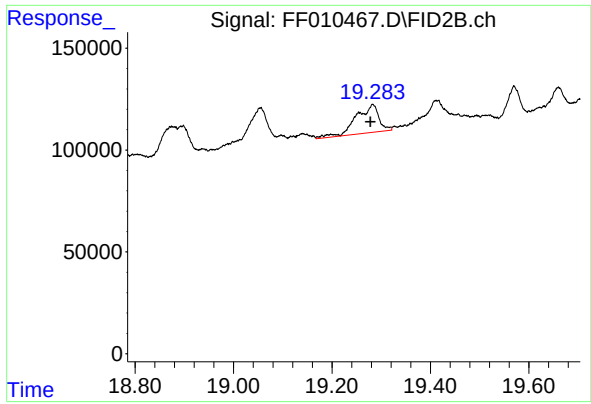

#15 N-TETRATRIACONTANE

R.T.: 19.283 min
Delta R.T.: 0.005 min
Response: 445866
Conc: 4.20 ug/ml

Instrument :

FID_F

ClientSampleId :