

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050222\
Data File : FF010468.D
Signal(s) : FID2B.ch
Acq On : 02 May 2022 11:54
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 03 01:30:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
Quant Title :
QLast Update : Fri Apr 29 04:08:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.614	2374030	19.358 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.506	35206	0.294 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050222\
Data File : FF010468.D
Signal(s) : FID2B.ch
Acq On : 02 May 2022 11:54
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 03 01:30:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
Quant Title :
QLast Update : Fri Apr 29 04:08:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

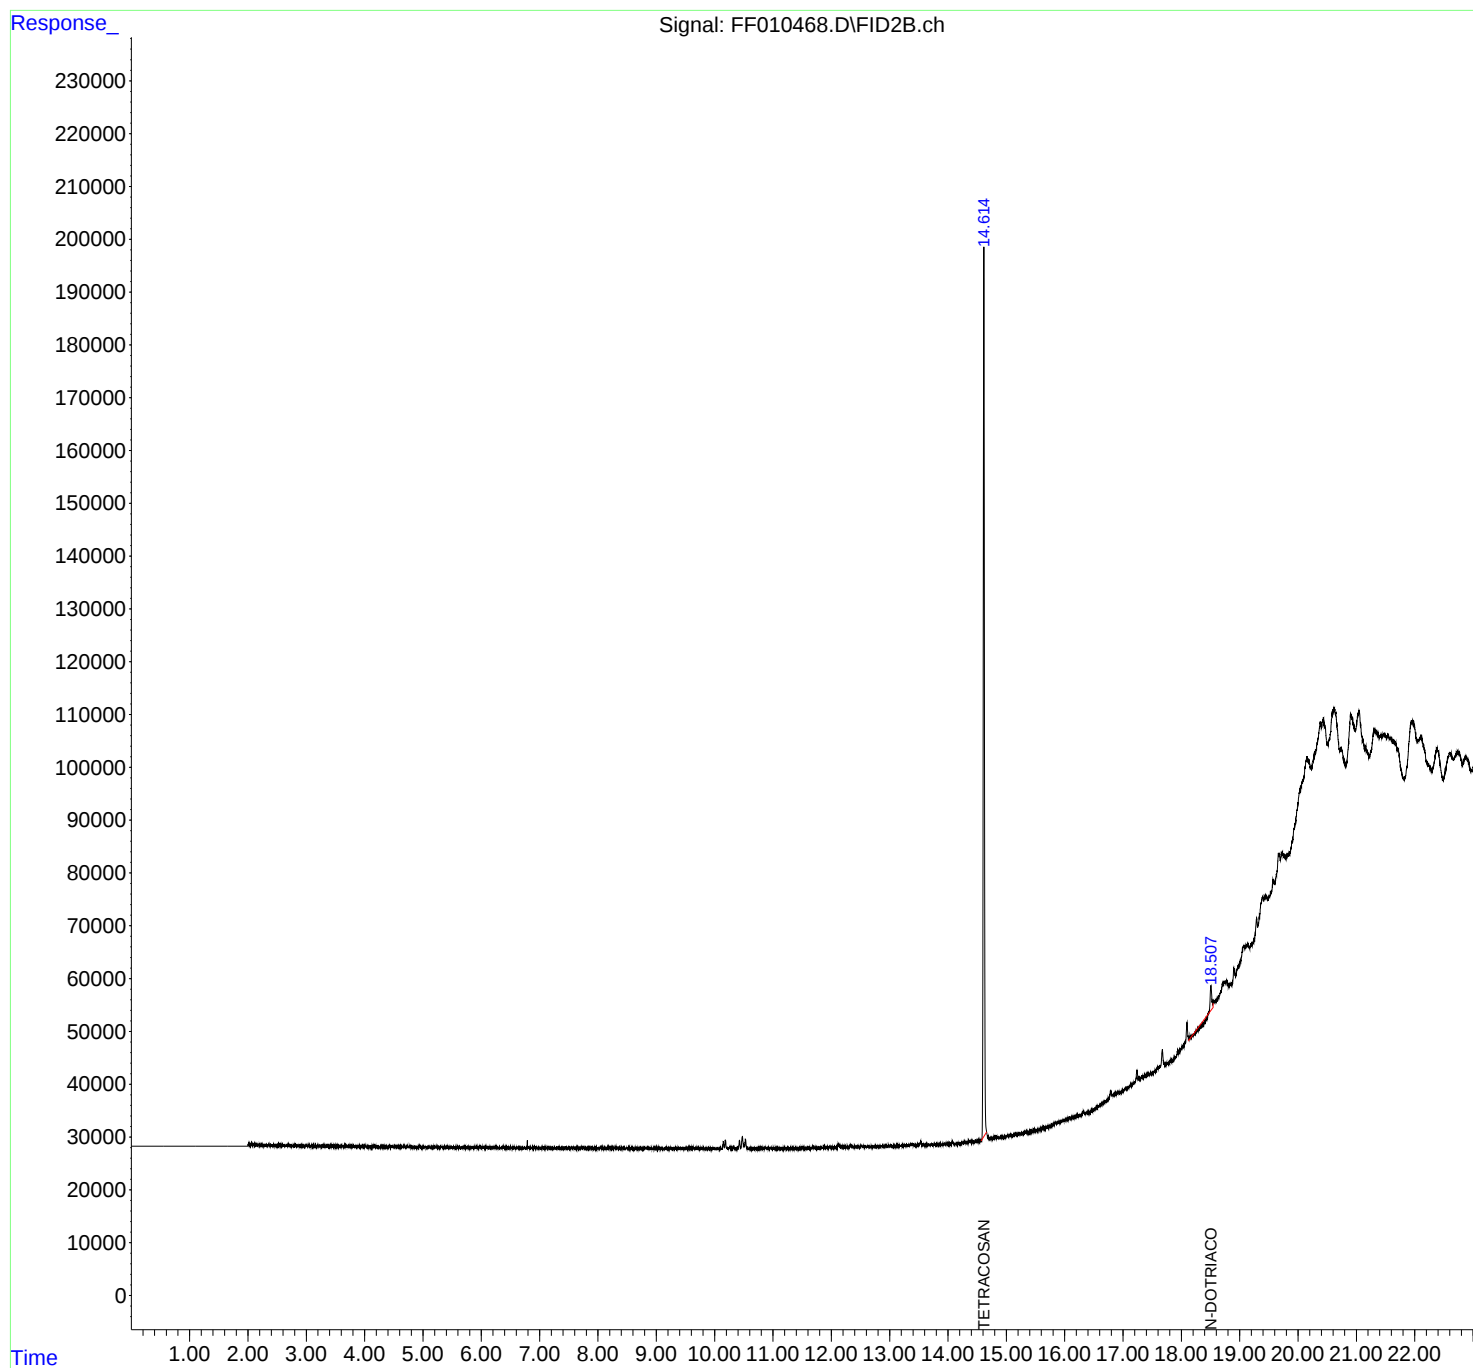


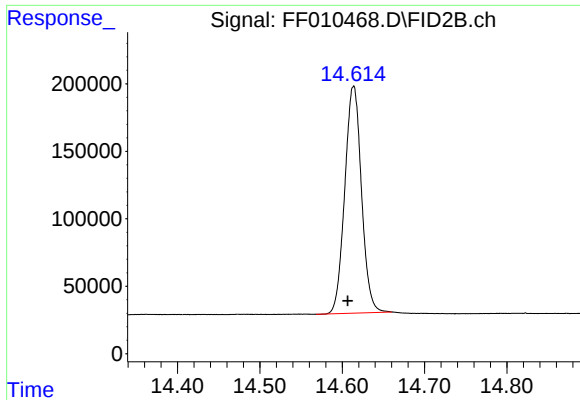

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.614 min
Delta R.T.: 0.007 min
Response: 2374030
Conc: 19.36 ug/ml

Instrument :
FID_F
ClientSampleId :

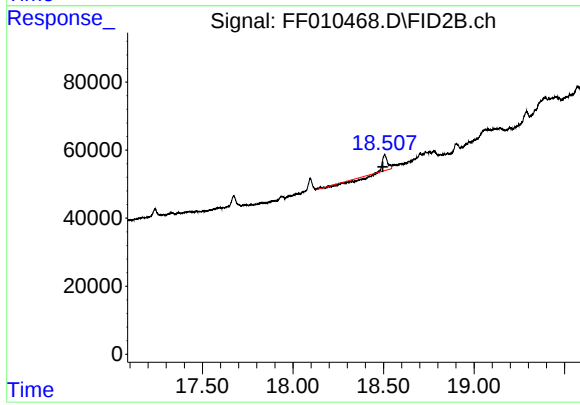

#14 N-DOTRIACONTANE

R.T.: 18.506 min
Delta R.T.: 0.010 min
Response: 35206
Conc: 0.29 ug/ml