

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050223\
 Data File : FF012555.D
 Signal(s) : FID2B.ch
 Acq On : 02 May 2023 10:02
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 03 01:21:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
 Quant Title :
 QLast Update : Thu Apr 13 15:26:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
8) N-DOCOSANE	14.097	124690	0.926 ug/ml
10) N-TETRACOSANE	15.185	362956	2.683 ug/ml
11) N-HEXACOSANE	16.226	65882	0.495 ug/ml
12) N-OCTACOSANE	17.174	60463	0.458 ug/ml
13) N-TRIACONTANE	18.062	56310	0.432 ug/ml
14) N-DOTRIACONTANE	18.898	150326	1.192 ug/ml
15) N-TETRATRIACONTANE	19.677	64907	0.572 ug/ml
16) N-HEXATRIACONTANE	20.455	148973	1.459 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050223\
Data File : FF012555.D
Signal(s) : FID2B.ch
Acq On : 02 May 2023 10:02
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 03 01:21:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

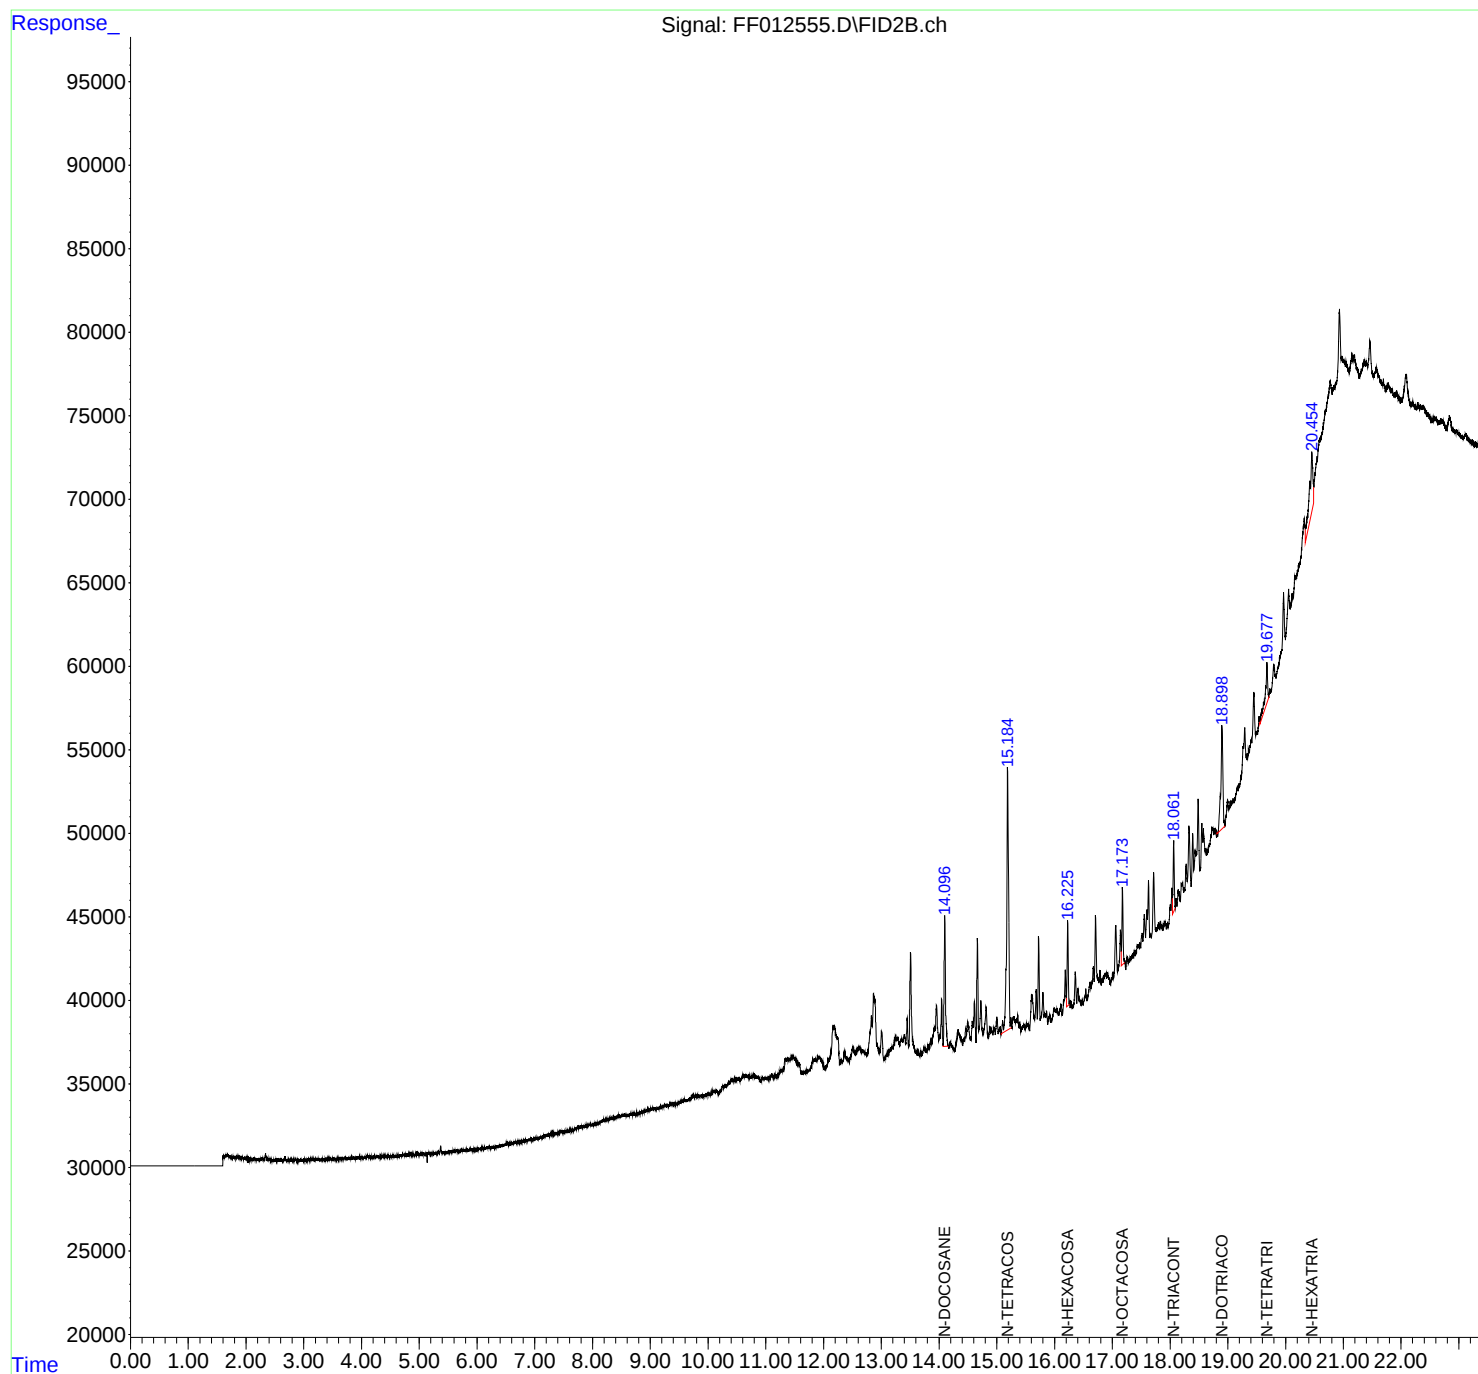


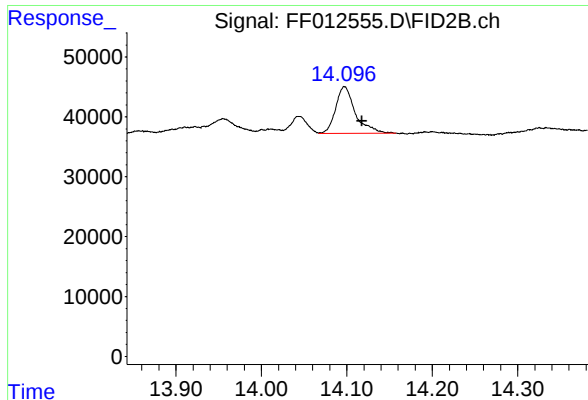

#8 N-DOCOSANE


R.T.: 14.097 min
Delta R.T.: -0.020 min
Response: 124690
Conc: 0.93 ug/ml

Instrument :
FID_F
ClientSampleId :

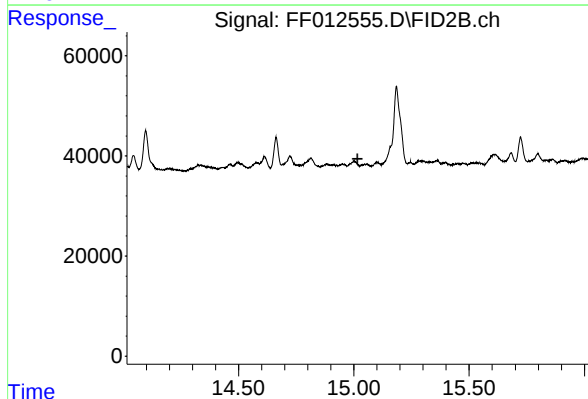


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.016 min
Response: 0
Conc: N.D.

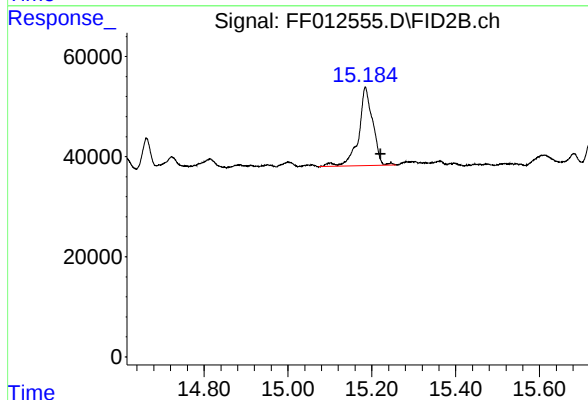


#10 N-TETRACOSANE

R.T.: 15.185 min
Delta R.T.: -0.036 min
Response: 362956
Conc: 2.68 ug/ml

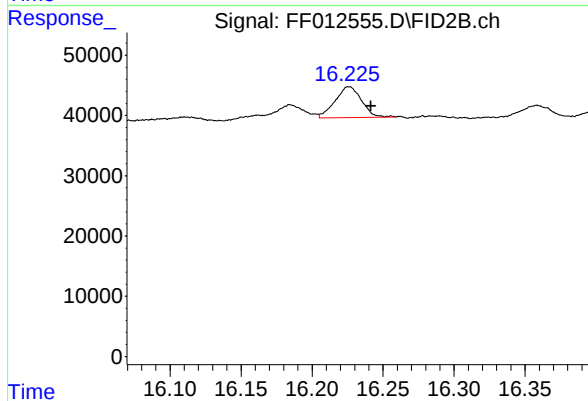

#11 N-HEXACOSANE


R.T.: 16.226 min
Delta R.T.: -0.015 min
Response: 65882
Conc: 0.49 ug/ml

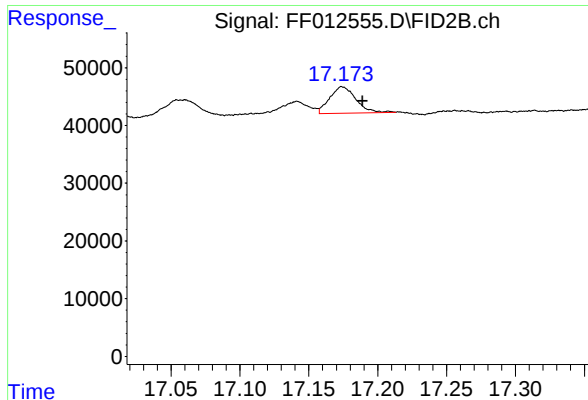

#12 N-OCTACOSANE


R.T.: 17.174 min
Delta R.T.: -0.015 min
Response: 60463
Conc: 0.46 ug/ml

Instrument :
FID_F
ClientSampleId :

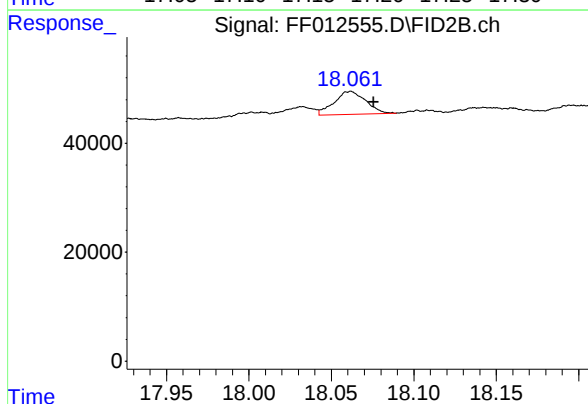


#13 N-TRIACONTANE

R.T.: 18.062 min
Delta R.T.: -0.014 min
Response: 56310
Conc: 0.43 ug/ml

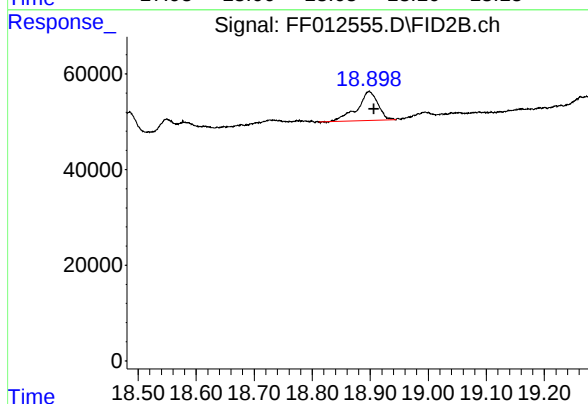


#14 N-DOTRIACONTANE

R.T.: 18.898 min
Delta R.T.: -0.009 min
Response: 150326
Conc: 1.19 ug/ml

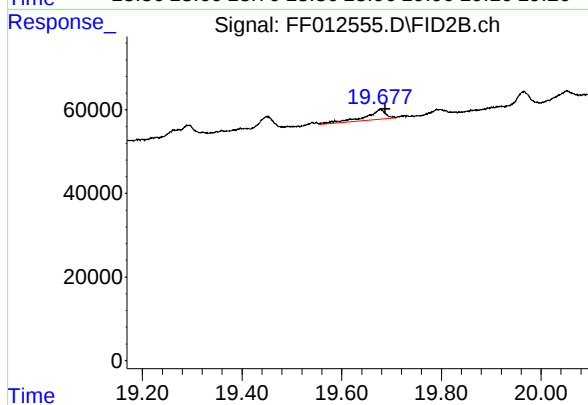

#15 N-TETRATRIACONTANE

R.T.: 19.677 min
Delta R.T.: -0.010 min
Response: 64907
Conc: 0.57 ug/ml

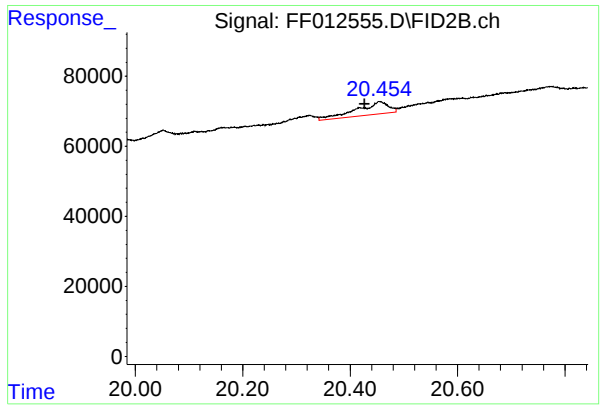

#16 N-HEXATRIACONTANE

R.T.: 20.455 min
Delta R.T.: 0.028 min
Response: 148973
Conc: 1.46 ug/ml

Instrument :

FID_F

ClientSampleId :