

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050223\
 Data File : FF012564.D
 Signal(s) : FID2B.ch
 Acq On : 02 May 2023 15:12
 Operator : YP\AJ
 Sample : 02529-03 10X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 03 01:22:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
 Quant Title :
 QLast Update : Thu Apr 13 15:26:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.015	1365551	11.360 ug/ml
Target Compounds			
3) N-DODECANE	6.677f	22364	0.181 ug/ml
4) N-TETRADECANE	8.573	504608	3.934 ug/ml
5) N-HEXADECANE	10.177	5129495	38.417 ug/ml
6) N-OCTADECANE	11.596	10431470	76.469 ug/ml
7) N-EICOSANE	12.922	9248149	67.159 ug/ml
8) N-DOCOSANE	14.108	3332764	24.758 ug/ml
10) N-TETRACOSANE	15.211	302093	2.233 ug/ml
16) N-HEXATRIACONTANE	20.400	90796	0.889 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050223\
Data File : FF012564.D
Signal(s) : FID2B.ch
Acq On : 02 May 2023 15:12
Operator : YP\AJ
Sample : 02529-03 10X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 03 01:22:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

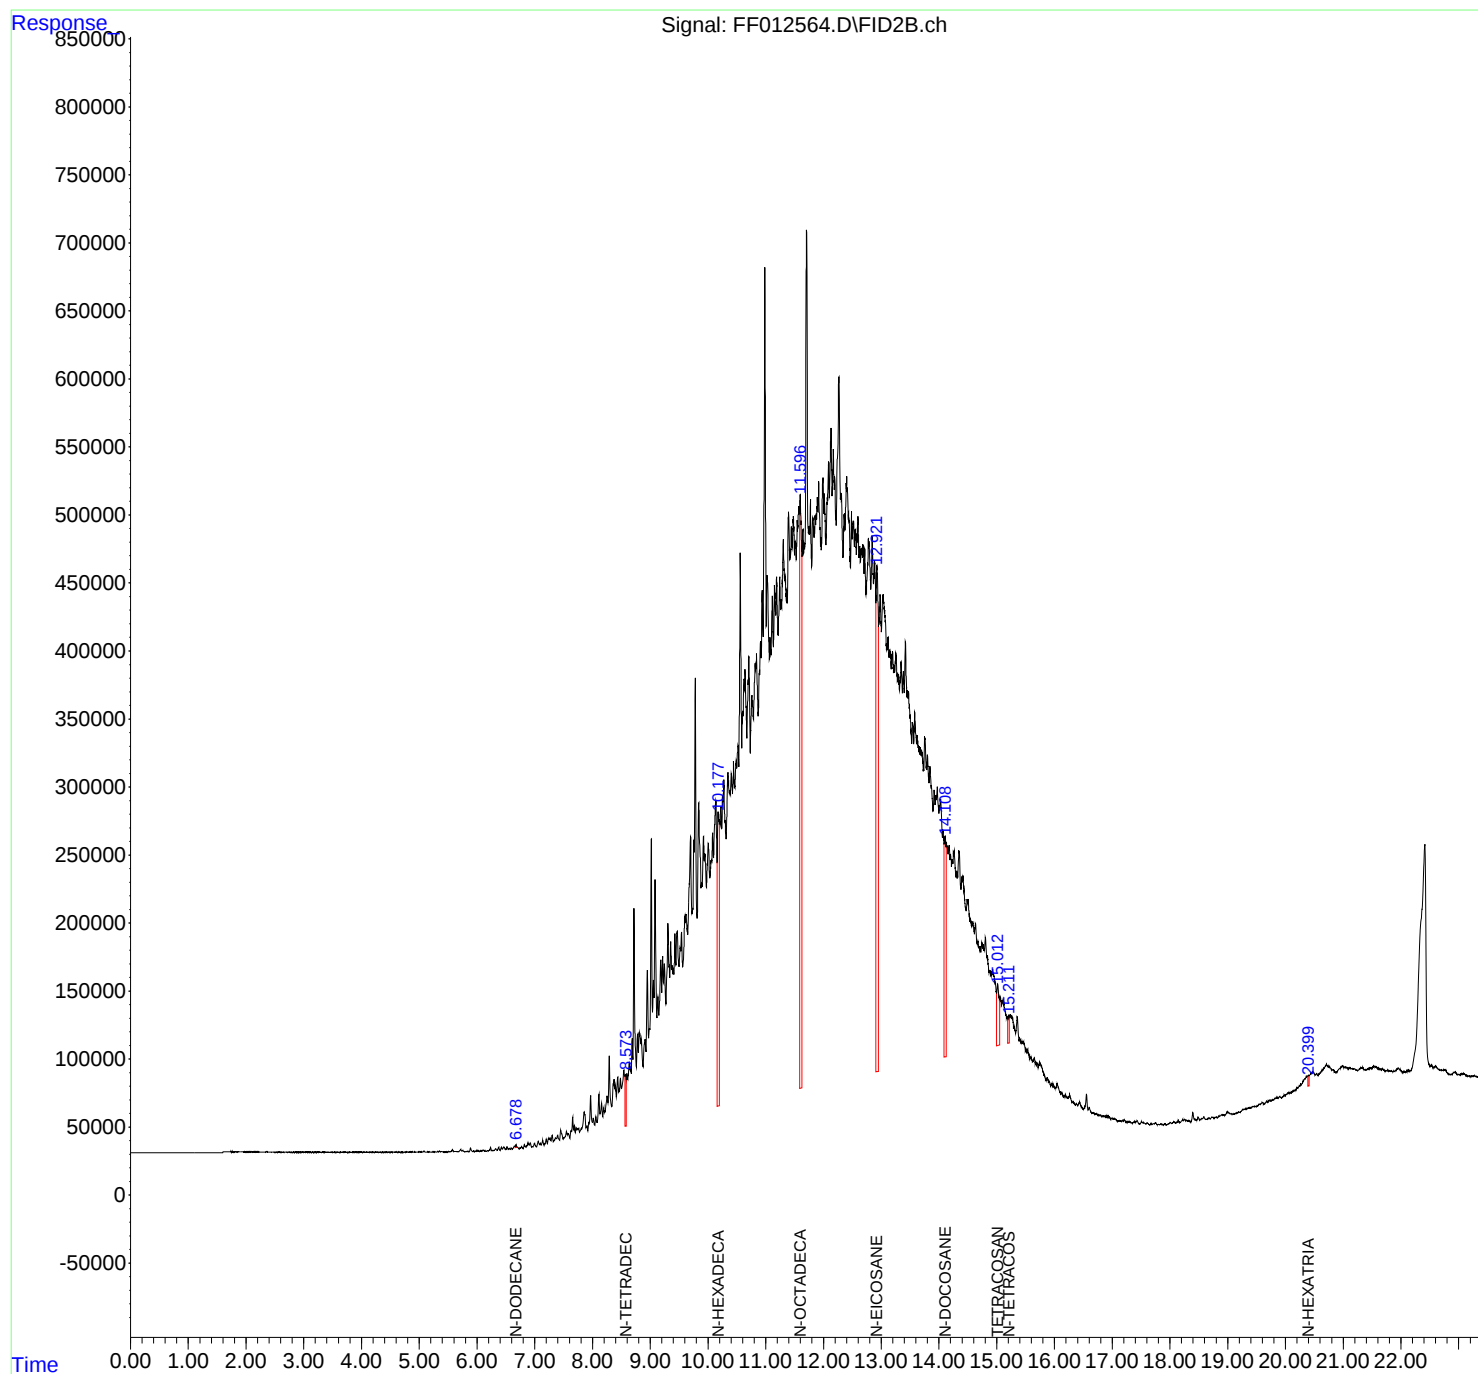


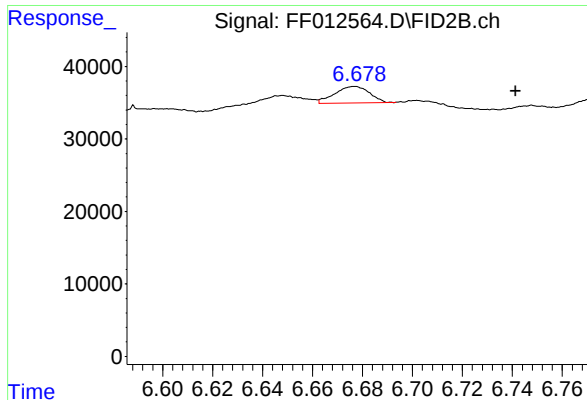

#3 N-DODECANE


R.T.: 6.677 min
Delta R.T.: -0.064 min
Response: 22364
Conc: 0.18 ug/ml

Instrument :
FID_F
ClientSampleId :

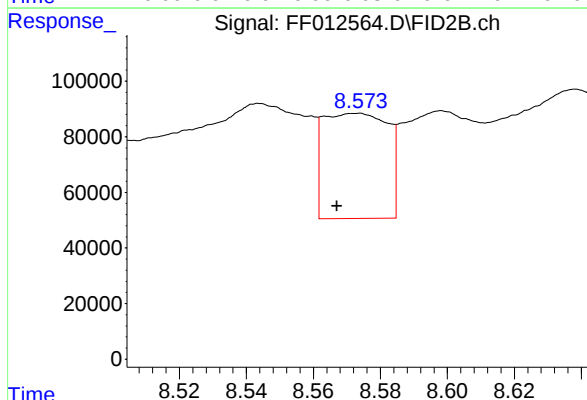


#4 N-TETRADECANE

R.T.: 8.573 min
Delta R.T.: 0.006 min
Response: 504608
Conc: 3.93 ug/ml

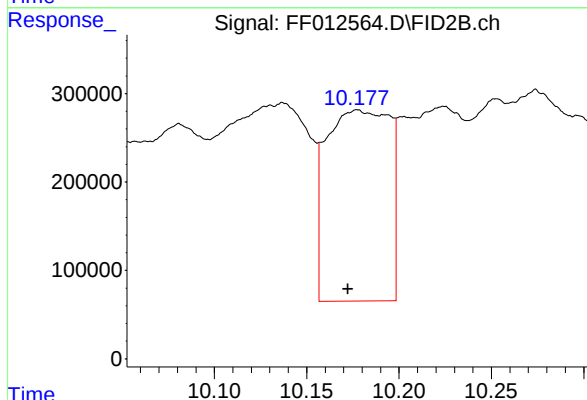


#5 N-HEXADECANE

R.T.: 10.177 min
Delta R.T.: 0.005 min
Response: 5129495
Conc: 38.42 ug/ml

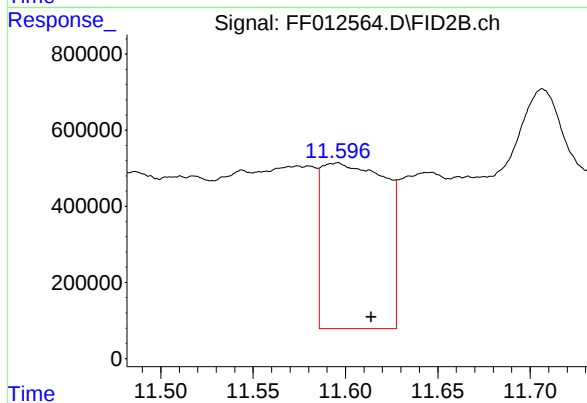

#6 N-OCTADECANE


R.T.: 11.596 min
Delta R.T.: -0.018 min
Response: 10431470
Conc: 76.47 ug/ml

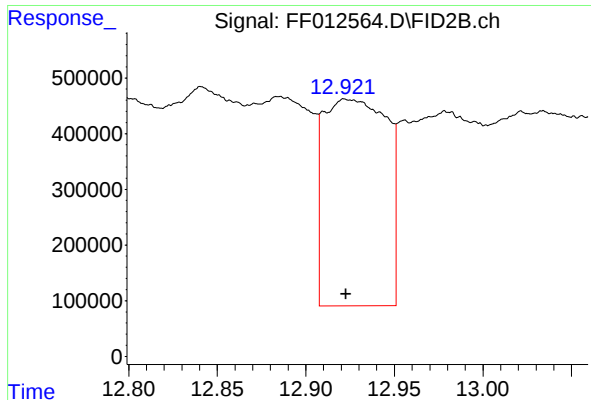

#7 N-EICOSANE


R.T.: 12.922 min
Delta R.T.: 0.000 min
Response: 9248149
Conc: 67.16 ug/ml

Instrument :
FID_F
ClientSampleId :

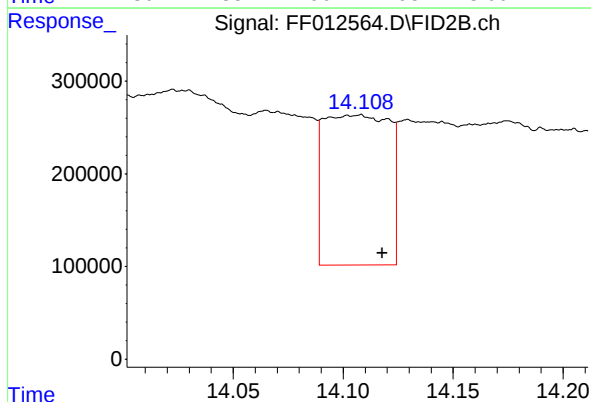


#8 N-DOCOSANE

R.T.: 14.108 min
Delta R.T.: -0.010 min
Response: 3332764
Conc: 24.76 ug/ml

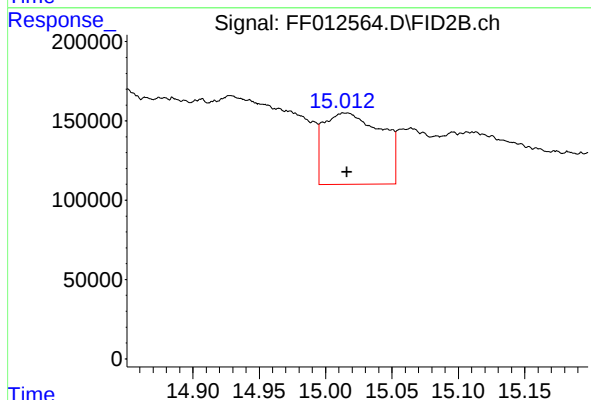


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.015 min
Delta R.T.: 0.000 min
Response: 1365551
Conc: 11.36 ug/ml

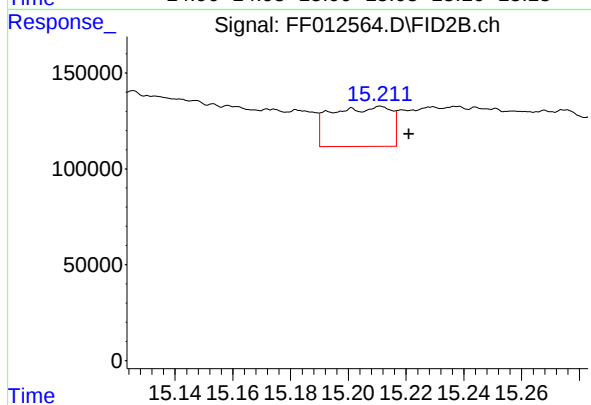

#10 N-TETRACOSANE

R.T.: 15.211 min
Delta R.T.: -0.010 min
Response: 302093
Conc: 2.23 ug/ml

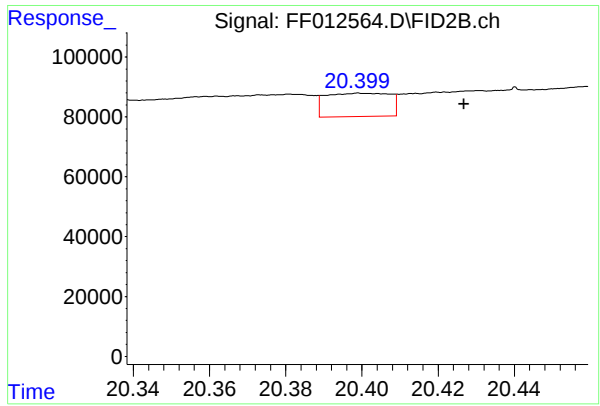

#16 N-HEXATRIACONTANE

R.T.: 20.400 min
Delta R.T.: -0.027 min
Response: 90796
Conc: 0.89 ug/ml

Instrument :

FID_F

ClientSampleId :