

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050319\
 Data File : FF004427.D
 Signal(s) : FID2B.ch
 Acq On : 03 May 2019 11:30
 Operator : AJ\SJ
 Sample : K2204-05 10X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 03 14:40:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050219.M
 Quant Title :
 QLast Update : Fri May 03 03:23:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.509	278042	2.222 ug/ml
Target Compounds			
7) N-EICOSANE	12.484f	534464	3.794 ug/ml
8) N-DOCOSANE	13.658	130184	0.918 ug/ml
10) N-TETRACOSANE	14.713	564652	3.961 ug/ml
12) N-OCTACOSANE	16.730	193519	1.380 ug/ml
13) N-TRIACONTANE	17.576	252411	1.770 ug/ml
14) N-DOTRIACONTANE	18.410	372408	2.654 ug/ml
15) N-TETRATRIACONTANE	19.177	275557	2.021 ug/ml
16) N-HEXATRIACONTANE	19.939	1868231	14.395 ug/ml
17) N-OCTATRIACONTANE	20.617	1722716	14.429 ug/ml
18) N-TETRACONTANE	21.505	105406	0.894 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050319\
Data File : FF004427.D
Signal(s) : FID2B.ch
Acq On : 03 May 2019 11:30
Operator : AJ\SJ
Sample : K2204-05 10X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 03 14:40:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050219.M
Quant Title :
QLast Update : Fri May 03 03:23:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

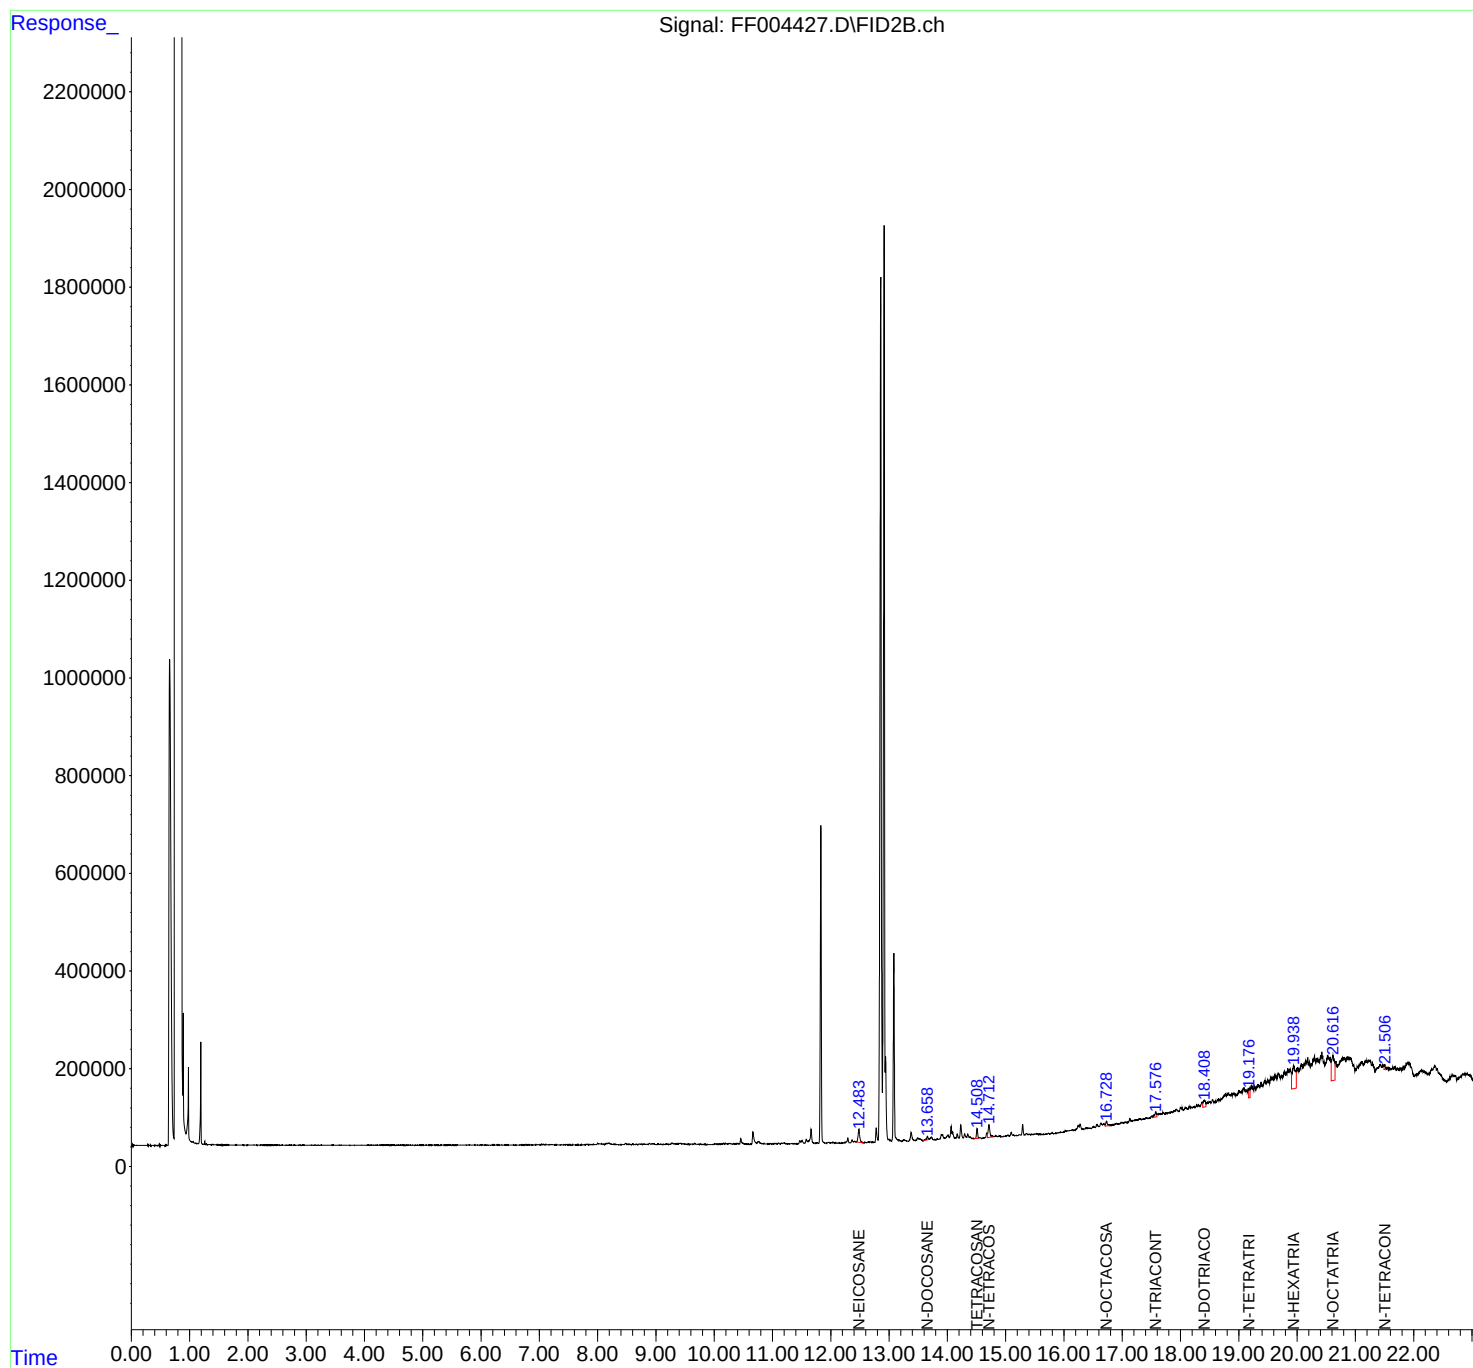

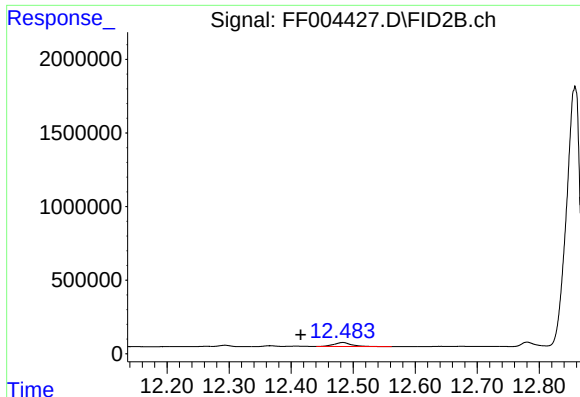


#7 N-EICOSANE

R.T.: 12.484 min
Delta R.T.: 0.068 min
Response: 534464
Conc: 3.79 ug/ml

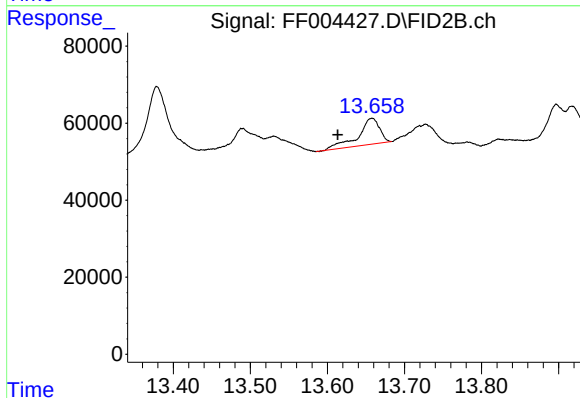


#8 N-DOCOSANE

R.T.: 13.658 min
Delta R.T.: 0.045 min
Response: 130184
Conc: 0.92 ug/ml

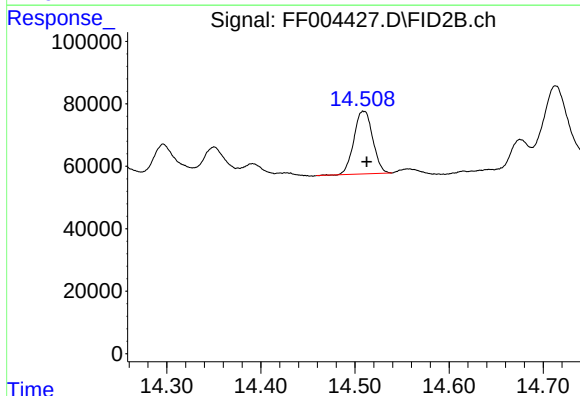


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.509 min
Delta R.T.: -0.003 min
Response: 278042
Conc: 2.22 ug/ml

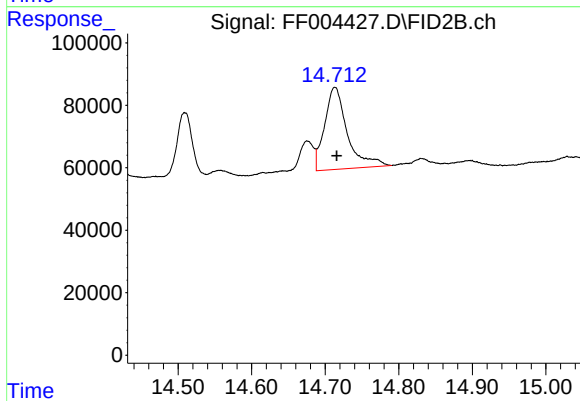


#10 N-TETRACOSANE

R.T.: 14.713 min
Delta R.T.: -0.002 min
Response: 564652
Conc: 3.96 ug/ml

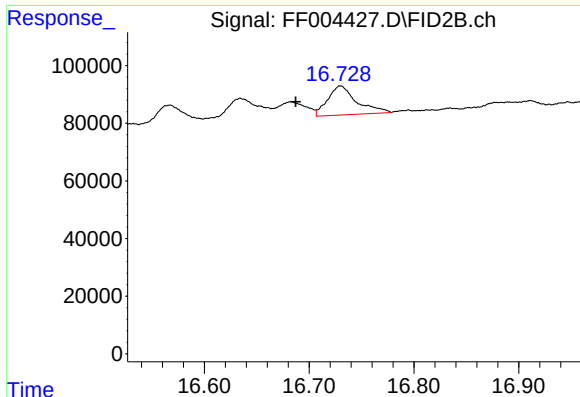


#12 N-OCTACOSANE

R.T.: 16.730 min
Delta R.T.: 0.043 min
Response: 193519
Conc: 1.38 ug/ml

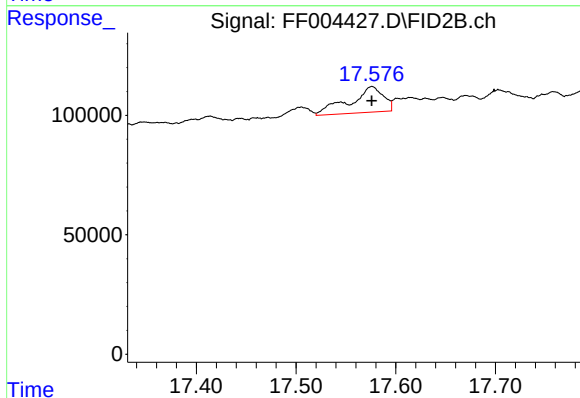


#13 N-TRIACONTANE

R.T.: 17.576 min
Delta R.T.: 0.000 min
Response: 252411
Conc: 1.77 ug/ml

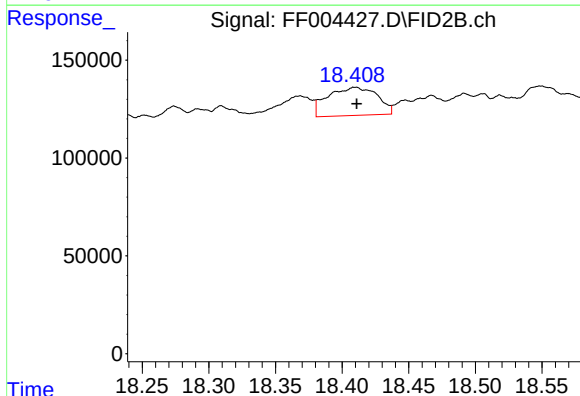


#14 N-DOTRIACONTANE

R.T.: 18.410 min
Delta R.T.: -0.001 min
Response: 372408
Conc: 2.65 ug/ml

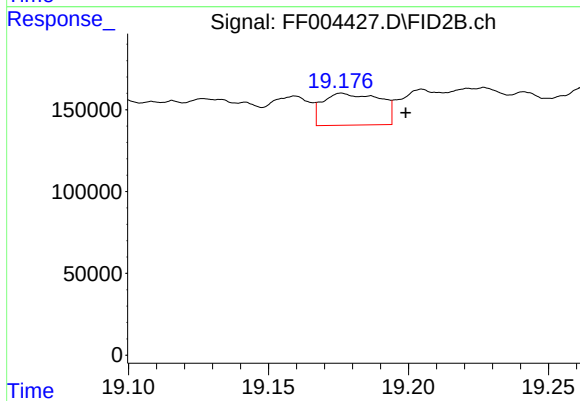


#15 N-TETRATRIACONTANE

R.T.: 19.177 min
Delta R.T.: -0.022 min
Response: 275557
Conc: 2.02 ug/ml

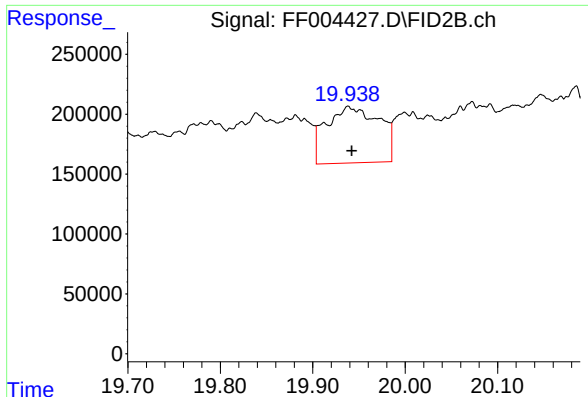


#16 N-HEXATRIACONTANE

R.T.: 19.939 min
Delta R.T.: -0.003 min
Response: 1868231
Conc: 14.40 ug/ml

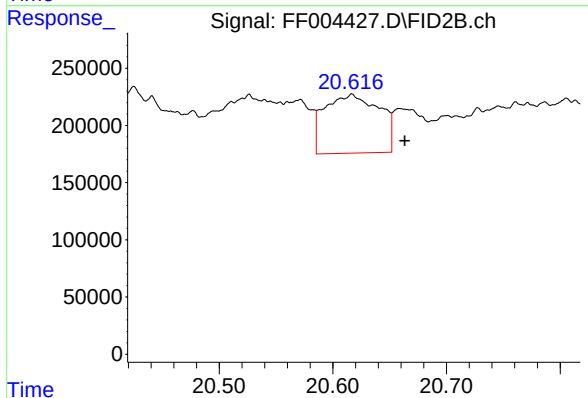

#17 N-OCTATRIACONTANE

R.T.: 20.617 min
Delta R.T.: -0.047 min
Response: 1722716
Conc: 14.43 ug/ml

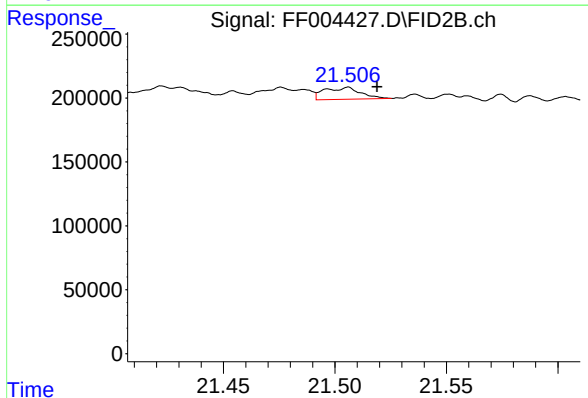

#18 N-TETRACONTANE

R.T.: 21.505 min
Delta R.T.: -0.014 min
Response: 105406
Conc: 0.89 ug/ml