

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050319\
Data File : FF004431.D
Signal(s) : FID2B.ch
Acq On : 03 May 2019 14:30
Operator : AJ\SJ
Sample : K2551-14 25X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 03 15:01:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050219.M
Quant Title :
QLast Update : Fri May 03 03:23:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
2) N-DECANE	4.264	691266	5.756 ug/ml
3) N-DODECANE	6.280	1261951	10.038 ug/ml
4) N-TETRADECANE	8.068	1979500	15.678 ug/ml
5) N-HEXADECANE	9.665	1673651	12.538 ug/ml
6) N-OCTADECANE	11.104	1314739	9.623 ug/ml
7) N-EICOSANE	12.413	708914	5.033 ug/ml
8) N-DOCOSANE	13.611	271569	1.914 ug/ml
14) N-DOTRIACONTANE	18.417	100900	0.719 ug/ml
16) N-HEXATRIACONTANE	19.984	396081	3.052 ug/ml
17) N-OCTATRIACONTANE	20.667	148499	1.244 ug/ml
18) N-TETRACONTANE	21.552	339862	2.882 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050319\
Data File : FF004431.D
Signal(s) : FID2B.ch
Acq On : 03 May 2019 14:30
Operator : AJ\SJ
Sample : K2551-14 25X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 03 15:01:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050219.M
Quant Title :
QLast Update : Fri May 03 03:23:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

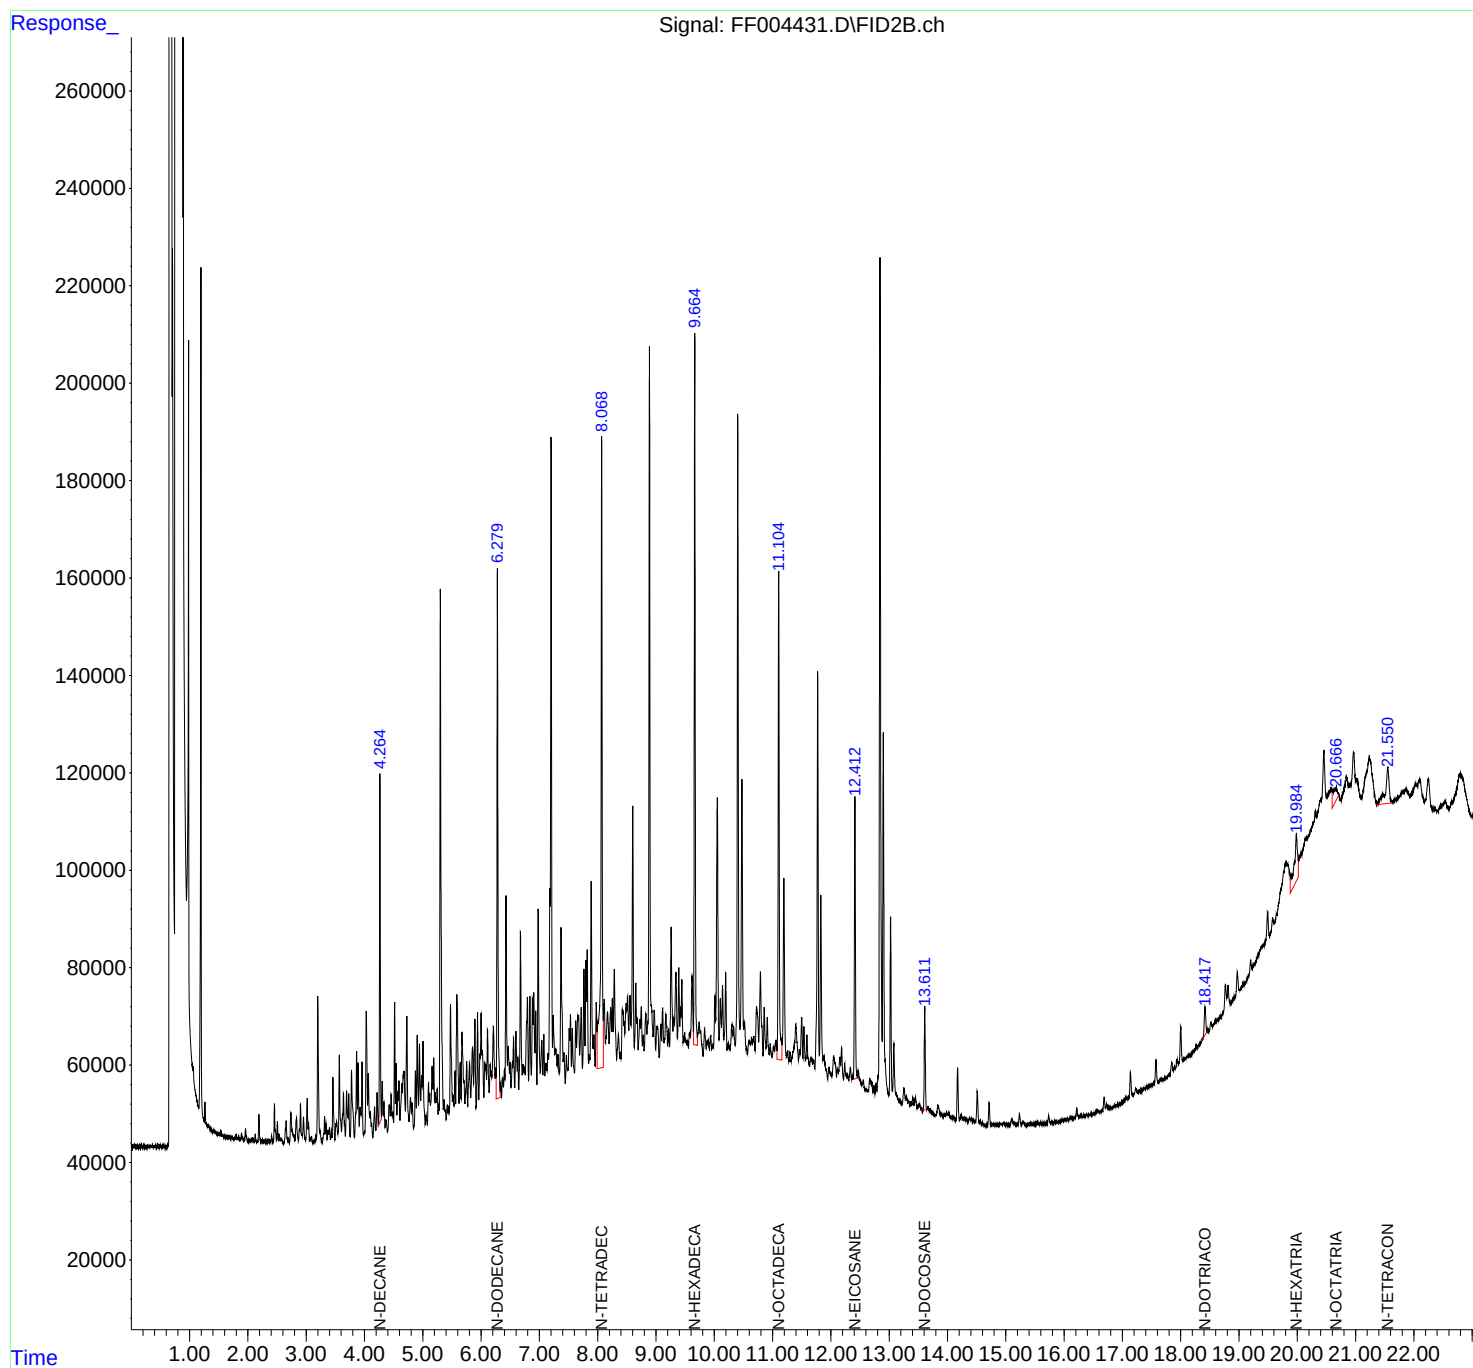

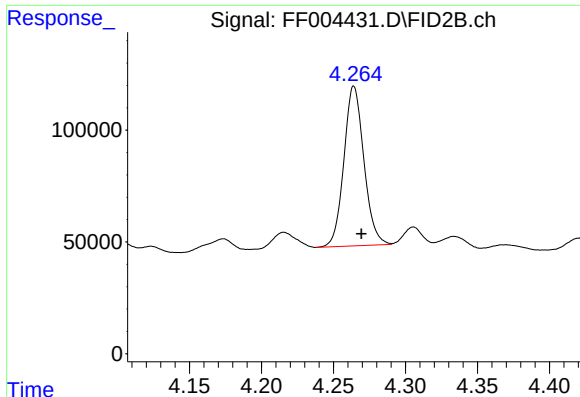


#2 N-DECANE

R.T.: 4.264 min
Delta R.T.: -0.005 min
Response: 691266
Conc: 5.76 ug/ml

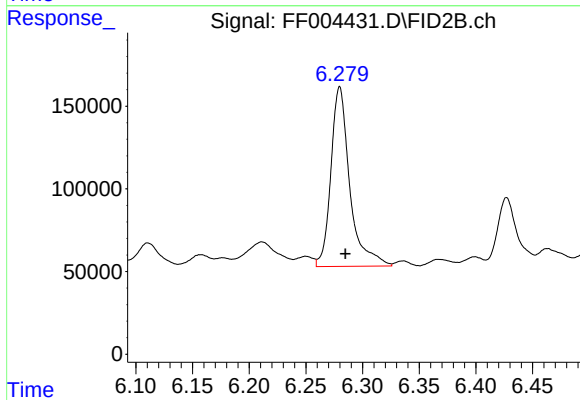


#3 N-DODECANE

R.T.: 6.280 min
Delta R.T.: -0.005 min
Response: 1261951
Conc: 10.04 ug/ml

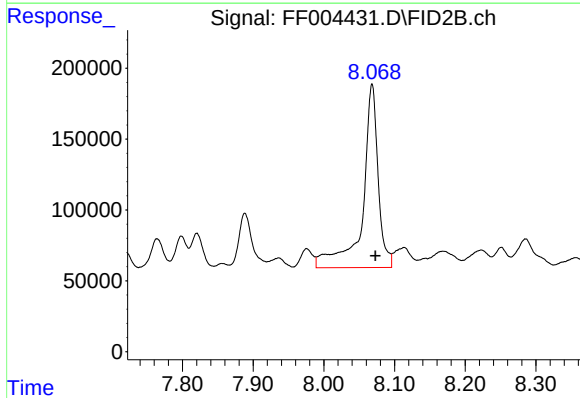


#4 N-TETRADECANE

R.T.: 8.068 min
Delta R.T.: -0.005 min
Response: 1979500
Conc: 15.68 ug/ml

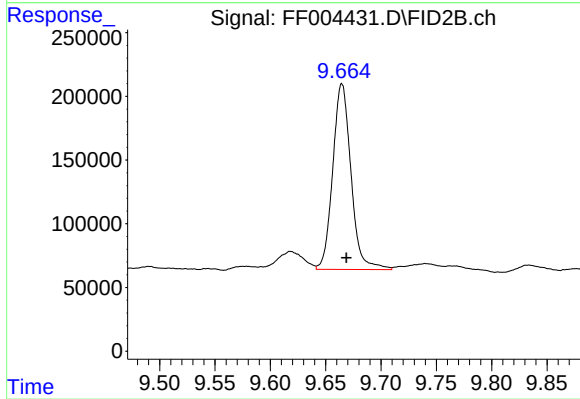


#5 N-HEXADECANE

R.T.: 9.665 min
Delta R.T.: -0.004 min
Response: 1673651
Conc: 12.54 ug/ml

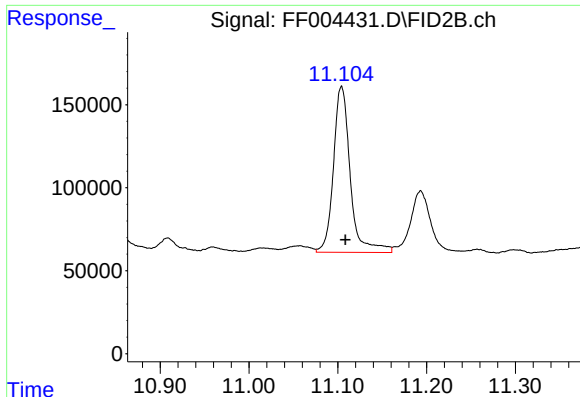


#6 N-OCTADECANE

R.T.: 11.104 min
Delta R.T.: -0.004 min
Response: 1314739
Conc: 9.62 ug/ml

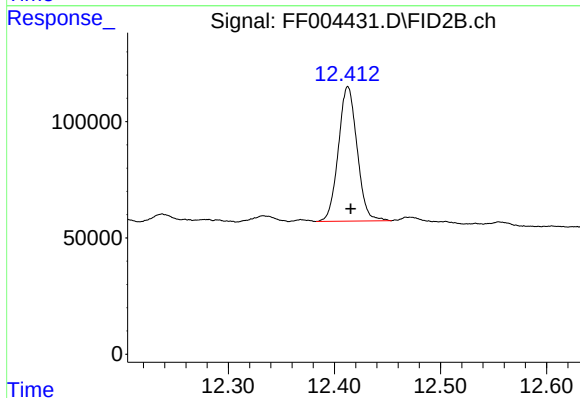


#7 N-EICOSANE

R.T.: 12.413 min
Delta R.T.: -0.003 min
Response: 708914
Conc: 5.03 ug/ml

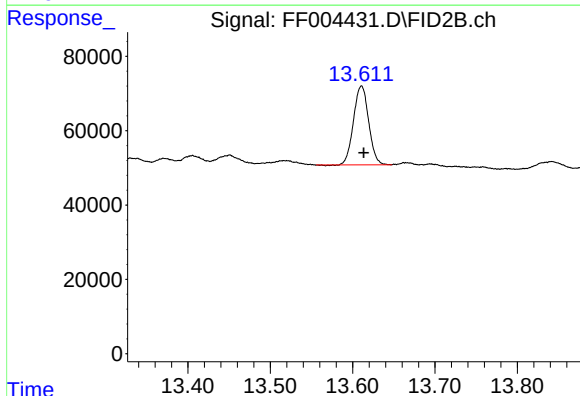


#8 N-DOCOSANE

R.T.: 13.611 min
Delta R.T.: -0.003 min
Response: 271569
Conc: 1.91 ug/ml

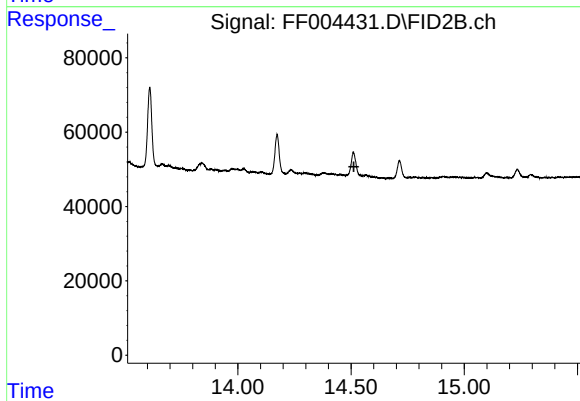


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.513 min
Response: 0
Conc: N.D.

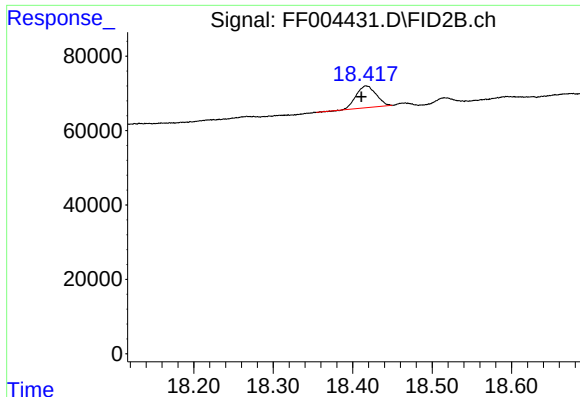


#14 N-DOTRIACONTANE

R.T.: 18.417 min
Delta R.T.: 0.006 min
Response: 100900
Conc: 0.72 ug/ml

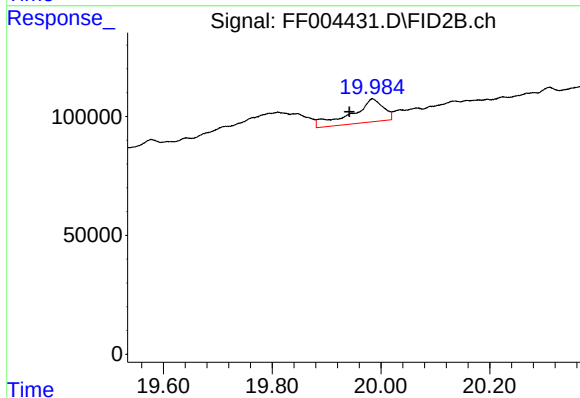


#16 N-HEXATRIACONTANE

R.T.: 19.984 min
Delta R.T.: 0.042 min
Response: 396081
Conc: 3.05 ug/ml

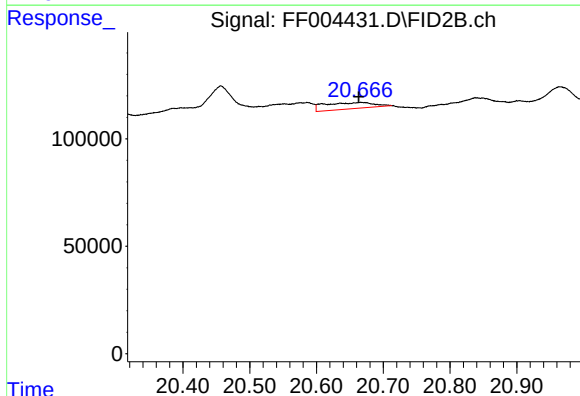

#17 N-OCTATRIACONTANE

R.T.: 20.667 min
Delta R.T.: 0.003 min
Response: 148499
Conc: 1.24 ug/ml

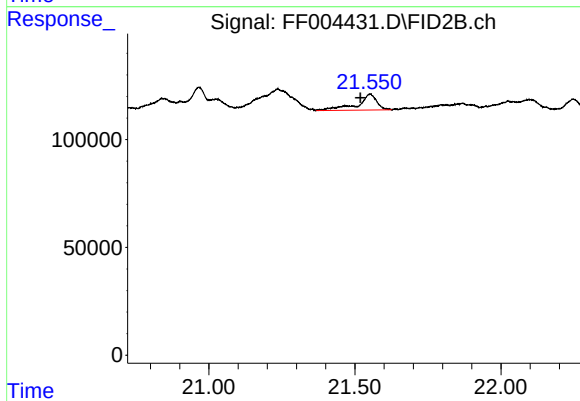

#18 N-TETRACONTANE

R.T.: 21.552 min
Delta R.T.: 0.033 min
Response: 339862
Conc: 2.88 ug/ml