

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050319\
 Data File : FF004440.D
 Signal(s) : FID2B.ch
 Acq On : 03 May 2019 18:59
 Operator : AJ\SJ
 Sample : K2668-06
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 03 22:45:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050219.M
 Quant Title :
 QLast Update : Fri May 03 03:23:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.510	2312348	18.481 ug/ml
Target Compounds			
4) N-TETRADECANE	8.070	94239	0.746 ug/ml
5) N-HEXADECANE	9.666	155995	1.169 ug/ml
6) N-OCTADECANE	11.104	126697	0.927 ug/ml
7) N-EICOSANE	12.412	102857	0.730 ug/ml
11) N-HEXACOSANE	15.733	216511	1.532 ug/ml
12) N-OCTACOSANE	16.683	652498	4.653 ug/ml
13) N-TRIACONTANE	17.572	797825	5.595 ug/ml
14) N-DOTRIACONTANE	18.407	678729	4.837 ug/ml
15) N-TETRATRIACONTANE	19.196	93196	0.684 ug/ml
16) N-HEXATRIACONTANE	19.979	326809	2.518 ug/ml
18) N-TETRACONTANE	21.547	522998	4.435 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050319\
Data File : FF004440.D
Signal(s) : FID2B.ch
Acq On : 03 May 2019 18:59
Operator : AJ\SJ
Sample : K2668-06
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 03 22:45:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050219.M
Quant Title :
QLast Update : Fri May 03 03:23:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

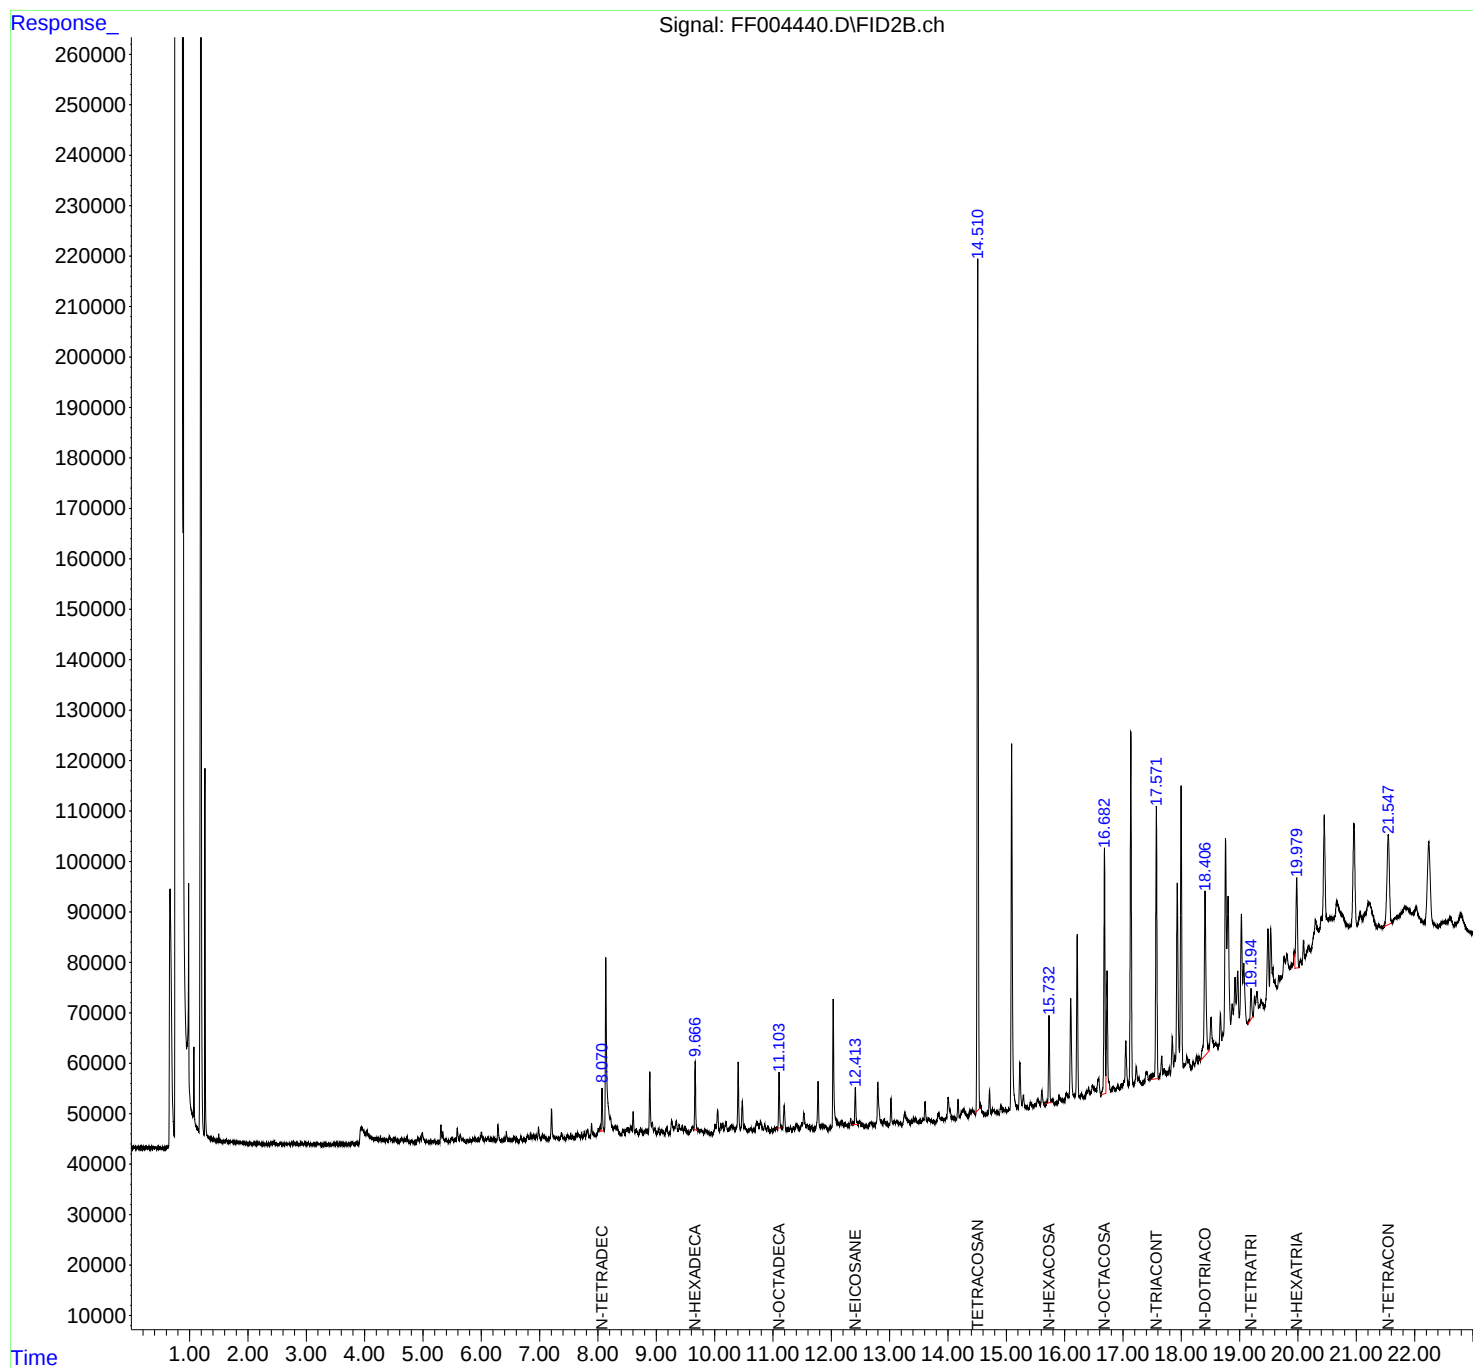

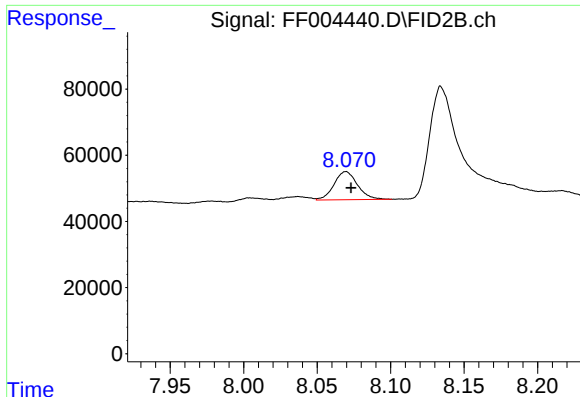


#4 N-TETRADECANE

R.T.: 8.070 min
Delta R.T.: -0.003 min
Response: 94239
Conc: 0.75 ug/ml

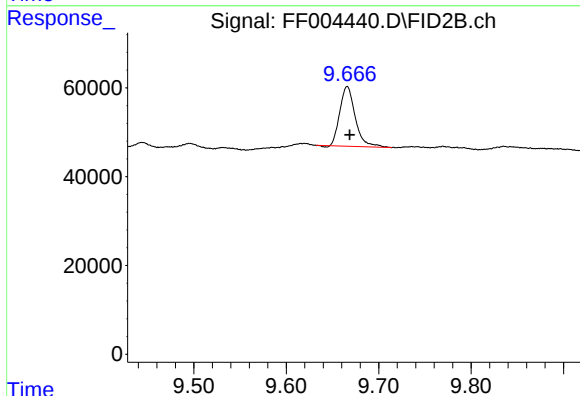


#5 N-HEXADECANE

R.T.: 9.666 min
Delta R.T.: -0.003 min
Response: 155995
Conc: 1.17 ug/ml

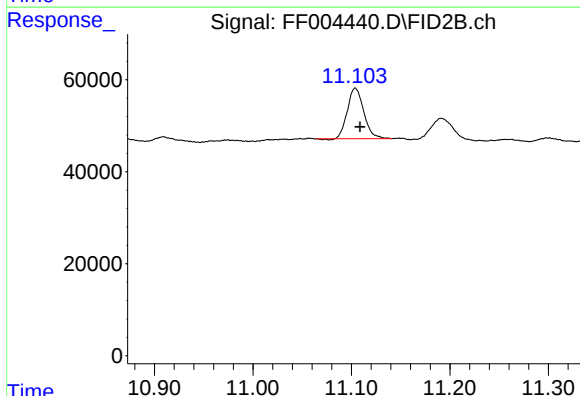


#6 N-OCTADECANE

R.T.: 11.104 min
Delta R.T.: -0.005 min
Response: 126697
Conc: 0.93 ug/ml

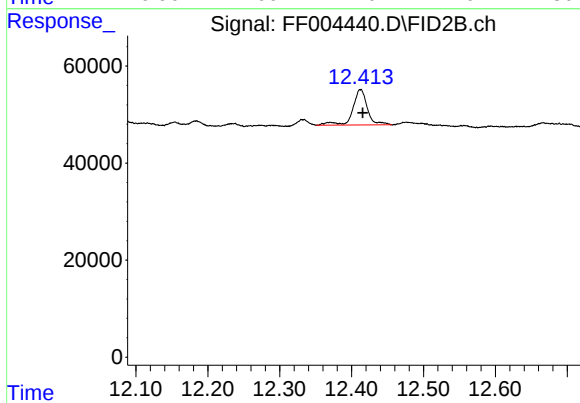


#7 N-EICOSANE

R.T.: 12.412 min
Delta R.T.: -0.003 min
Response: 102857
Conc: 0.73 ug/ml

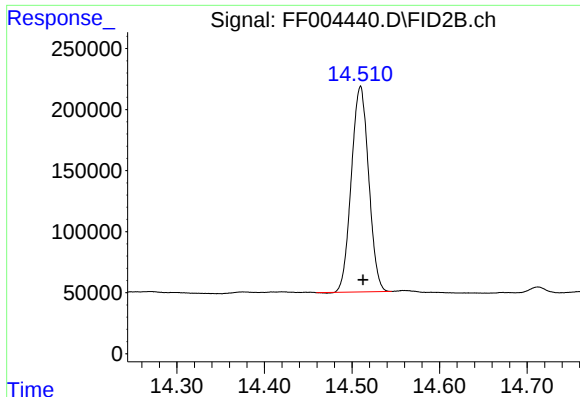


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.510 min
Delta R.T.: -0.003 min
Response: 2312348
Conc: 18.48 ug/ml

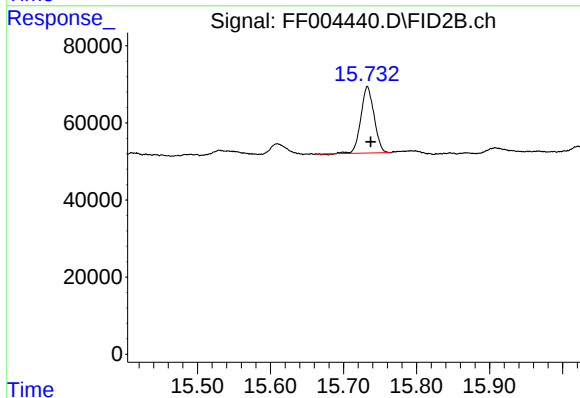


#11 N-HEXACOSANE

R.T.: 15.733 min
Delta R.T.: -0.004 min
Response: 216511
Conc: 1.53 ug/ml

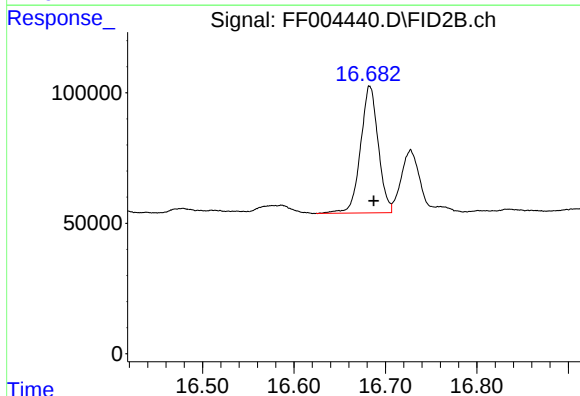


#12 N-OCTACOSANE

R.T.: 16.683 min
Delta R.T.: -0.004 min
Response: 652498
Conc: 4.65 ug/ml

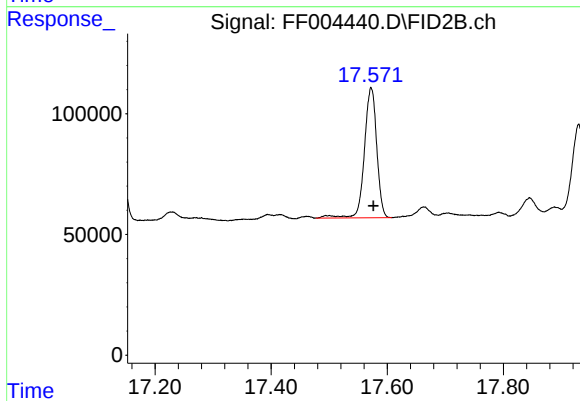


#13 N-TRIACONTANE

R.T.: 17.572 min
Delta R.T.: -0.003 min
Response: 797825
Conc: 5.60 ug/ml

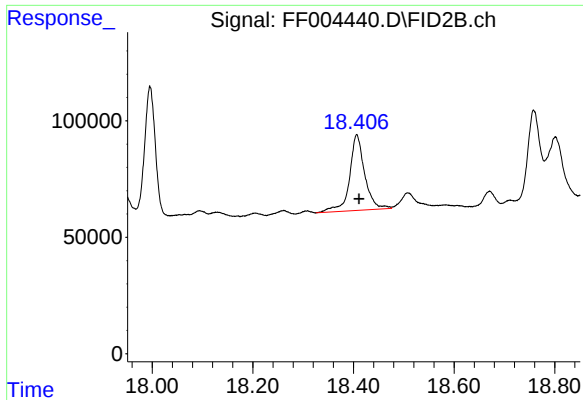


#14 N-DOTRIACONTANE

R.T.: 18.407 min
Delta R.T.: -0.004 min
Response: 678729
Conc: 4.84 ug/ml

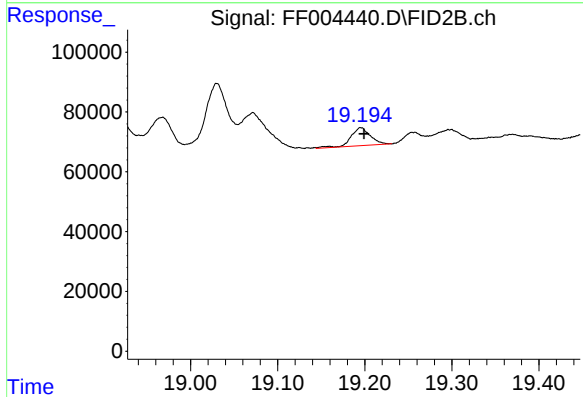


#15 N-TETRATRIACONTANE

R.T.: 19.196 min
Delta R.T.: -0.003 min
Response: 93196
Conc: 0.68 ug/ml

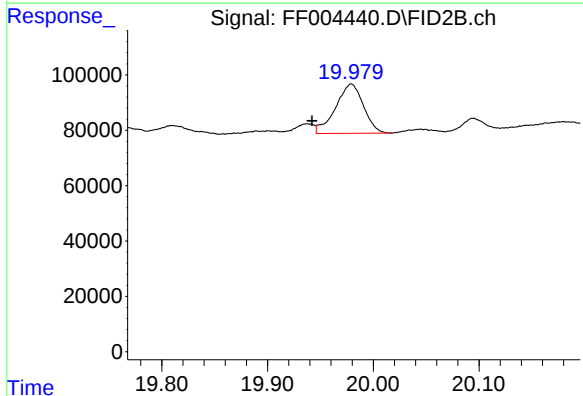

#16 N-HEXATRIACONTANE

R.T.: 19.979 min
Delta R.T.: 0.037 min
Response: 326809
Conc: 2.52 ug/ml

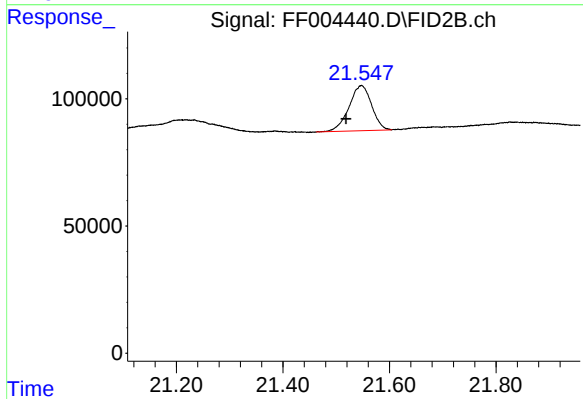

#18 N-TETRACONTANE

R.T.: 21.547 min
Delta R.T.: 0.028 min
Response: 522998
Conc: 4.43 ug/ml