

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050319\
 Data File : FF004442.D
 Signal(s) : FID2B.ch
 Acq On : 03 May 2019 19:57
 Operator : AJ\SJ
 Sample : K2635-03 10X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 03 22:46:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050219.M
 Quant Title :
 QLast Update : Fri May 03 03:23:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.509	162008	1.295 ug/ml
Target Compounds			
4) N-TETRADECANE	8.070	109056	0.864 ug/ml
5) N-HEXADECANE	9.666	237346	1.778 ug/ml
6) N-OCTADECANE	11.105	263611	1.930 ug/ml
7) N-EICOSANE	12.414	249698	1.773 ug/ml
8) N-DOCOSANE	13.611	123237	0.869 ug/ml
10) N-TETRACOSANE	14.714	222484	1.561 ug/ml
12) N-OCTACOSANE	16.687	122806	0.876 ug/ml
13) N-TRIACONTANE	17.573	122745	0.861 ug/ml
14) N-DOTRIACONTANE	18.413	237763	1.695 ug/ml
15) N-TETRATRIACONTANE	19.198	203655	1.494 ug/ml
16) N-HEXATRIACONTANE	19.942	108074	0.833 ug/ml
17) N-OCTATRIACONTANE	20.664	155381	1.301 ug/ml
18) N-TETRACONTANE	21.547	289973	2.459 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050319\
Data File : FF004442.D
Signal(s) : FID2B.ch
Acq On : 03 May 2019 19:57
Operator : AJ\SJ
Sample : K2635-03 10X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 03 22:46:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050219.M
Quant Title :
QLast Update : Fri May 03 03:23:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

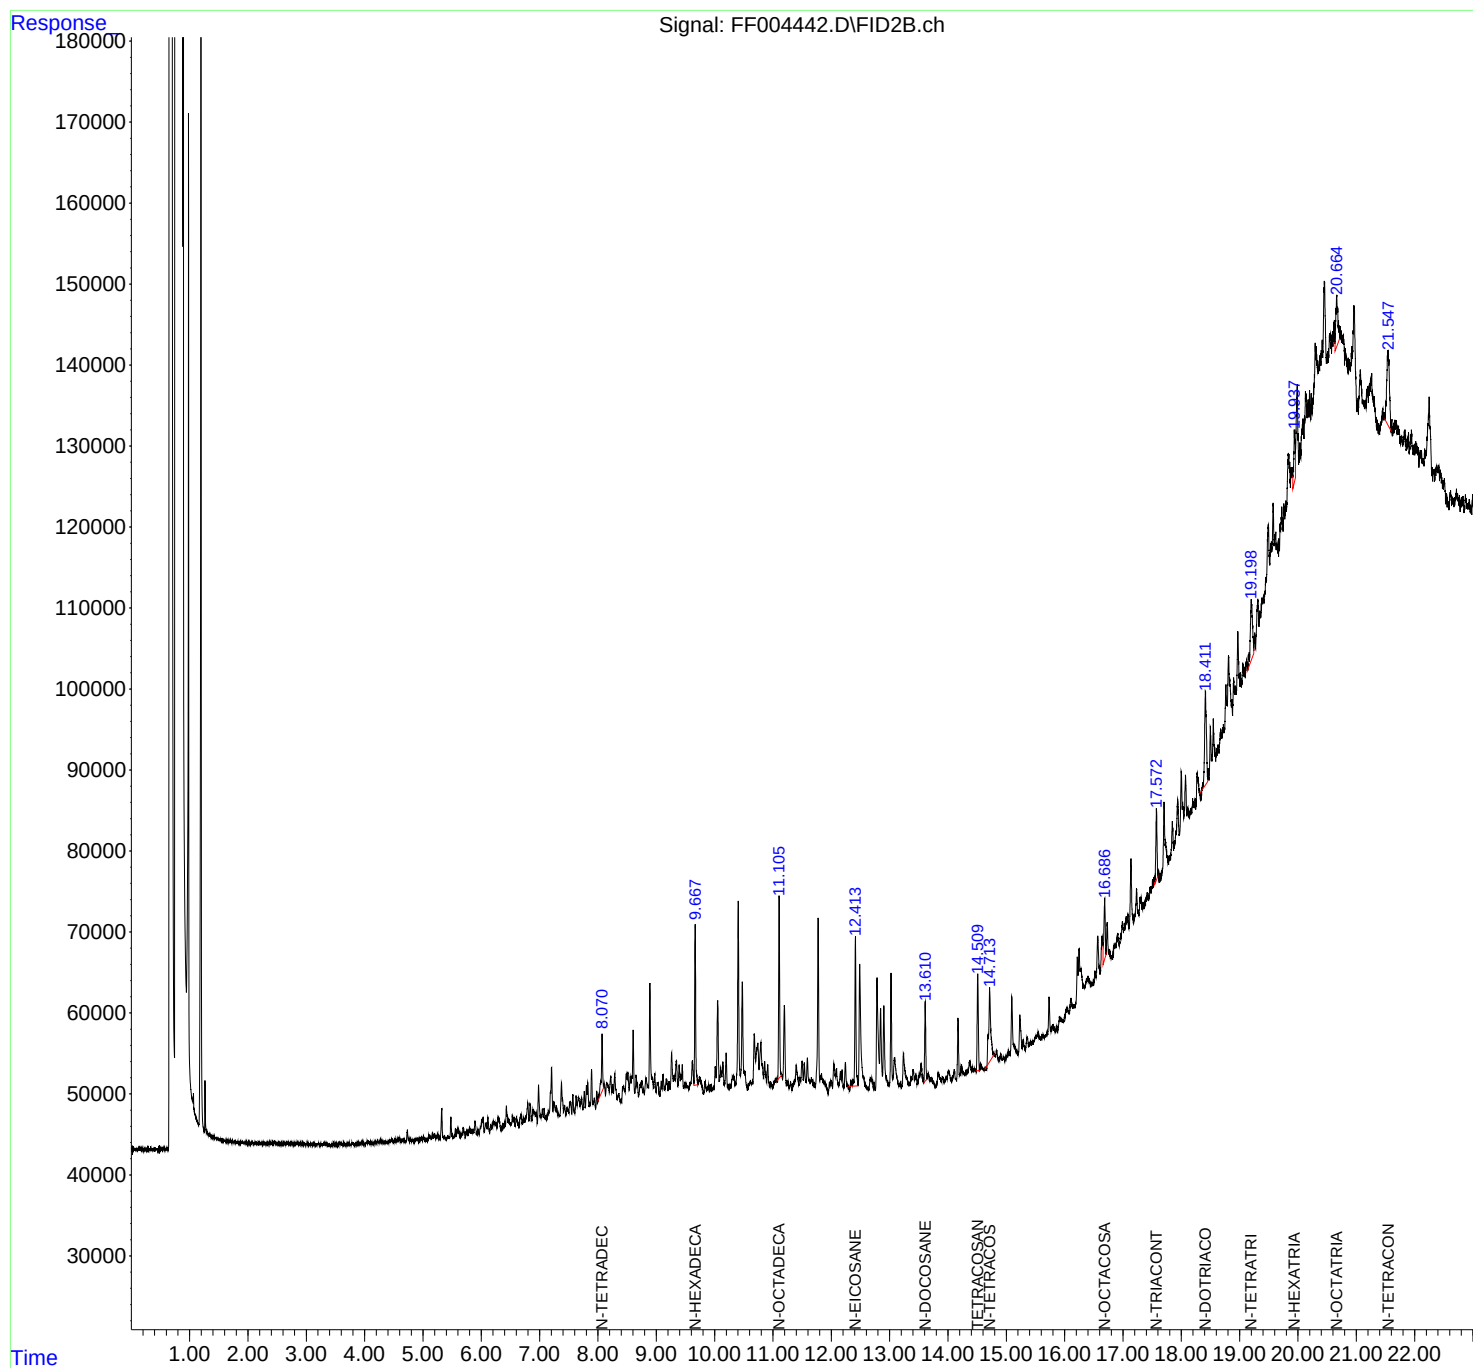

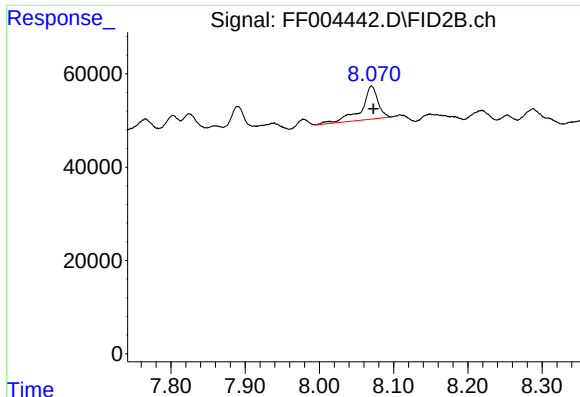


#4 N-TETRADECANE

R.T.: 8.070 min
Delta R.T.: -0.003 min
Response: 109056
Conc: 0.86 ug/ml

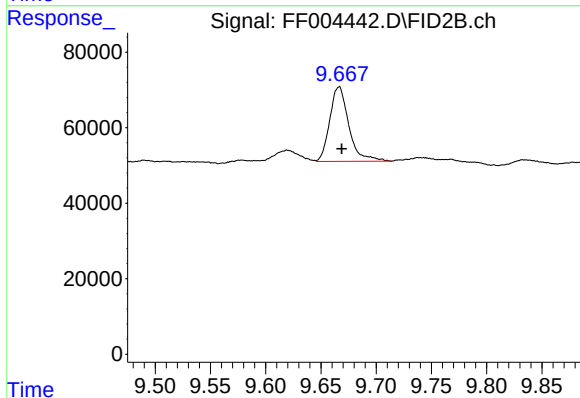


#5 N-HEXADECANE

R.T.: 9.666 min
Delta R.T.: -0.003 min
Response: 237346
Conc: 1.78 ug/ml

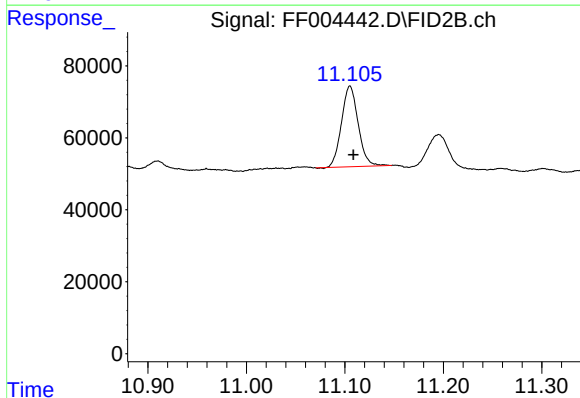


#6 N-OCTADECANE

R.T.: 11.105 min
Delta R.T.: -0.003 min
Response: 263611
Conc: 1.93 ug/ml

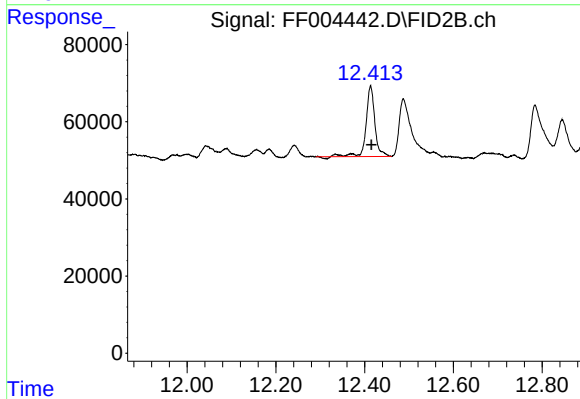


#7 N-EICOSANE

R.T.: 12.414 min
Delta R.T.: -0.002 min
Response: 249698
Conc: 1.77 ug/ml

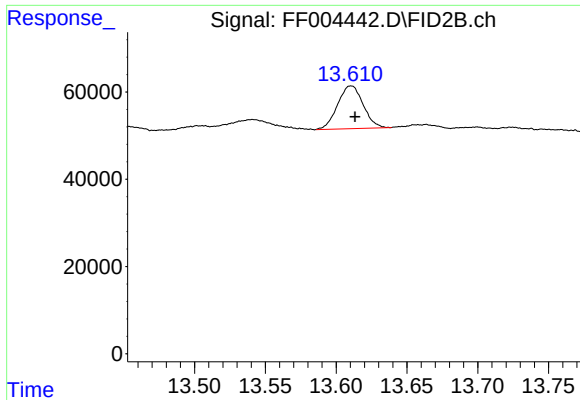


#8 N-DOCOSANE

R.T.: 13.611 min
Delta R.T.: -0.003 min
Response: 123237
Conc: 0.87 ug/ml

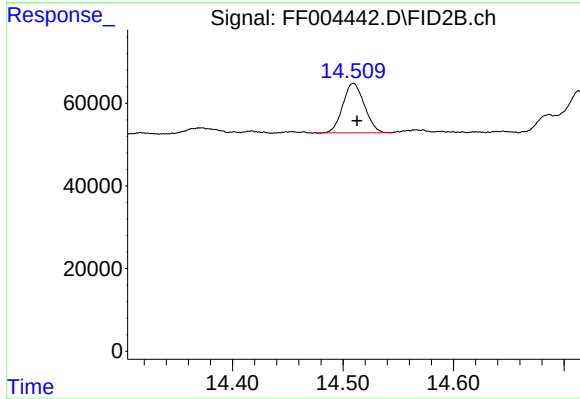


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.509 min
Delta R.T.: -0.003 min
Response: 162008
Conc: 1.29 ug/ml

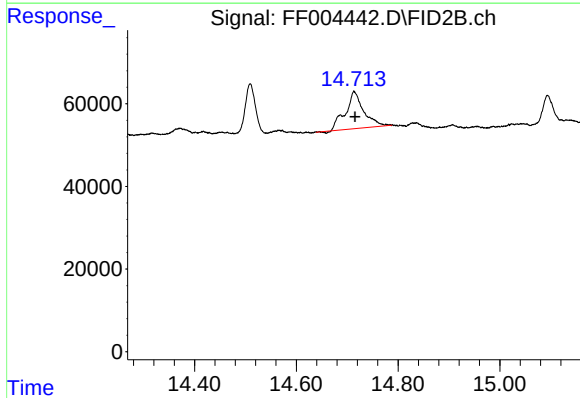


#10 N-TETRACOSANE

R.T.: 14.714 min
Delta R.T.: -0.002 min
Response: 222484
Conc: 1.56 ug/ml

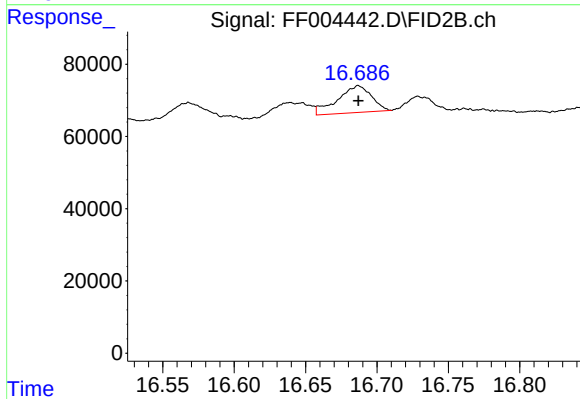


#12 N-OCTACOSANE

R.T.: 16.687 min
Delta R.T.: 0.000 min
Response: 122806
Conc: 0.88 ug/ml

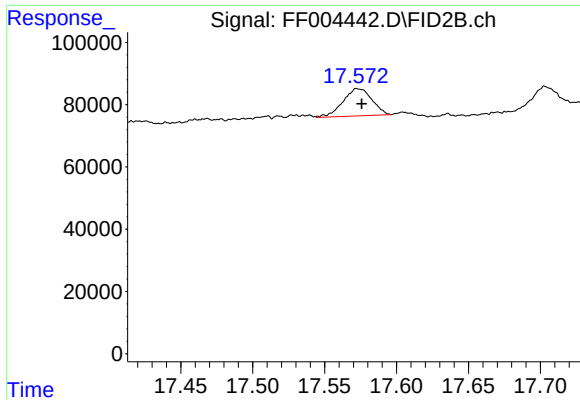


#13 N-TRIACONTANE

R.T.: 17.573 min
Delta R.T.: -0.003 min
Response: 122745
Conc: 0.86 ug/ml

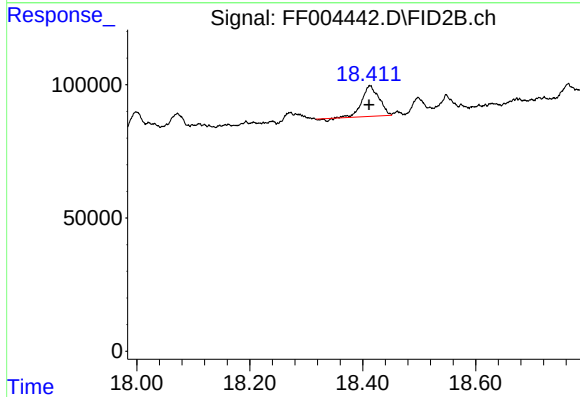


#14 N-DOTRIACONTANE

R.T.: 18.413 min
Delta R.T.: 0.002 min
Response: 237763
Conc: 1.69 ug/ml

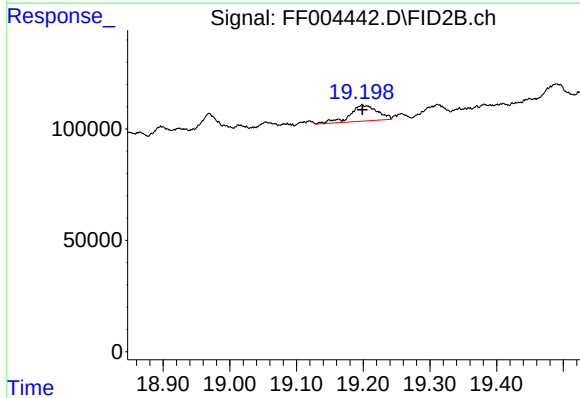


#15 N-TETRATRIACONTANE

R.T.: 19.198 min
Delta R.T.: 0.000 min
Response: 203655
Conc: 1.49 ug/ml

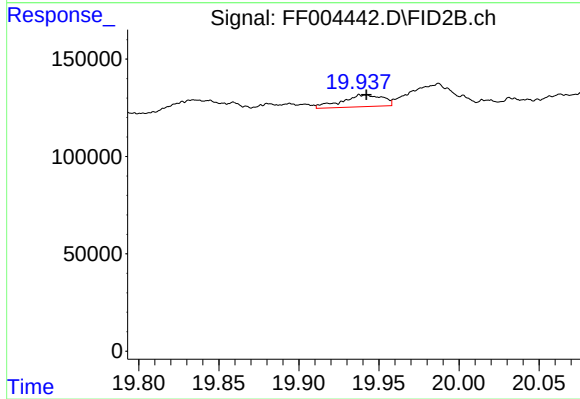


#16 N-HEXATRIACONTANE

R.T.: 19.942 min
Delta R.T.: 0.000 min
Response: 108074
Conc: 0.83 ug/ml

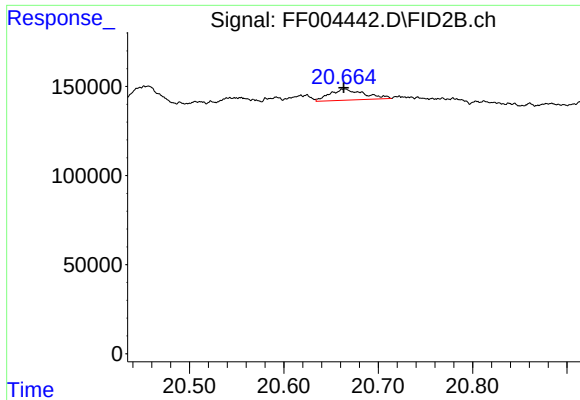

#17 N-OCTATRIACONTANE

R.T.: 20.664 min
Delta R.T.: 0.000 min
Response: 155381
Conc: 1.30 ug/ml

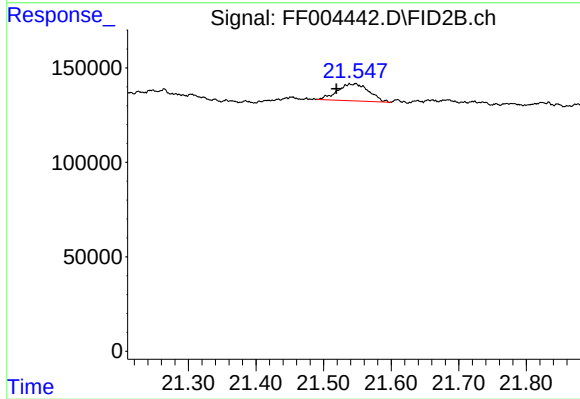

#18 N-TETRACONTANE

R.T.: 21.547 min
Delta R.T.: 0.029 min
Response: 289973
Conc: 2.46 ug/ml