

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050319\
 Data File : FF004454.D
 Signal(s) : FID2B.ch
 Acq On : 04 May 2019 02:15
 Operator : AJ\SJ
 Sample : PB119427BS
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 04 03:21:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050219.M
 Quant Title :
 QLast Update : Fri May 03 03:23:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.511	2502899	20.004 ug/ml
Target Compounds				
2)	N-DECANE	4.269	2626084	21.868 ug/ml
3)	N-DODECANE	6.283	2757693	21.936 ug/ml
4)	N-TETRADECANE	8.071	2762386	21.879 ug/ml
5)	N-HEXADECANE	9.667	2867675	21.483 ug/ml
6)	N-OCTADECANE	11.106	2876767	21.057 ug/ml
7)	N-EICOSANE	12.414	2901234	20.597 ug/ml
8)	N-DOCOSANE	13.611	2869964	20.229 ug/ml
10)	N-TETRACOSANE	14.713	2844075	19.949 ug/ml
11)	N-HEXACOSANE	15.735	2786542	19.713 ug/ml
12)	N-OCTACOSANE	16.685	2743076	19.562 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050319\
Data File : FF004454.D
Signal(s) : FID2B.ch
Acq On : 04 May 2019 02:15
Operator : AJ\SJ
Sample : PB119427BS
Misc :
ALS Vial : 73 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 04 03:21:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050219.M
Quant Title :
QLast Update : Fri May 03 03:23:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

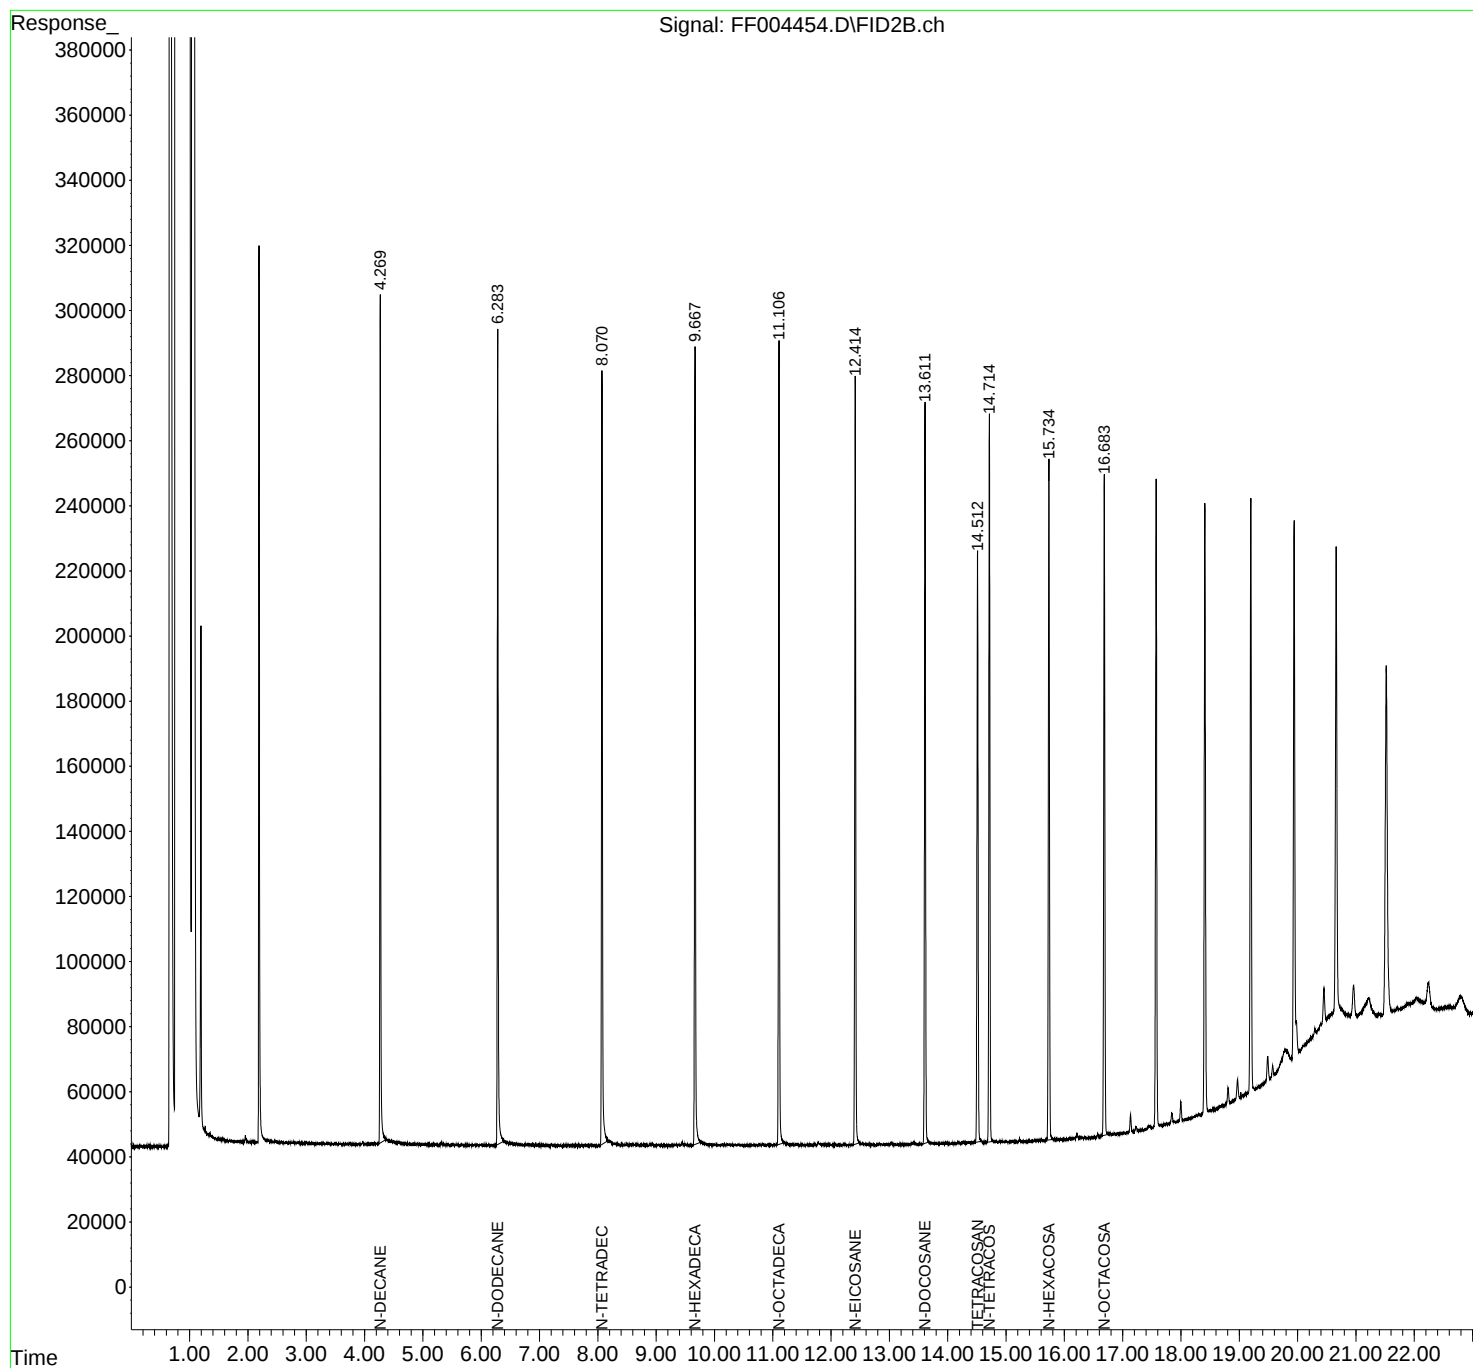

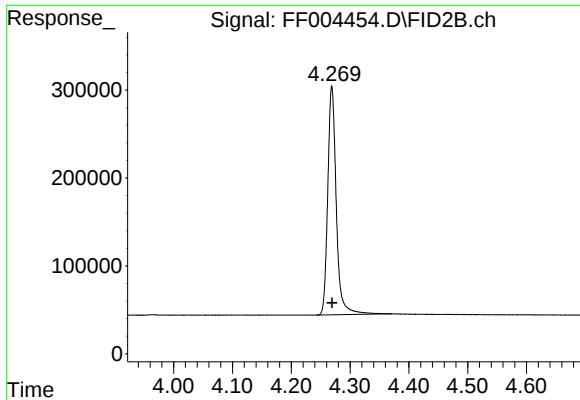


#2 N-DECANE

R.T.: 4.269 min
Delta R.T.: 0.000 min
Response: 2626084
Conc: 21.87 ug/ml

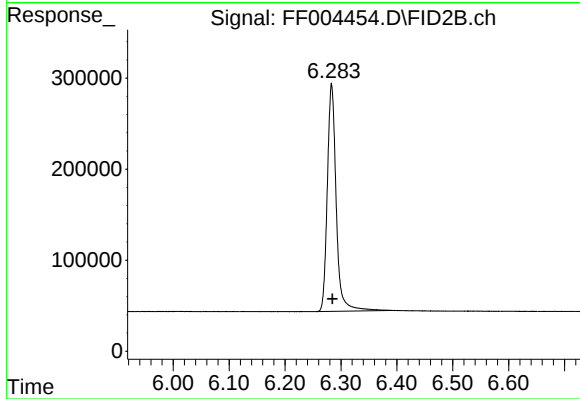


#3 N-DODECANE

R.T.: 6.283 min
Delta R.T.: -0.002 min
Response: 2757693
Conc: 21.94 ug/ml

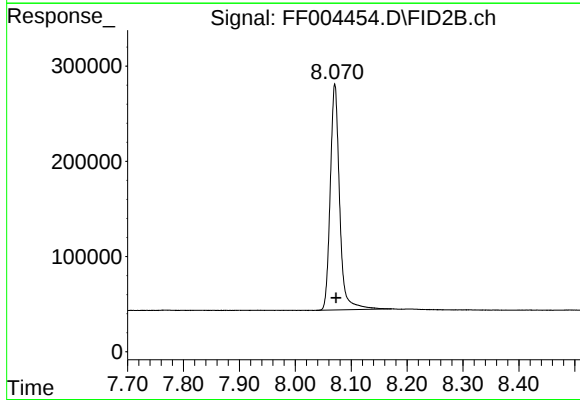


#4 N-TETRADECANE

R.T.: 8.071 min
Delta R.T.: -0.002 min
Response: 2762386
Conc: 21.88 ug/ml

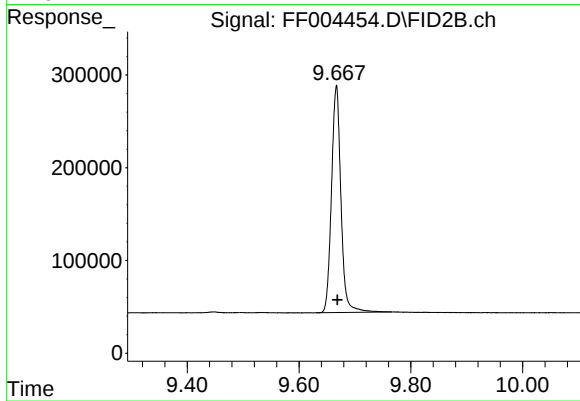


#5 N-HEXADECANE

R.T.: 9.667 min
Delta R.T.: -0.002 min
Response: 2867675
Conc: 21.48 ug/ml

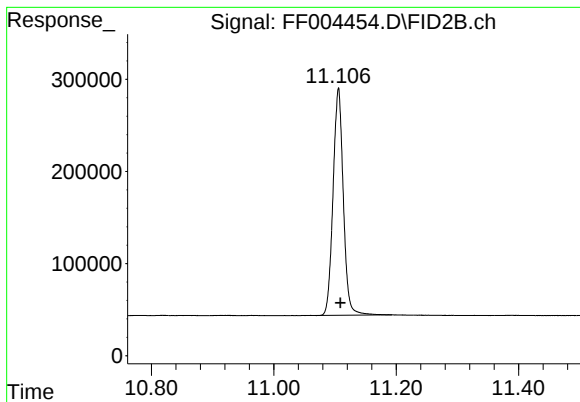


#6 N-OCTADECANE

R.T.: 11.106 min
Delta R.T.: -0.003 min
Response: 2876767
Conc: 21.06 ug/ml

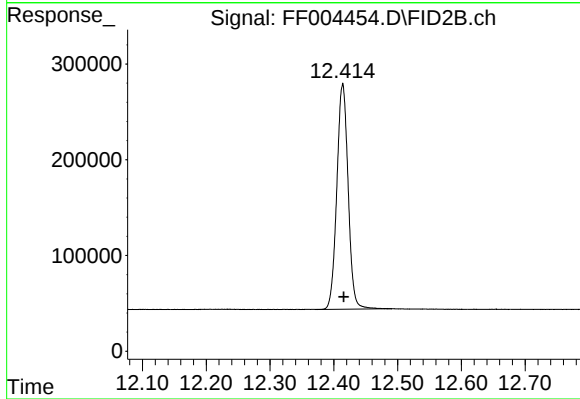


#7 N-EICOSANE

R.T.: 12.414 min
Delta R.T.: -0.001 min
Response: 2901234
Conc: 20.60 ug/ml

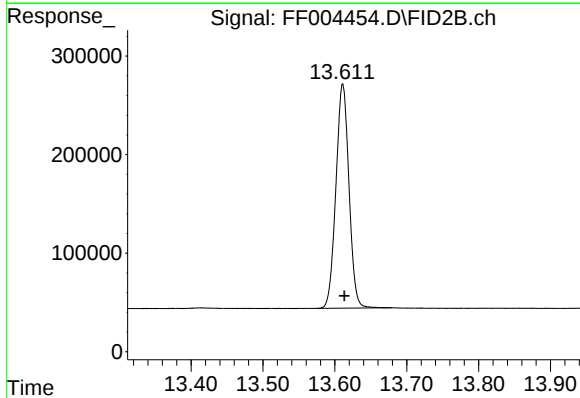


#8 N-DOCOSANE

R.T.: 13.611 min
Delta R.T.: -0.002 min
Response: 2869964
Conc: 20.23 ug/ml

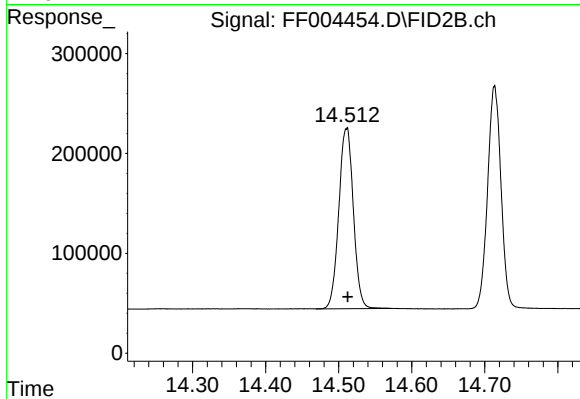


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.511 min
Delta R.T.: -0.002 min
Response: 2502899
Conc: 20.00 ug/ml

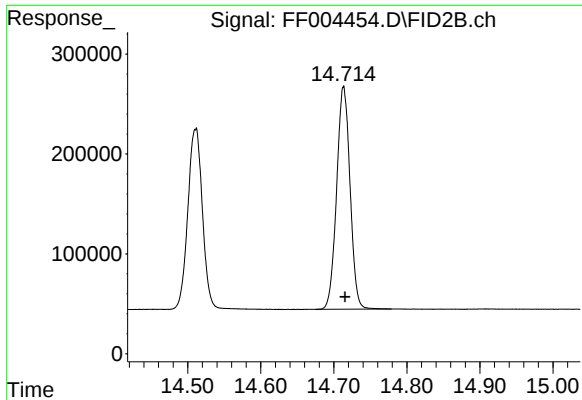


#10 N-TETRACOSANE

R.T.: 14.713 min
Delta R.T.: -0.002 min
Response: 2844075
Conc: 19.95 ug/ml

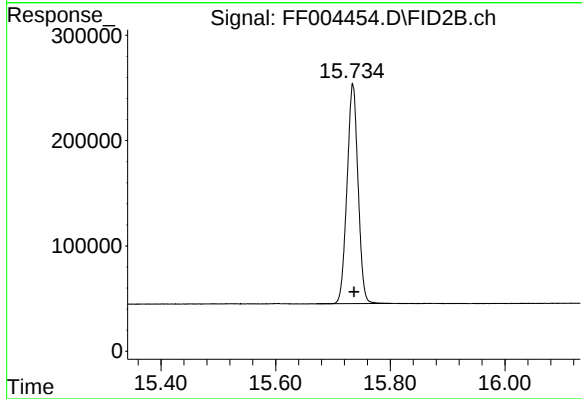

#11 N-HEXACOSANE

R.T.: 15.735 min
Delta R.T.: -0.002 min
Response: 2786542
Conc: 19.71 ug/ml

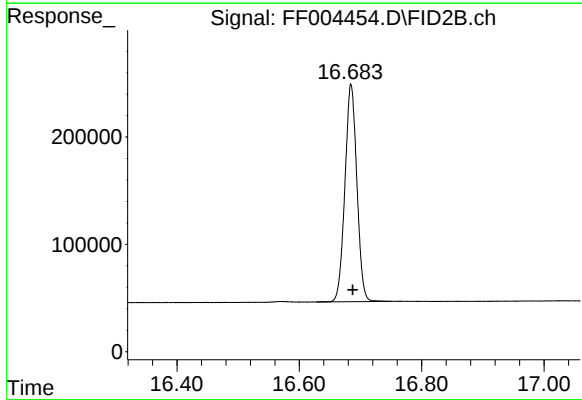

#12 N-OCTACOSANE

R.T.: 16.685 min
Delta R.T.: -0.003 min
Response: 2743076
Conc: 19.56 ug/ml