

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050322AL\
 Data File : FF010491.D
 Signal(s) : FID2B.ch
 Acq On : 03 May 2022 19:57
 Operator : AJ\MA
 Sample : N2618-09
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 04 01:44:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH -FF050322.M
 Quant Title : GC Extractables
 QLast Update : Tue May 03 13:18:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.292	5434991	49.976 ug/ml
Spiked Amount 50.000		Recovery =	99.95%
Target Compounds			
2) T n-Decane (C10)	3.723	16452	0.140 ug/ml
4) T n-Dodecane (C12)	5.707	161390	1.344 ug/ml
6) T n-Tetradecane (C14)	7.497	47162	0.391 ug/ml
14) T n-Tetracosane (C24)	14.143	41765	0.339 ug/ml
15) T n-Hexacosane (C26)	15.163	80171	0.674 ug/ml
16) T n-Octacosane (C28)	16.110	84216	0.738 ug/ml
17) T n-Tricontane (C30)	16.997	79370	0.728 ug/ml
18) T n-Dotriacontane (C32)	17.828	64423	0.629 ug/ml
19) T n-Tetratriacontane (C34)	18.609	33861	0.367 ug/ml
20) T n-Hexatriacontane (C36)	19.348	19675	0.236 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050322AL\
Data File : FF010491.D
Signal(s) : FID2B.ch
Acq On : 03 May 2022 19:57
Operator : AJ\MA
Sample : N2618-09
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 04 01:44:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH -FF050322.M
Quant Title : GC Extractables
QLast Update : Tue May 03 13:18:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

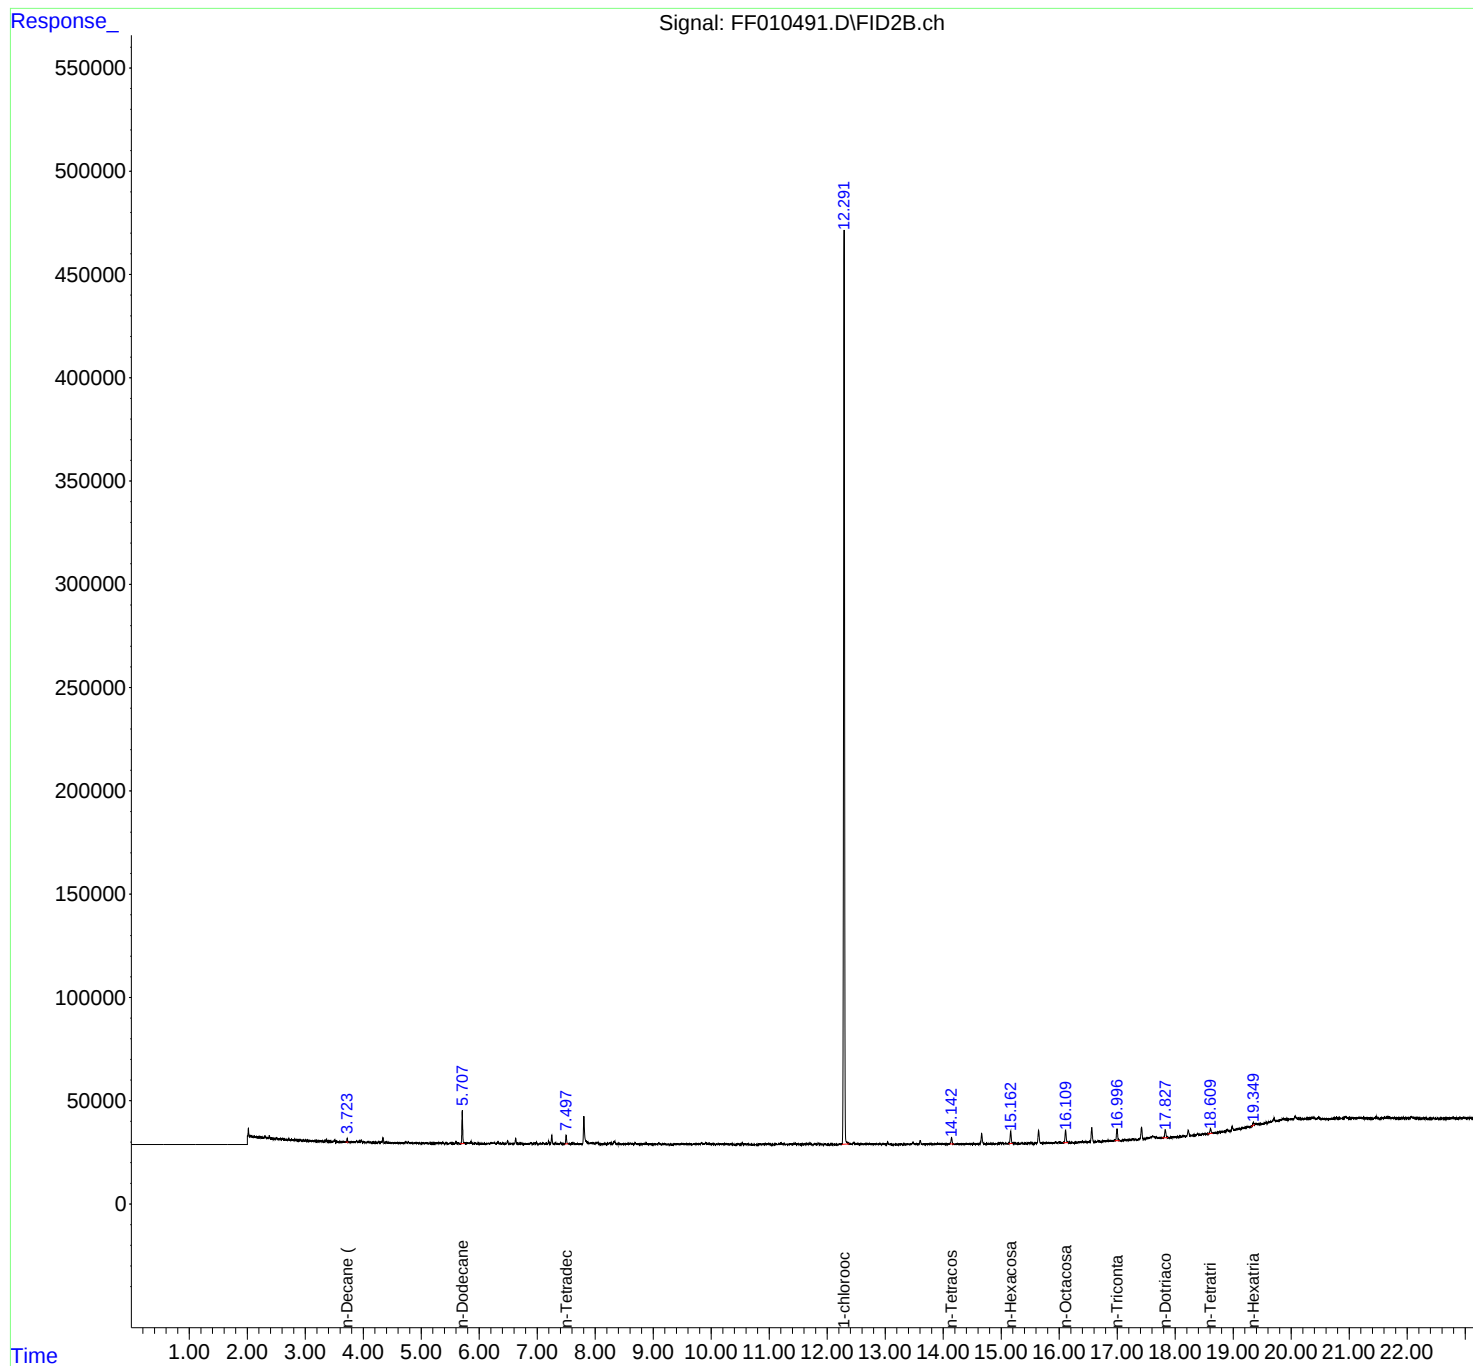


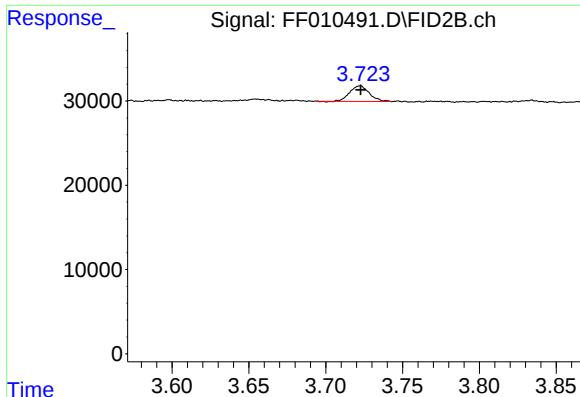

#2 n-Decane (C10)


R.T.: 3.723 min
Delta R.T.: 0.000 min
Response: 16452
Conc: 0.14 ug/ml

Instrument :
FID_F
ClientSampleId :

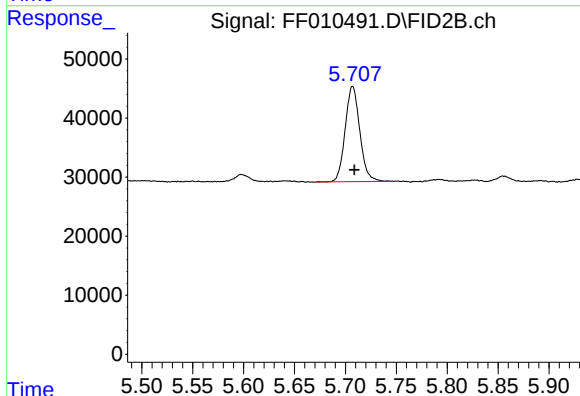


#4 n-Dodecane (C12)

R.T.: 5.707 min
Delta R.T.: -0.002 min
Response: 161390
Conc: 1.34 ug/ml

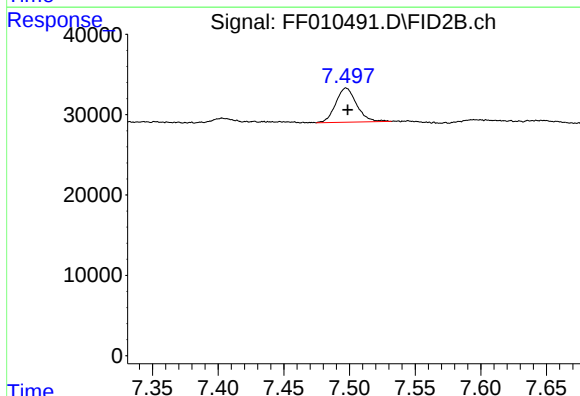


#6 n-Tetradecane (C14)

R.T.: 7.497 min
Delta R.T.: -0.001 min
Response: 47162
Conc: 0.39 ug/ml

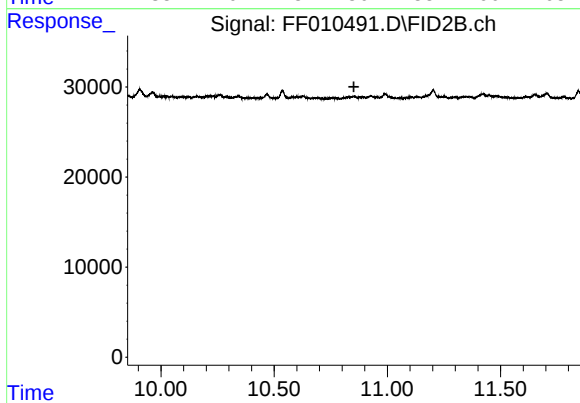

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 10.852 min
Response: 0
Conc: N.D.

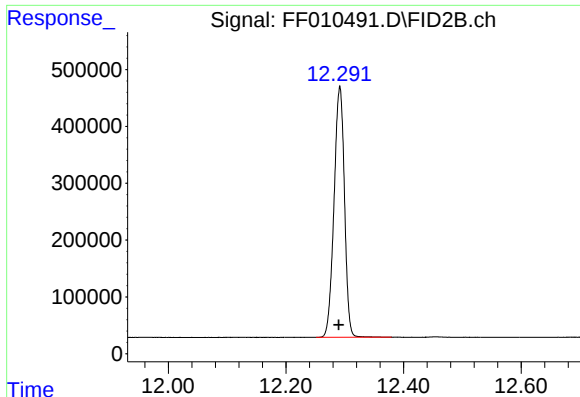

#12 1-chlorooctadecane (SURR)


R.T.: 12.292 min
Delta R.T.: 0.002 min
Response: 5434991
Conc: 49.98 ug/ml

Instrument :
FID_F
ClientSampleId :

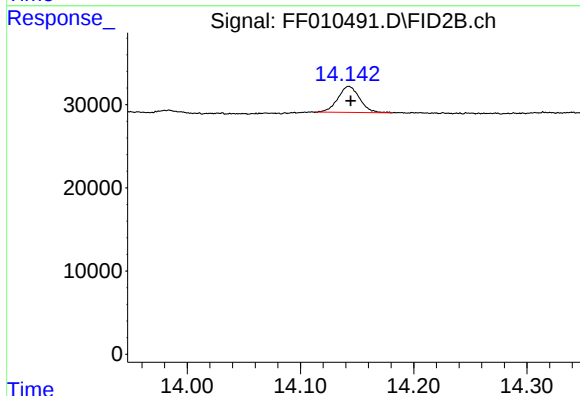


#14 n-Tetracosane (C24)

R.T.: 14.143 min
Delta R.T.: -0.002 min
Response: 41765
Conc: 0.34 ug/ml

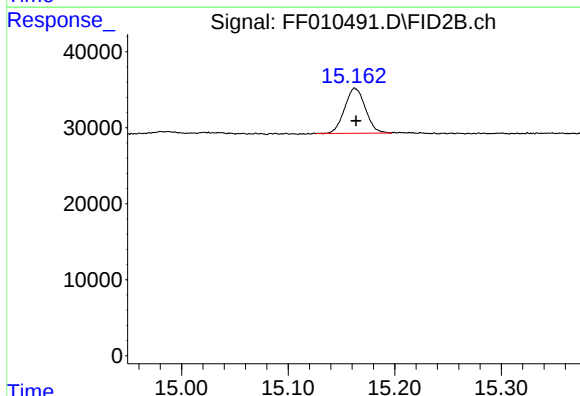


#15 n-Hexacosane (C26)

R.T.: 15.163 min
Delta R.T.: -0.001 min
Response: 80171
Conc: 0.67 ug/ml

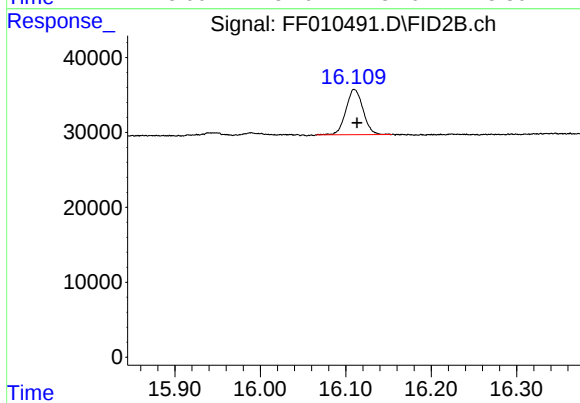

#16 n-Octacosane (C28)


R.T.: 16.110 min
Delta R.T.: -0.003 min
Response: 84216
Conc: 0.74 ug/ml

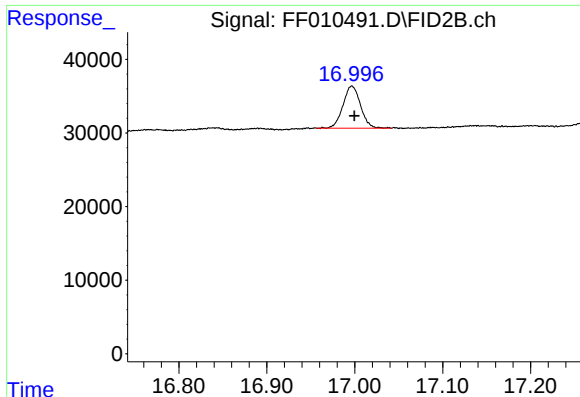

#17 n-Tricontane (C30)


R.T.: 16.997 min
Delta R.T.: -0.003 min
Response: 79370
Conc: 0.73 ug/ml

Instrument :
FID_F
ClientSampleId :

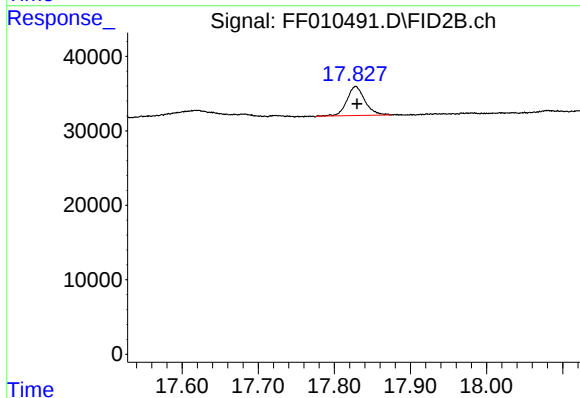


#18 n-Dotriacontane (C32)

R.T.: 17.828 min
Delta R.T.: -0.002 min
Response: 64423
Conc: 0.63 ug/ml

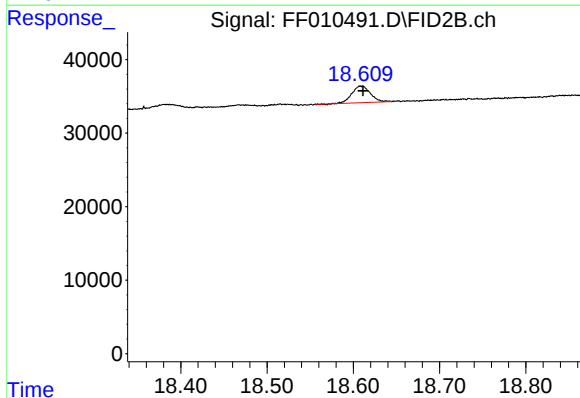

#19 n-Tetratriacontane (C34)

R.T.: 18.609 min
Delta R.T.: -0.002 min
Response: 33861
Conc: 0.37 ug/ml

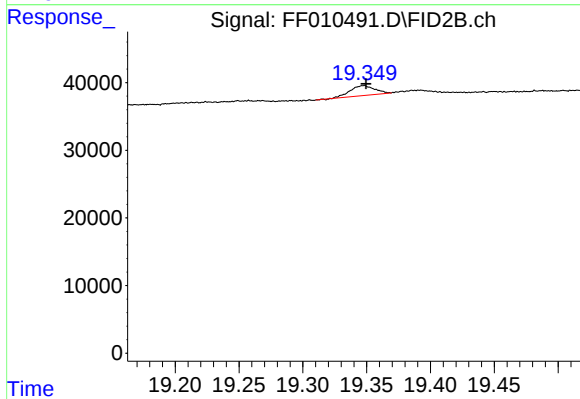

#20 n-Hexatriacontane (C36)

R.T.: 19.348 min
Delta R.T.: -0.002 min
Response: 19675
Conc: 0.24 ug/ml