

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050322AL\
 Data File : FF010497.D
 Signal(s) : FID2B.ch
 Acq On : 03 May 2022 22:50
 Operator : AJ\MA
 Sample : N2637-05
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 04 01:45:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH -FF050322.M
 Quant Title : GC Extractables
 QLast Update : Tue May 03 13:18:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.291	3286764	30.222 ug/ml
Spiked Amount 50.000		Recovery =	60.44%
Target Compounds			
4) T n-Dodecane (C12)	5.708	139331	1.160 ug/ml
6) T n-Tetradecane (C14)	7.498	34791	0.288 ug/ml
13) T n-Docosane (C22)	13.041	43440	0.347 ug/ml
14) T n-Tetracosane (C24)	14.143	109858	0.892 ug/ml
15) T n-Hexacosane (C26)	15.163	274033	2.303 ug/ml
16) T n-Octacosane (C28)	16.112	458161	4.014 ug/ml
17) T n-Tricontane (C30)	16.998	441537	4.049 ug/ml
18) T n-Dotriacontane (C32)	17.829	285502	2.786 ug/ml
19) T n-Tetratriacontane (C34)	18.609	149268	1.617 ug/ml
20) T n-Hexatriacontane (C36)	19.347	123461	1.480 ug/ml
21) T n-Octatriacontane (C38)	20.069	79723	1.071 ug/ml
22) T n-Tetracontane (C40)	20.941	122604	1.640 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050322AL\
Data File : FF010497.D
Signal(s) : FID2B.ch
Acq On : 03 May 2022 22:50
Operator : AJ\MA
Sample : N2637-05
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 04 01:45:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH -FF050322.M
Quant Title : GC Extractables
QLast Update : Tue May 03 13:18:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

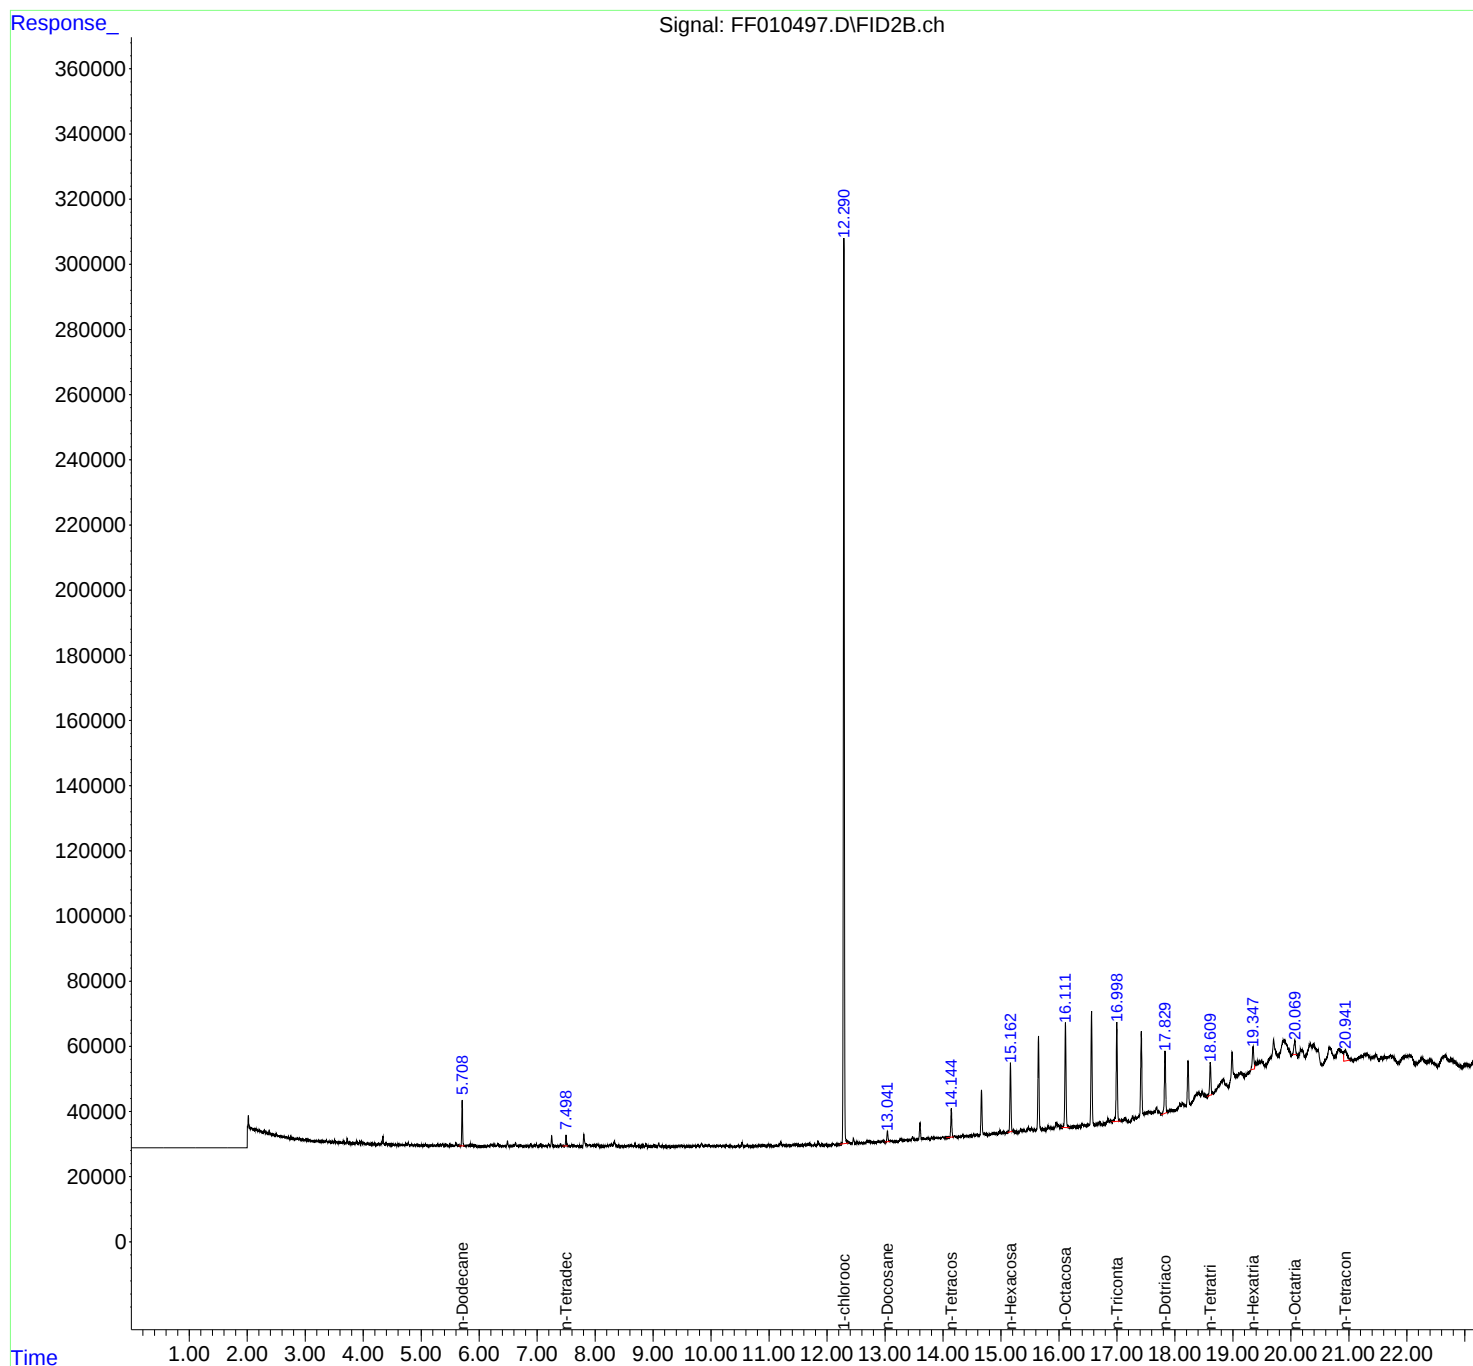


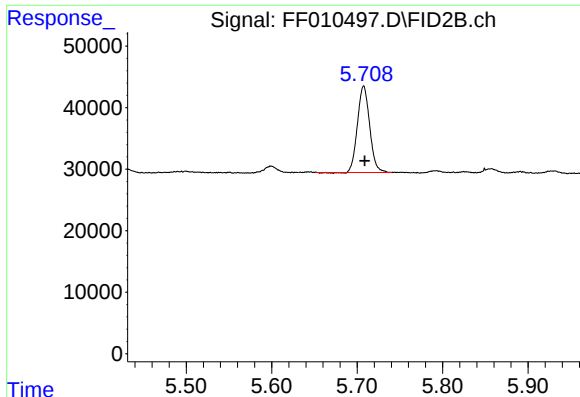

#4 n-Dodecane (C12)


R.T.: 5.708 min
Delta R.T.: -0.001 min
Response: 139331
Conc: 1.16 ug/ml

Instrument :
FID_F
ClientSampleId :

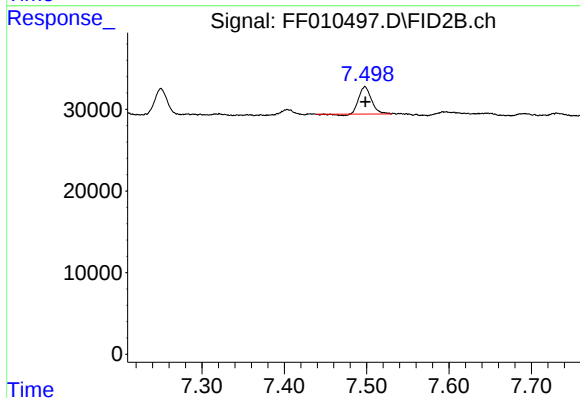


#6 n-Tetradecane (C14)

R.T.: 7.498 min
Delta R.T.: 0.000 min
Response: 34791
Conc: 0.29 ug/ml

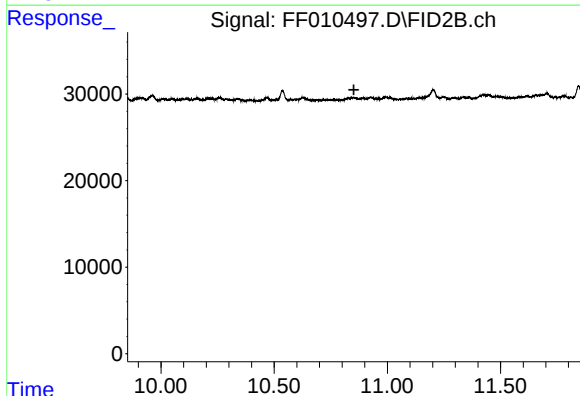


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 10.852 min
Response: 0
Conc: N.D.

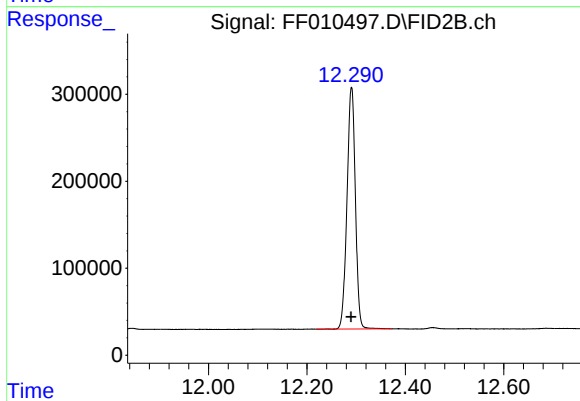

#12 1-chlorooctadecane (SURR)


R.T.: 12.291 min
Delta R.T.: 0.000 min
Response: 3286764
Conc: 30.22 ug/ml

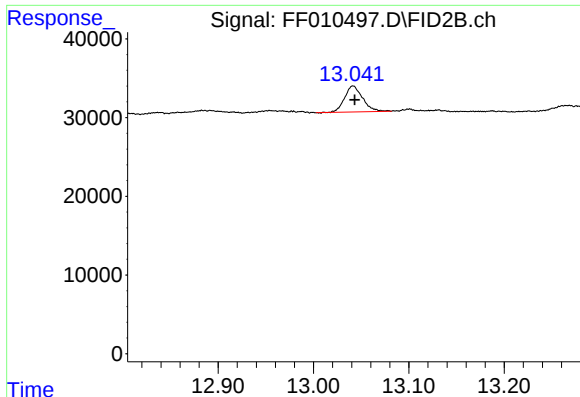

#13 n-Docosane (C22)


R.T.: 13.041 min
Delta R.T.: -0.002 min
Response: 43440
Conc: 0.35 ug/ml

Instrument :
FID_F
ClientSampleId :

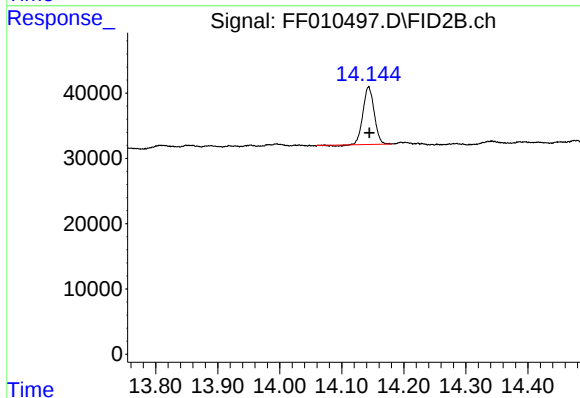


#14 n-Tetracosane (C24)

R.T.: 14.143 min
Delta R.T.: -0.001 min
Response: 109858
Conc: 0.89 ug/ml

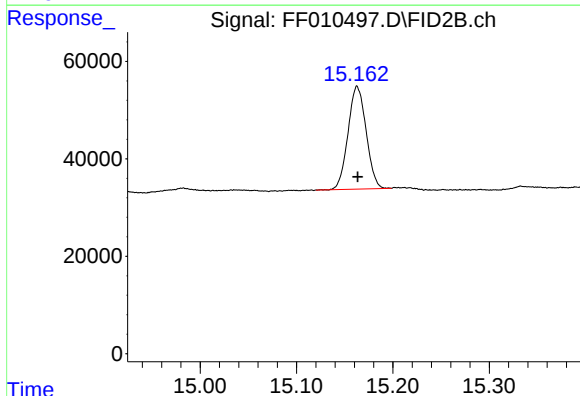


#15 n-Hexacosane (C26)

R.T.: 15.163 min
Delta R.T.: 0.000 min
Response: 274033
Conc: 2.30 ug/ml

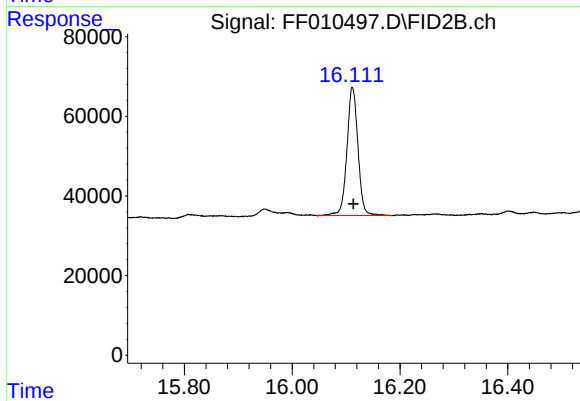

#16 n-Octacosane (C28)


R.T.: 16.112 min
Delta R.T.: -0.002 min
Response: 458161
Conc: 4.01 ug/ml

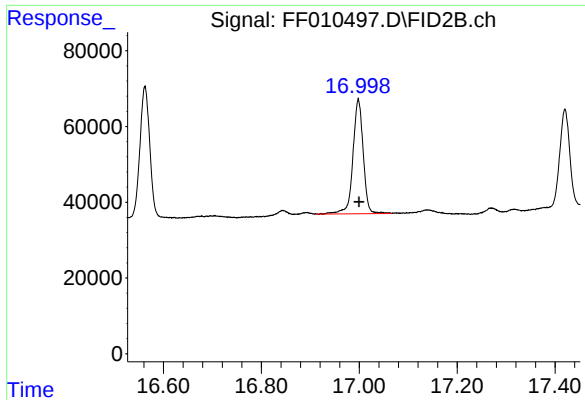

#17 n-Tricontane (C30)


R.T.: 16.998 min
Delta R.T.: -0.001 min
Response: 441537
Conc: 4.05 ug/ml

Instrument :
FID_F
ClientSampleId :

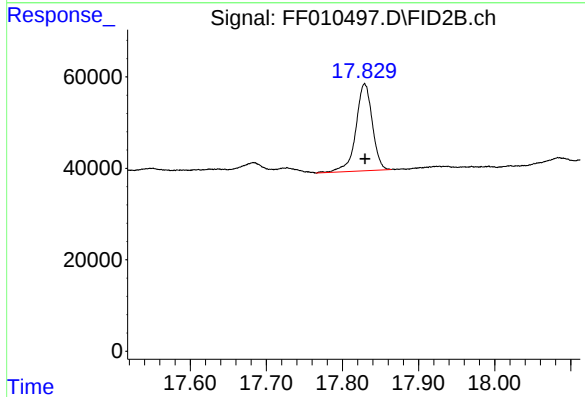


#18 n-Dotriacontane (C32)

R.T.: 17.829 min
Delta R.T.: 0.000 min
Response: 285502
Conc: 2.79 ug/ml

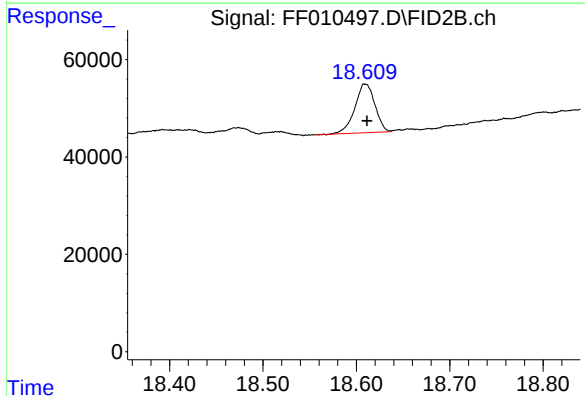


#19 n-Tetratriacontane (C34)

R.T.: 18.609 min
Delta R.T.: -0.002 min
Response: 149268
Conc: 1.62 ug/ml

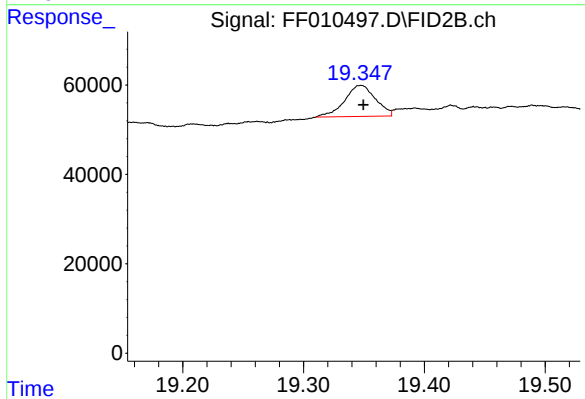

#20 n-Hexatriacontane (C36)


R.T.: 19.347 min
Delta R.T.: -0.002 min
Response: 123461
Conc: 1.48 ug/ml

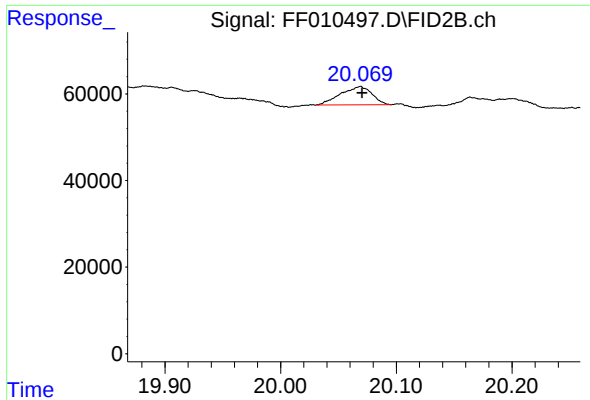

#21 n-Octatriacontane (C38)

R.T.: 20.069 min
Delta R.T.: -0.002 min
Response: 79723
Conc: 1.07 ug/ml

Instrument :
FID_F
ClientSampleId :

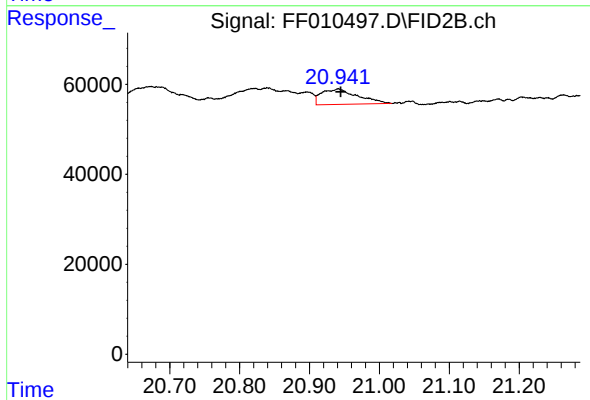

#22 n-Tetracontane (C40)

R.T.: 20.941 min
Delta R.T.: -0.004 min
Response: 122604
Conc: 1.64 ug/ml