

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050323\
 Data File : FF012568.D
 Signal(s) : FID2B.ch
 Acq On : 03 May 2023 07:53
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 04 01:22:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
 Quant Title :
 QLast Update : Thu Apr 13 15:26:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.875	90945	0.660 ug/ml
8) N-DOCOSANE	14.095	109358	0.812 ug/ml
10) N-TETRACOSANE	15.183	250096	1.849 ug/ml
11) N-HEXACOSANE	16.222	64841	0.487 ug/ml
12) N-OCTACOSANE	17.171	66580	0.505 ug/ml
13) N-TRIACONTANE	18.059	80647	0.618 ug/ml
14) N-DOTRIACONTANE	18.894	123673	0.980 ug/ml
16) N-HEXATRIACONTANE	20.453	72005	0.705 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050323\
Data File : FF012568.D
Signal(s) : FID2B.ch
Acq On : 03 May 2023 07:53
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 04 01:22:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

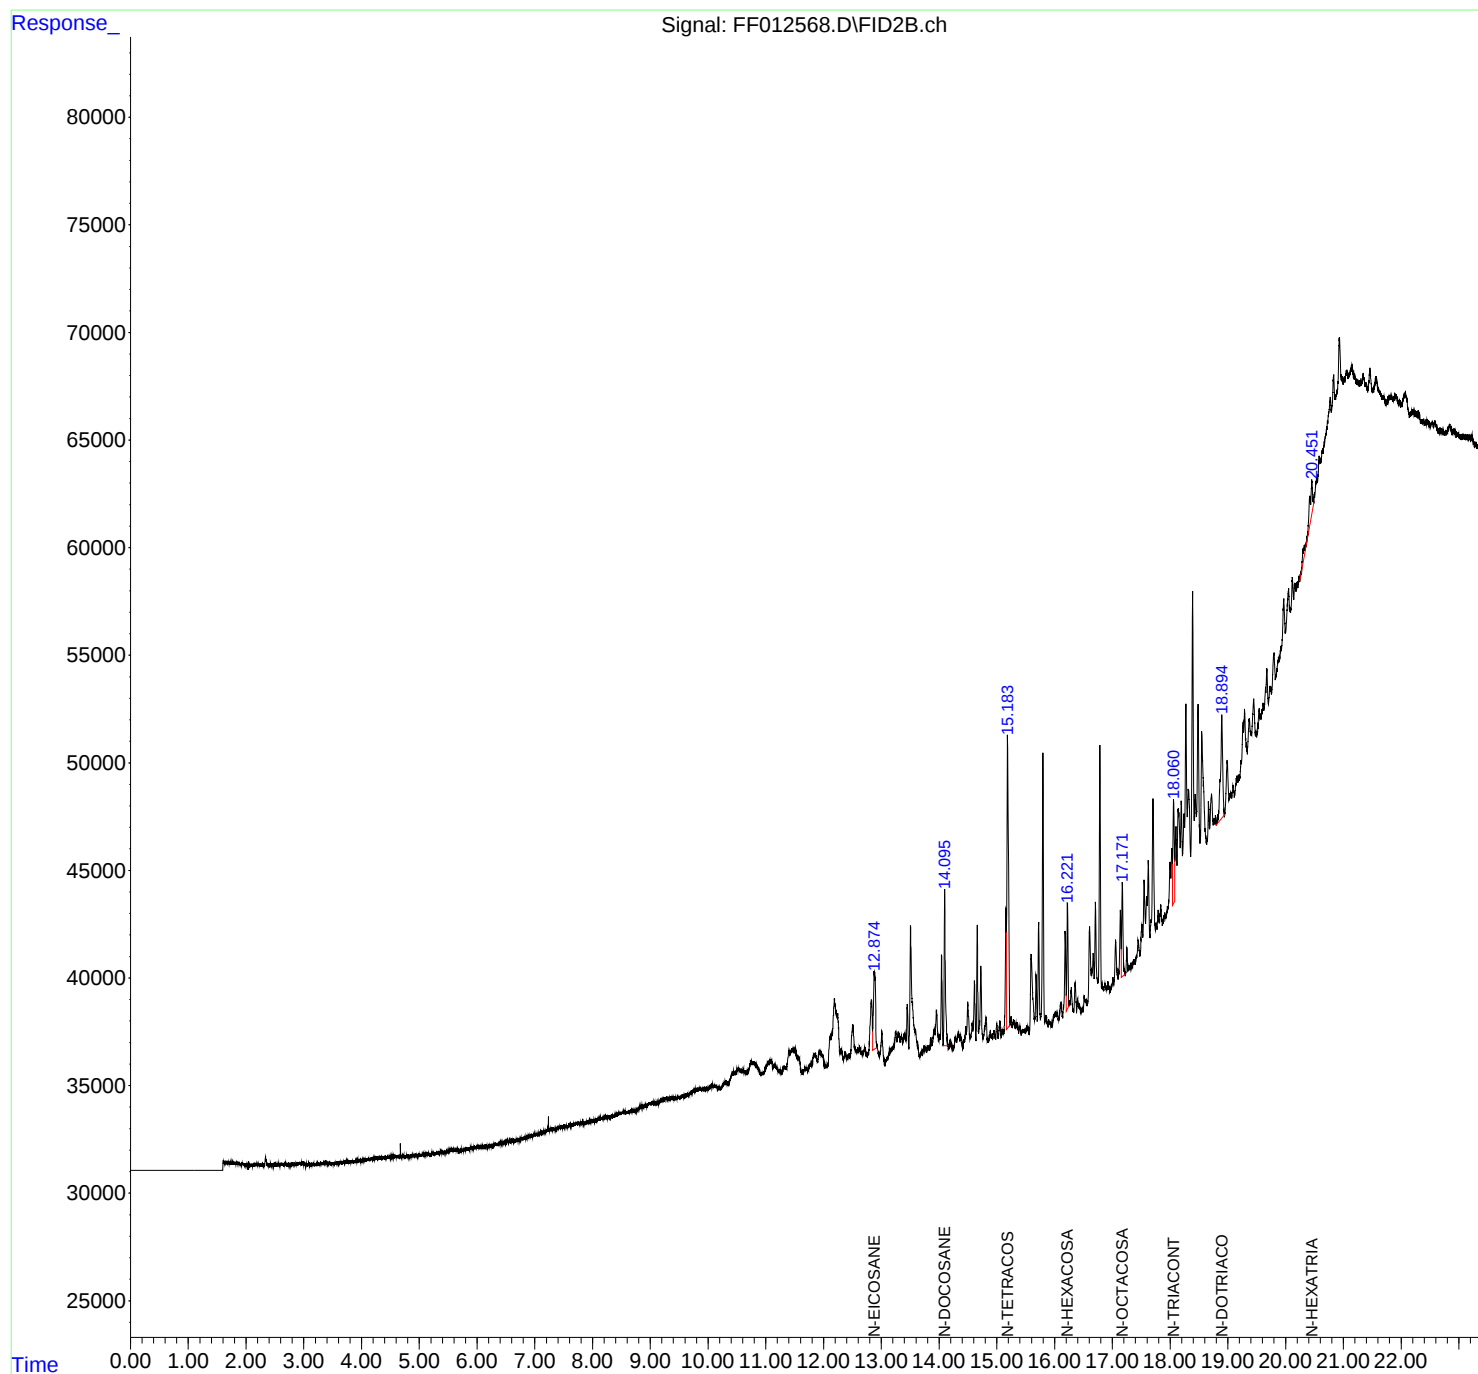


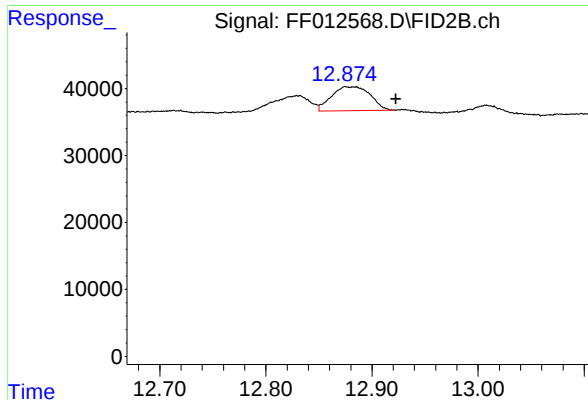

#7 N-EICOSANE


R.T.: 12.875 min
Delta R.T.: -0.047 min
Response: 90945
Conc: 0.66 ug/ml

Instrument :
FID_F
ClientSampleId :

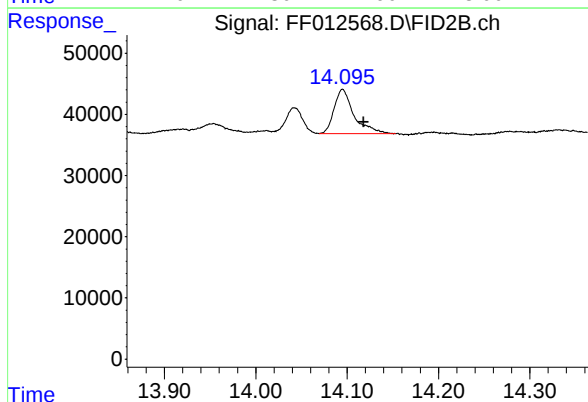


#8 N-DOCOSANE

R.T.: 14.095 min
Delta R.T.: -0.023 min
Response: 109358
Conc: 0.81 ug/ml

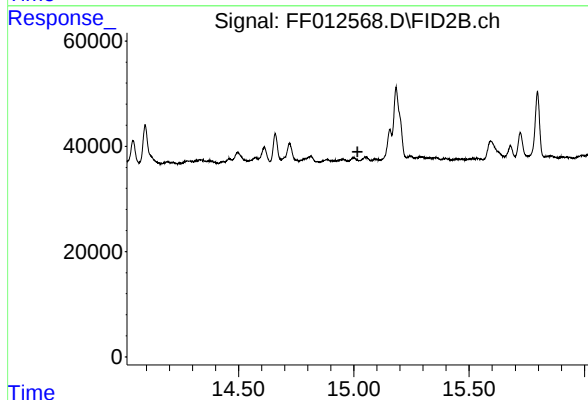


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.016 min
Response: 0
Conc: N.D.

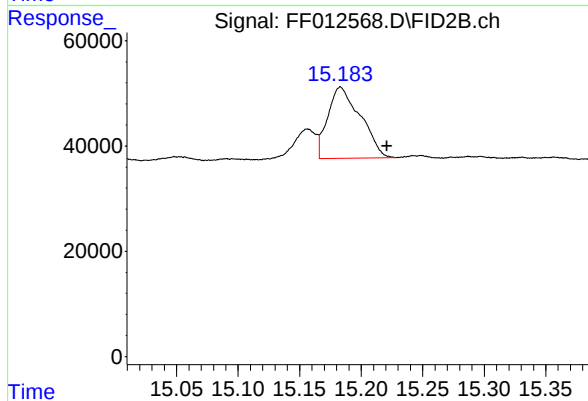

#10 N-TETRACOSANE


R.T.: 15.183 min
Delta R.T.: -0.038 min
Response: 250096
Conc: 1.85 ug/ml

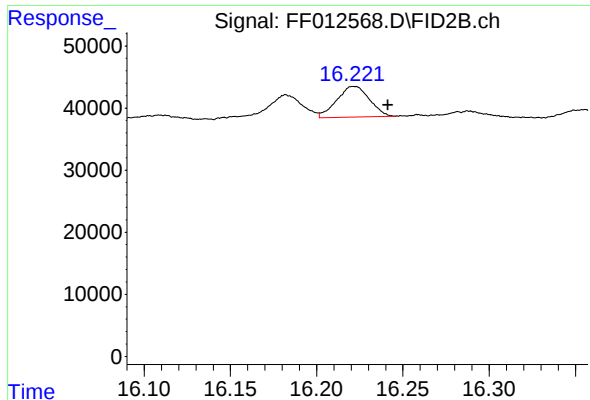

#11 N-HEXACOSANE


R.T.: 16.222 min
Delta R.T.: -0.020 min
Response: 64841
Conc: 0.49 ug/ml

Instrument :
FID_F
ClientSampleId :

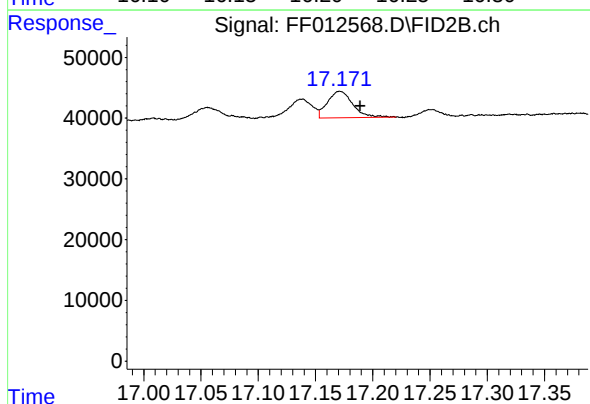


#12 N-OCTACOSANE

R.T.: 17.171 min
Delta R.T.: -0.018 min
Response: 66580
Conc: 0.50 ug/ml

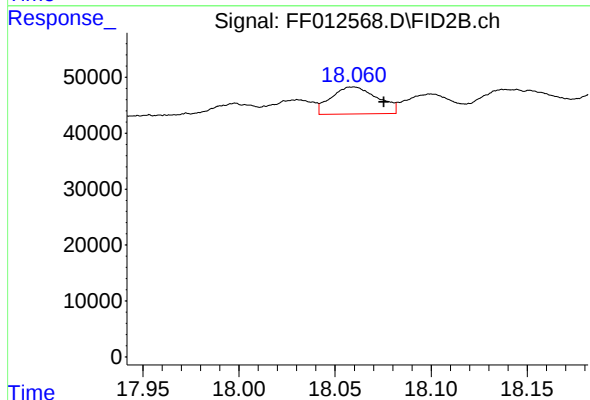


#13 N-TRIACONTANE

R.T.: 18.059 min
Delta R.T.: -0.016 min
Response: 80647
Conc: 0.62 ug/ml

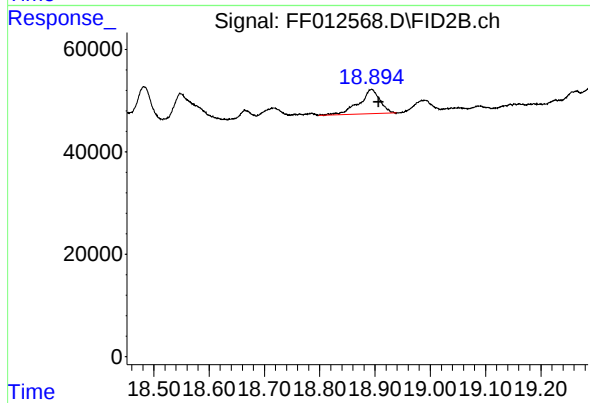

#14 N-DOTRIACONTANE

R.T.: 18.894 min
Delta R.T.: -0.013 min
Response: 123673
Conc: 0.98 ug/ml

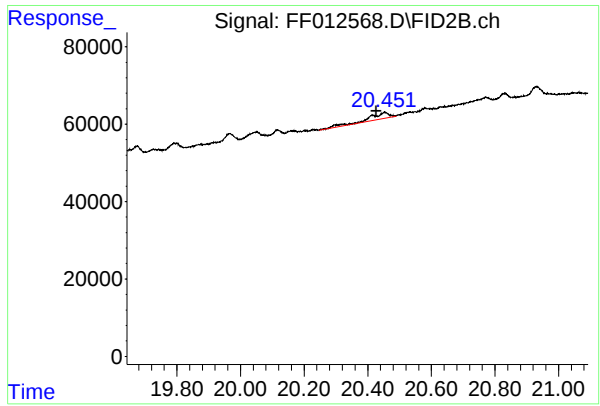

#16 N-HEXATRIACONTANE

R.T.: 20.453 min
Delta R.T.: 0.026 min
Response: 72005
Conc: 0.71 ug/ml

Instrument :
FID_F
ClientSampleId :