

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050323\
 Data File : FF012571.D
 Signal(s) : FID2B.ch
 Acq On : 03 May 2023 09:20
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 04 01:22:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
 Quant Title :
 QLast Update : Thu Apr 13 15:26:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.729	2355424	19.071 ug/ml
12) N-OCTACOSANE	17.175	2350889	17.825 ug/ml
13) N-TRIACONTANE	18.062	48284	0.370 ug/ml
14) N-DOTRIACONTANE	18.892	64748	0.513 ug/ml
15) N-TETRATRIACONTANE	19.674	51679	0.456 ug/ml
16) N-HEXATRIACONTANE	20.419	80442	0.788 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050323\
Data File : FF012571.D
Signal(s) : FID2B.ch
Acq On : 03 May 2023 09:20
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 04 01:22:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

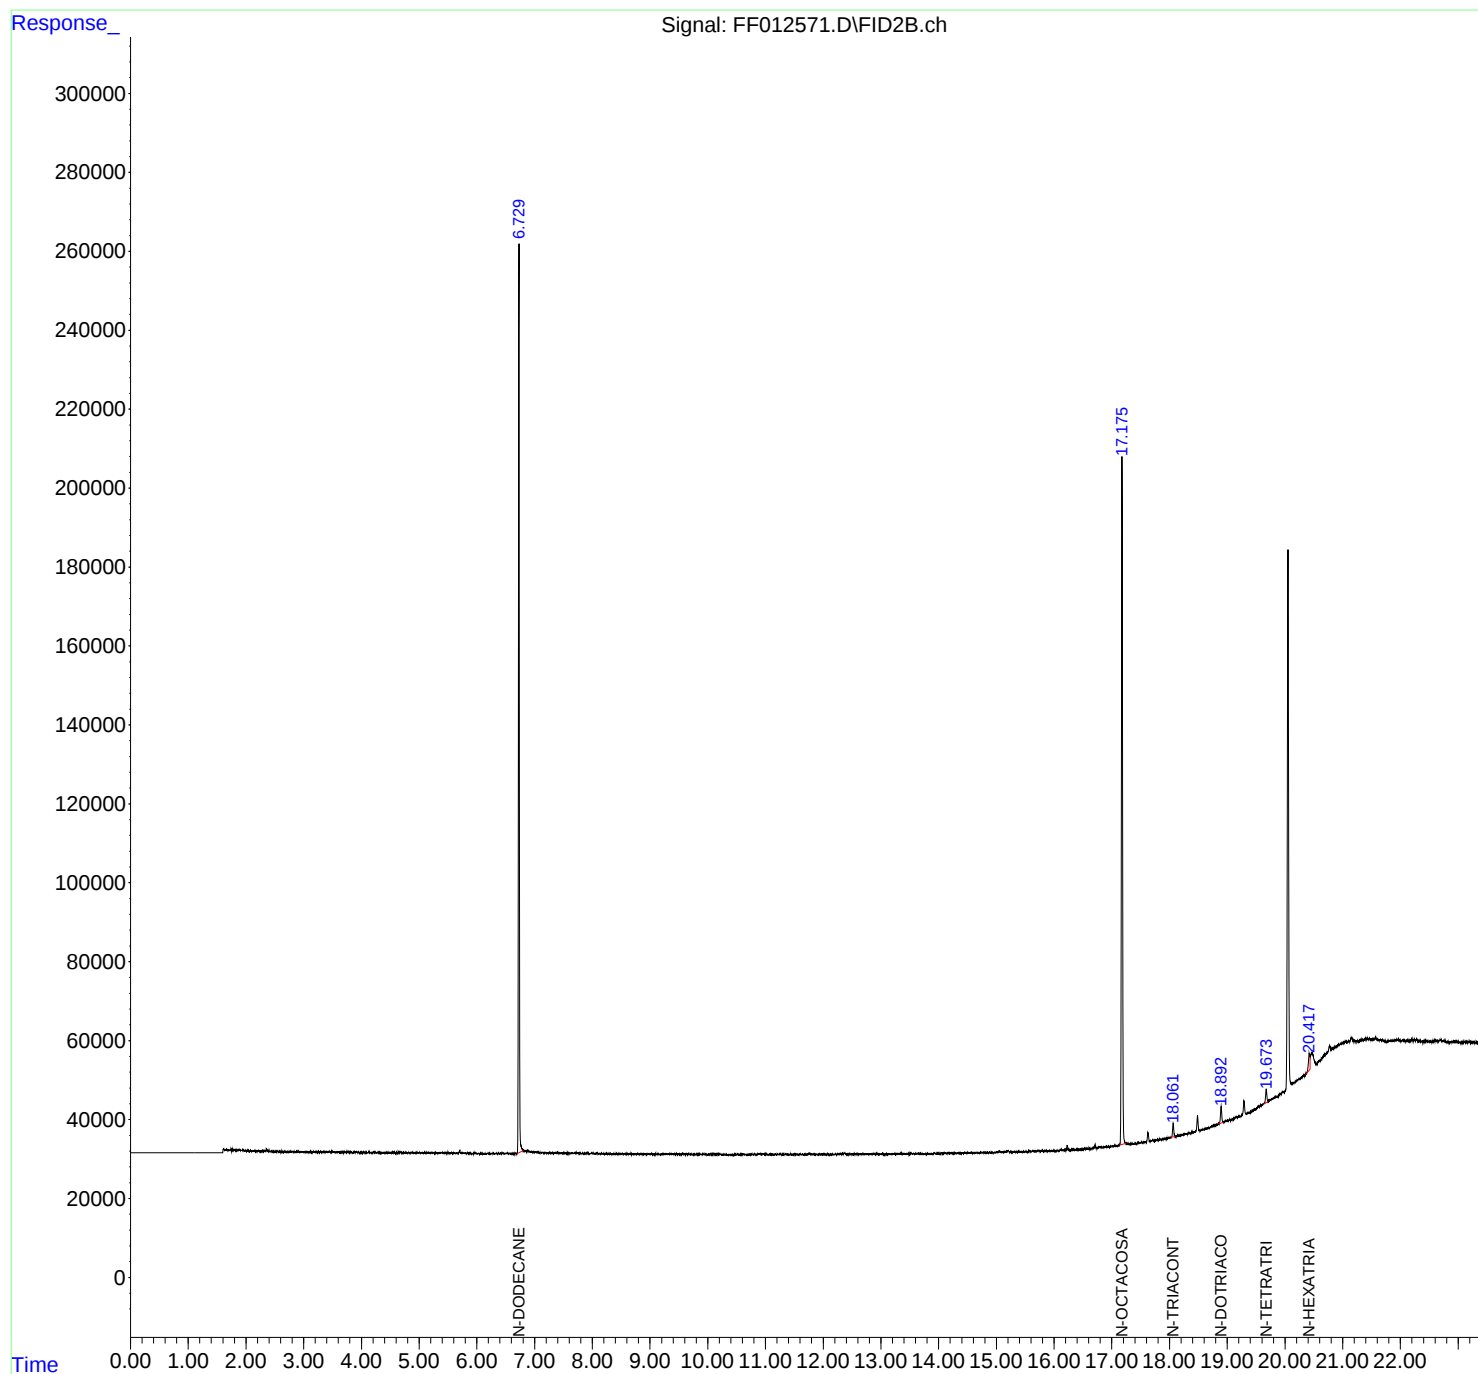


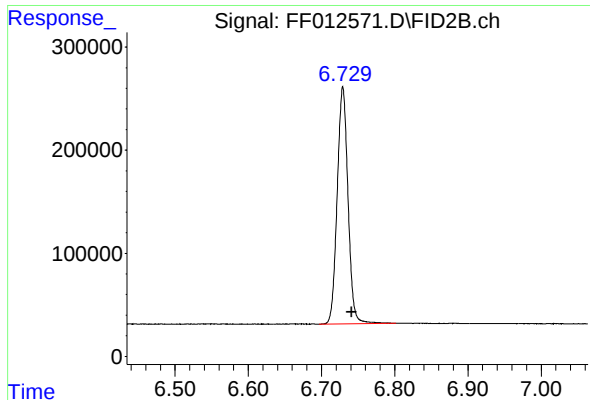

#3 N-DODECANE


R.T.: 6.729 min
Delta R.T.: -0.012 min
Response: 2355424
Conc: 19.07 ug/ml

Instrument :
FID_F
ClientSampleId :

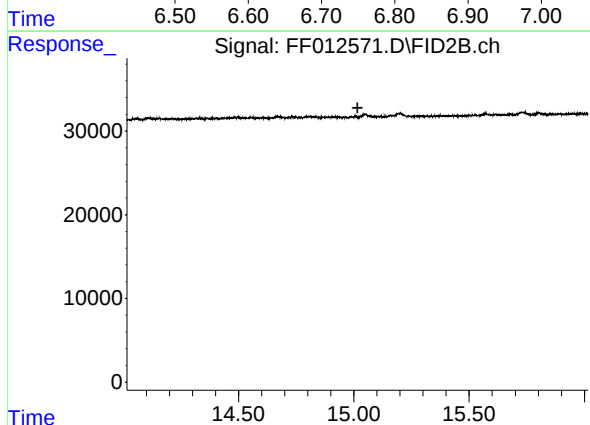


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.016 min
Response: 0
Conc: N.D.

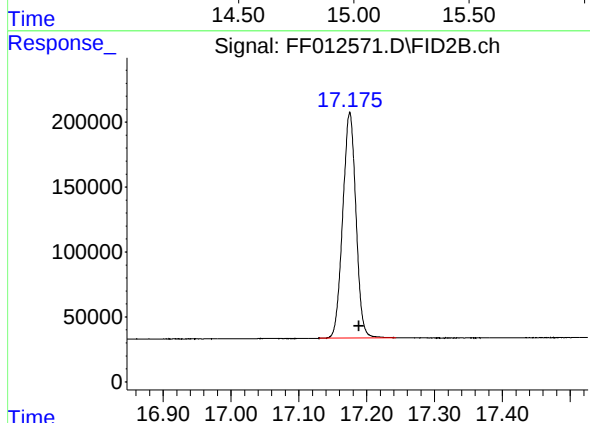


#12 N-OCTACOSANE

R.T.: 17.175 min
Delta R.T.: -0.014 min
Response: 2350889
Conc: 17.82 ug/ml

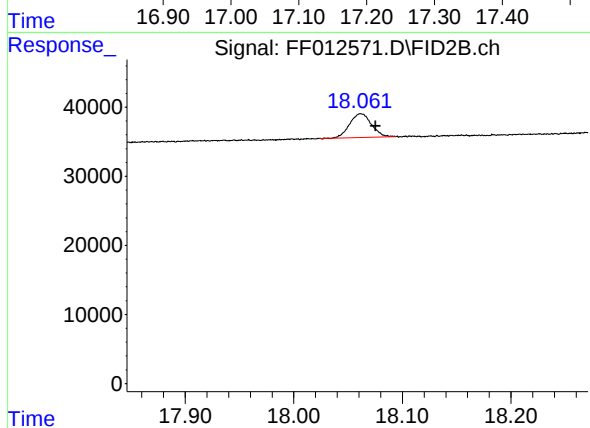

#13 N-TRIACONTANE


R.T.: 18.062 min
Delta R.T.: -0.014 min
Response: 48284
Conc: 0.37 ug/ml

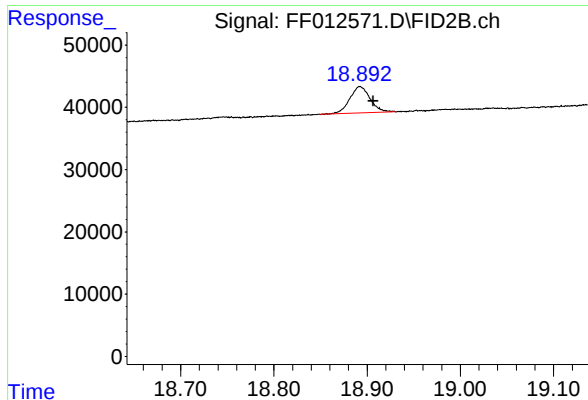

#14 N-DOTRIACONTANE


R.T.: 18.892 min
Delta R.T.: -0.015 min
Response: 64748
Conc: 0.51 ug/ml

Instrument :
FID_F
ClientSampleId :

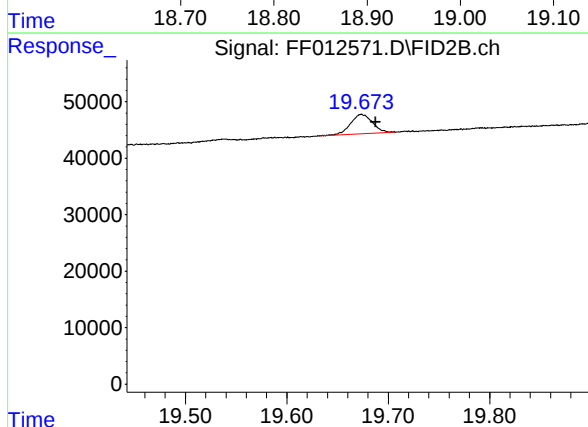

#15 N-TETRATRIACONTANE

R.T.: 19.674 min
Delta R.T.: -0.014 min
Response: 51679
Conc: 0.46 ug/ml

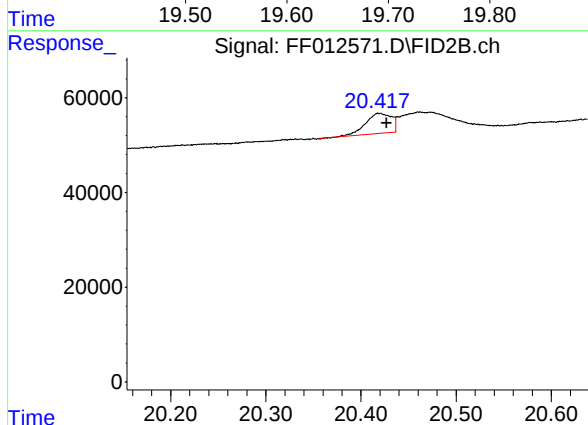

#16 N-HEXATRIACONTANE

R.T.: 20.419 min
Delta R.T.: -0.008 min
Response: 80442
Conc: 0.79 ug/ml